

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121521\
 Data File : FF009449.D
 Signal(s) : FID2B.ch
 Acq On : 16 Dec 2021 00:00
 Operator : AJ\MA
 Sample : M5074-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 03:42:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.480	1471062	12.699 ug/ml
Target Compounds			
4) N-TETRADECANE	8.055	77986	0.536 ug/ml
7) N-EICOSANE	12.389	50619	0.357 ug/ml
10) N-TETRACOSANE	14.658	200330	1.521 ug/ml
11) N-HEXACOSANE	15.761f	40266	0.322 ug/ml
12) N-OCTACOSANE	16.656	68635	0.576 ug/ml
13) N-TRIACONTANE	17.524	157814	1.378 ug/ml
14) N-DOTRIACONTANE	18.359	72829	0.666 ug/ml
15) N-TETRATRIACONTANE	19.136	27102	0.256 ug/ml
16) N-HEXATRIACONTANE	19.876	12887	0.129 ug/ml
17) N-OCTATRIACONTANE	20.583	13893	0.141 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121521\
Data File : FF009449.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 00:00
Operator : AJ\MA
Sample : M5074-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 03:42:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

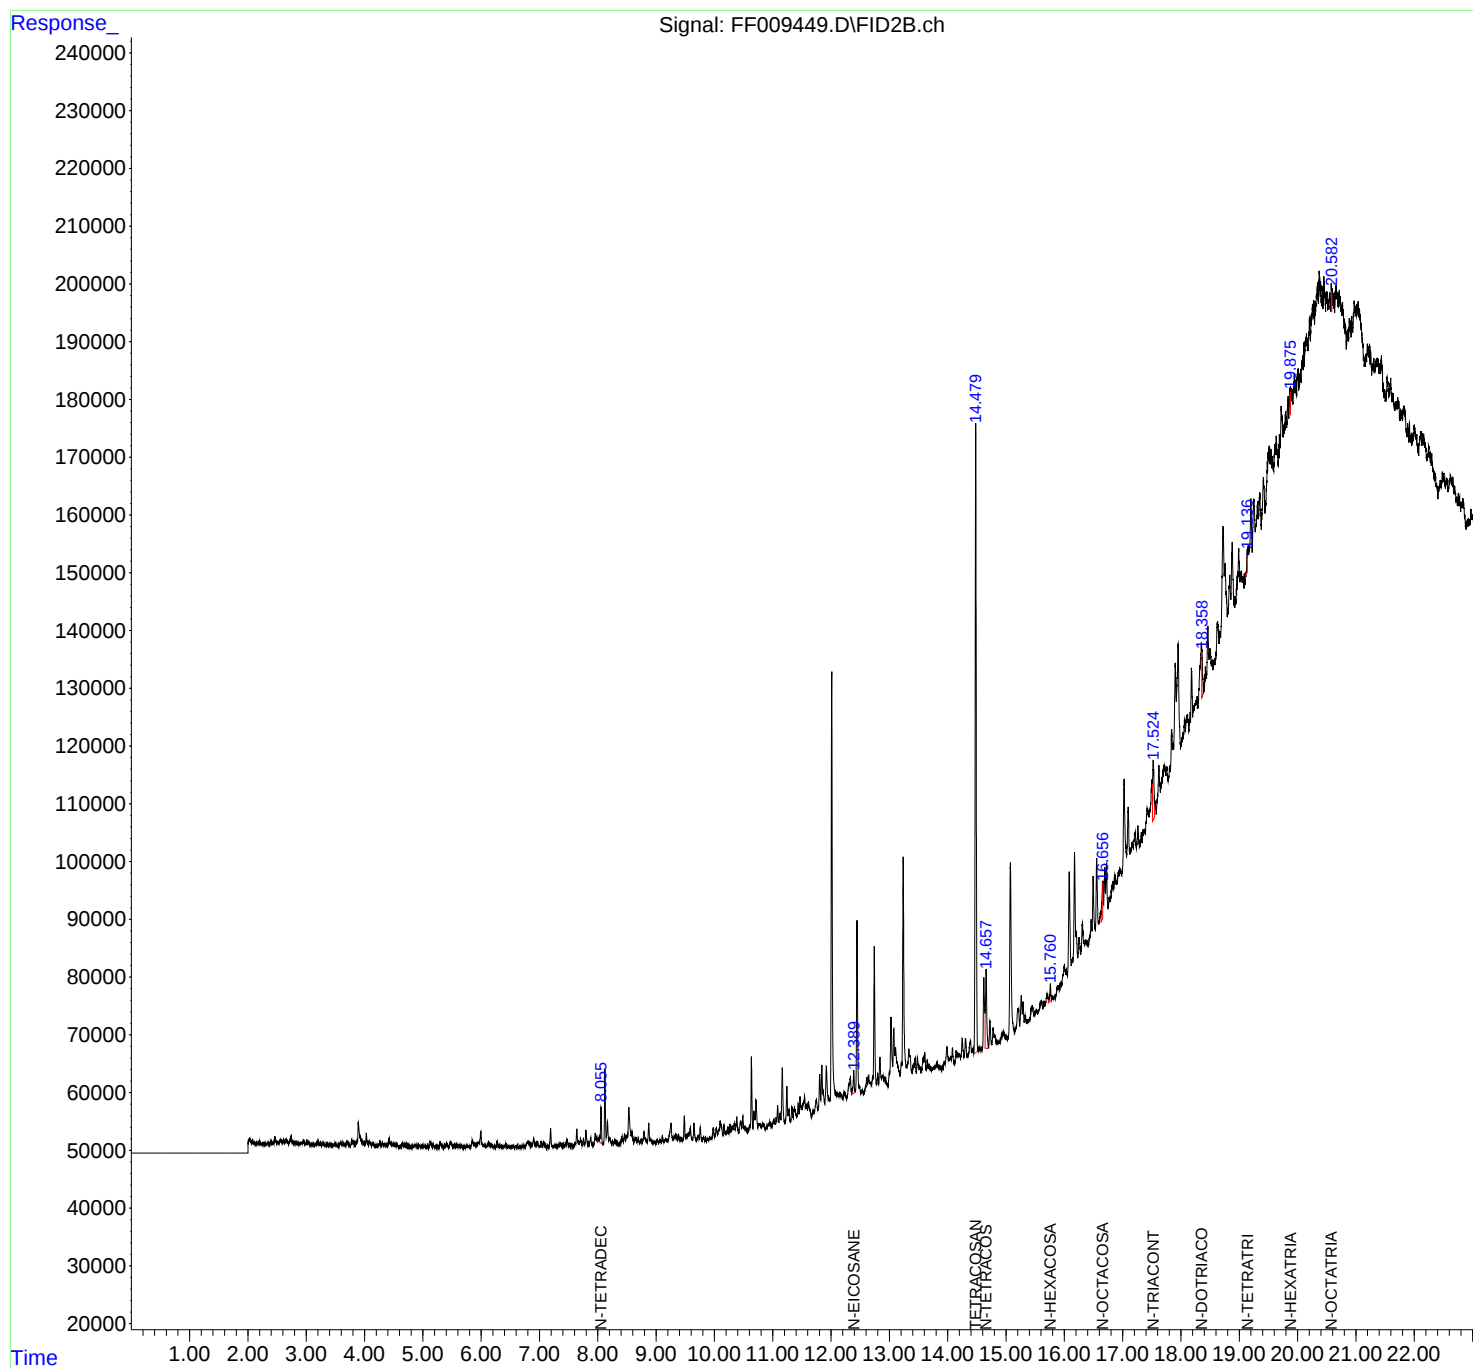


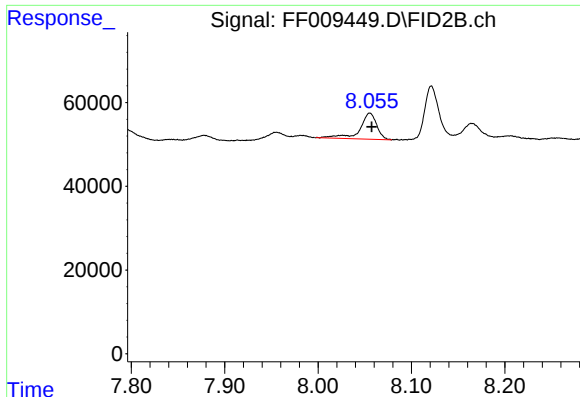

#4 N-TETRADECANE


R.T.: 8.055 min
Delta R.T.: -0.002 min
Response: 77986
Conc: 0.54 ug/ml

Instrument :
FID_F
ClientSampleId :

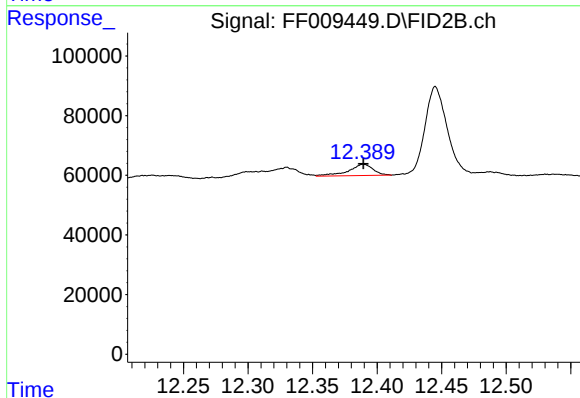


#7 N-EICOSANE

R.T.: 12.389 min
Delta R.T.: 0.000 min
Response: 50619
Conc: 0.36 ug/ml

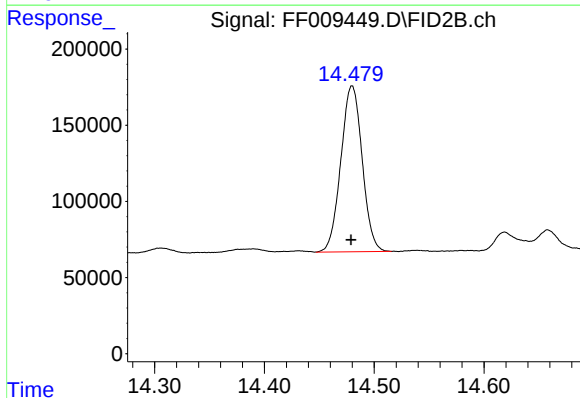


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.480 min
Delta R.T.: 0.000 min
Response: 1471062
Conc: 12.70 ug/ml

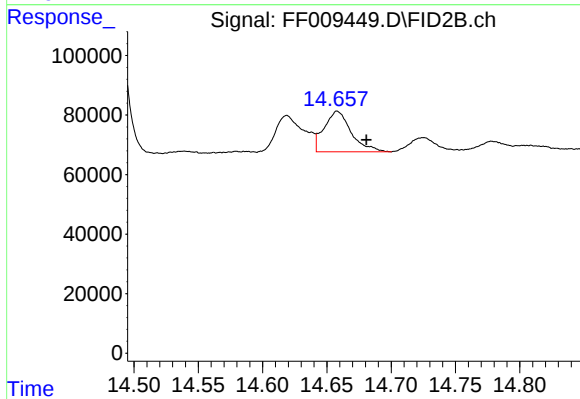

#10 N-TETRACOSANE


R.T.: 14.658 min
Delta R.T.: -0.023 min
Response: 200330
Conc: 1.52 ug/ml

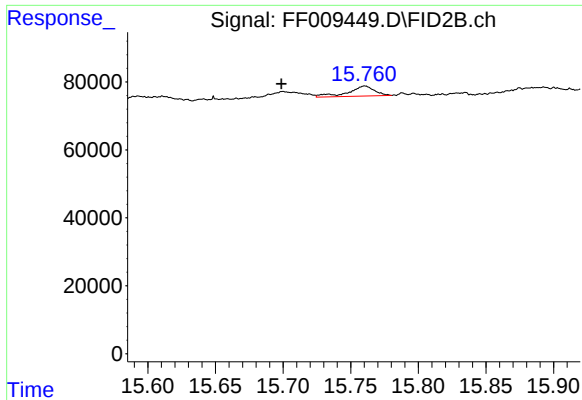

#11 N-HEXACOSANE


R.T.: 15.761 min
Delta R.T.: 0.062 min
Response: 40266
Conc: 0.32 ug/ml

Instrument :
FID_F
ClientSampleId :

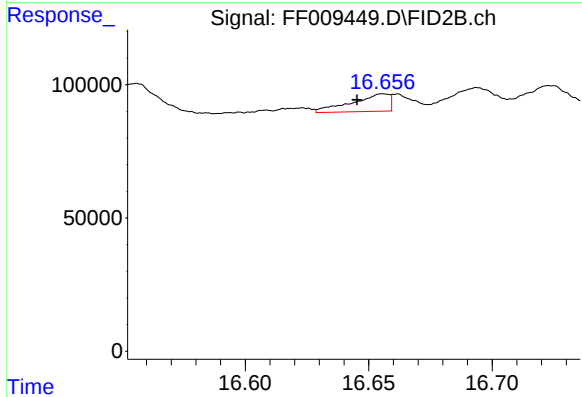


#12 N-OCTACOSANE

R.T.: 16.656 min
Delta R.T.: 0.011 min
Response: 68635
Conc: 0.58 ug/ml

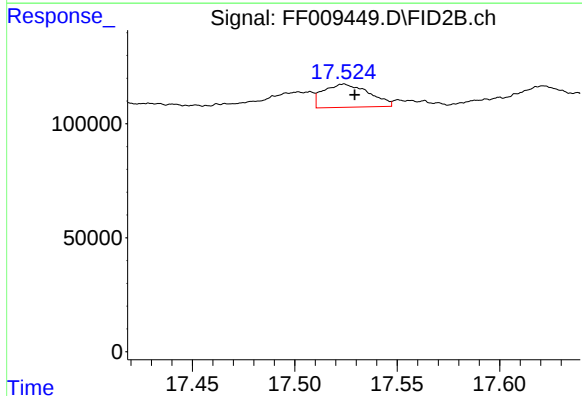


#13 N-TRIACONTANE

R.T.: 17.524 min
Delta R.T.: -0.005 min
Response: 157814
Conc: 1.38 ug/ml

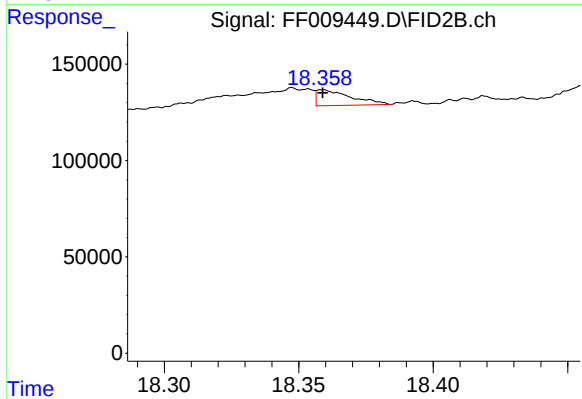

#14 N-DOTRIACONTANE


R.T.: 18.359 min
Delta R.T.: 0.000 min
Response: 72829
Conc: 0.67 ug/ml

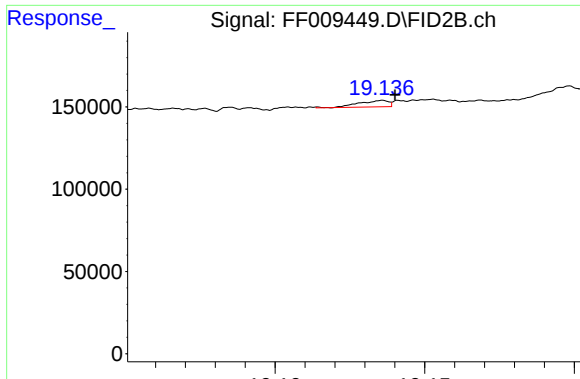

#15 N-TETRATRIACONTANE


R.T.: 19.136 min
Delta R.T.: -0.004 min
Response: 27102
Conc: 0.26 ug/ml

Instrument :
FID_F
ClientSampleId :

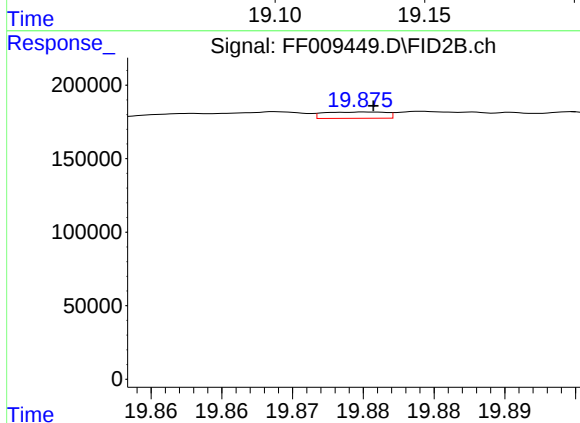

#16 N-HEXATRIACONTANE

R.T.: 19.876 min
Delta R.T.: 0.000 min
Response: 12887
Conc: 0.13 ug/ml

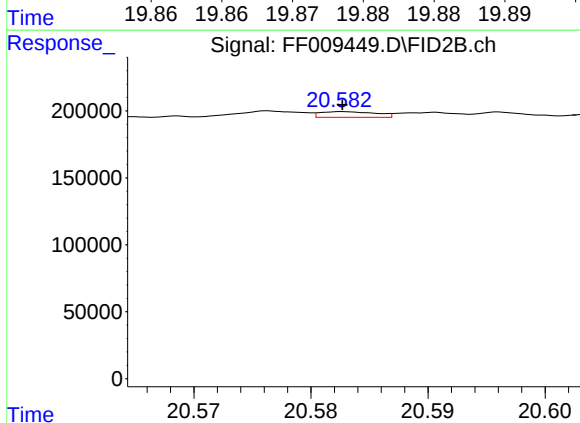

#17 N-OCTATRIACONTANE

R.T.: 20.583 min
Delta R.T.: 0.000 min
Response: 13893
Conc: 0.14 ug/ml