

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121521\
Data File : FF009445.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2021 21:57
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Dec 16 03:41:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.271	1335129	9.232 ug/ml
12) N-OCTACOSANE	16.645	1154115	9.692 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121521\
Data File : FF009445.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2021 21:57
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: Sample.e
Quant Time: Dec 16 03:41:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

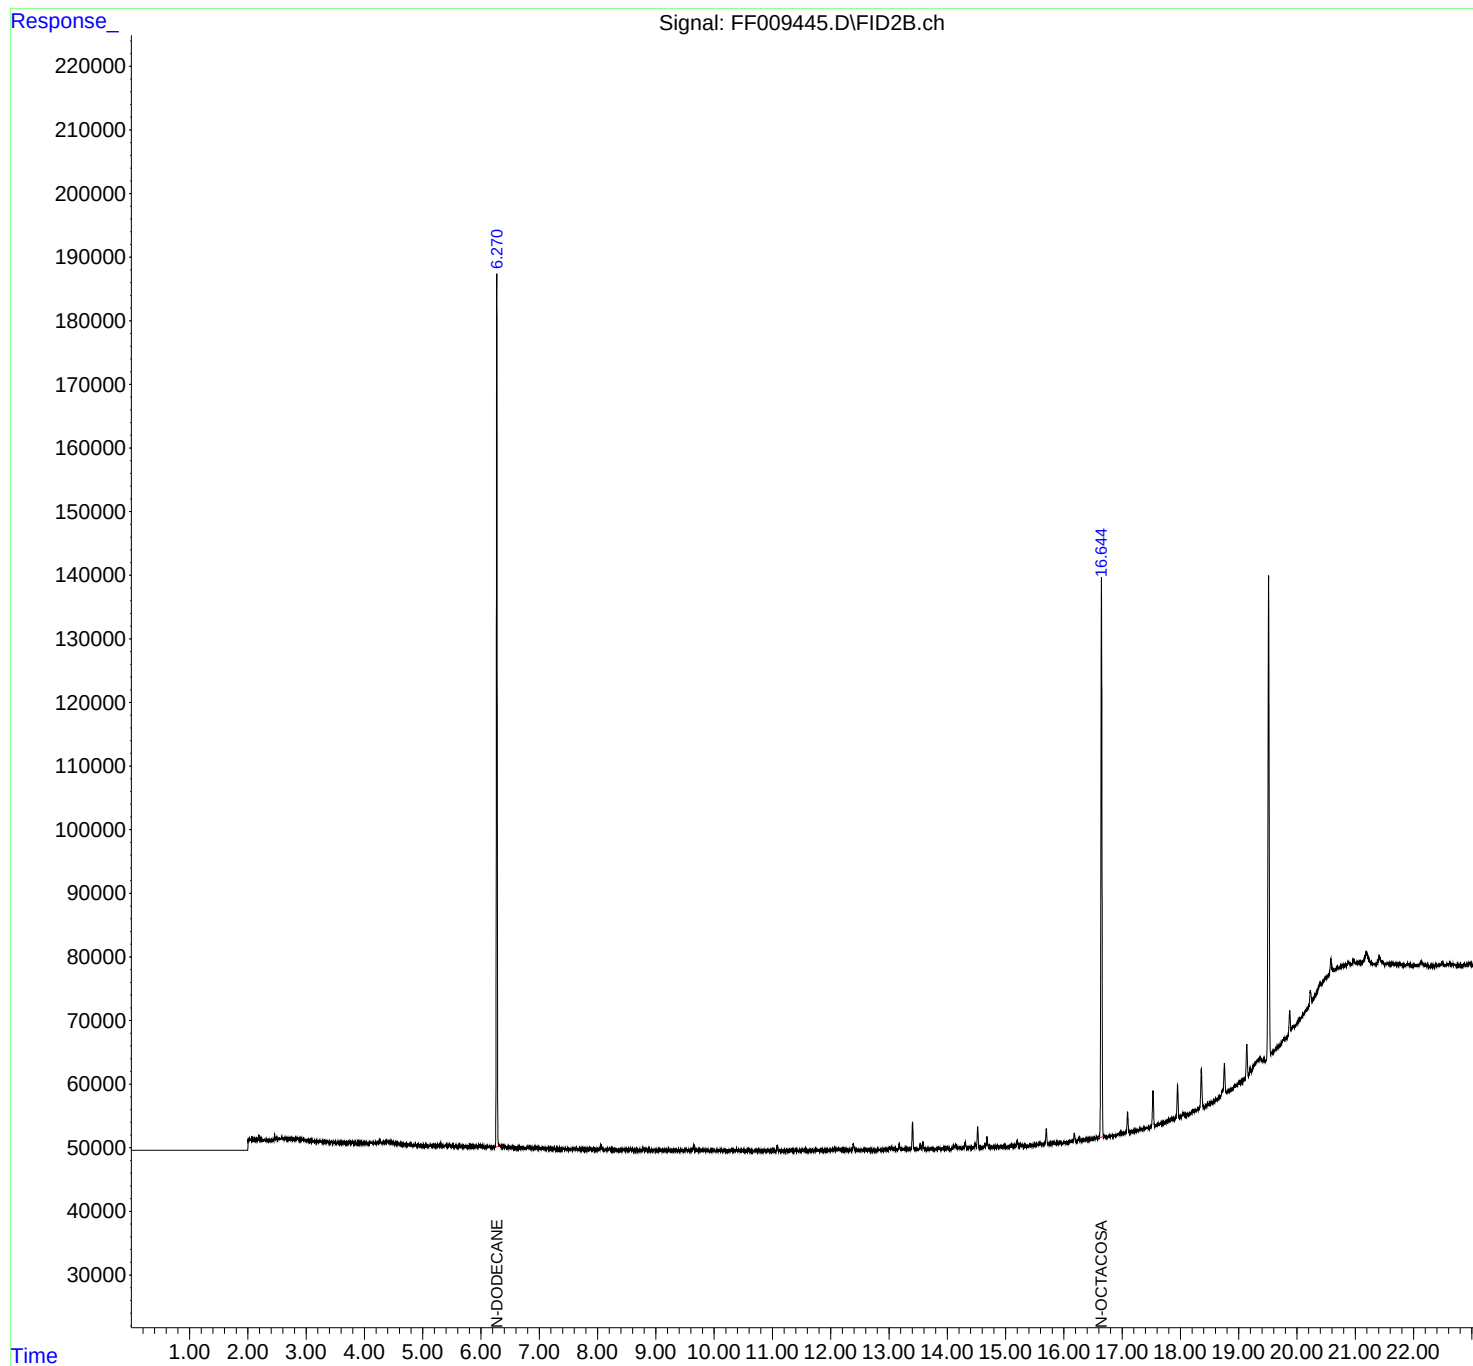


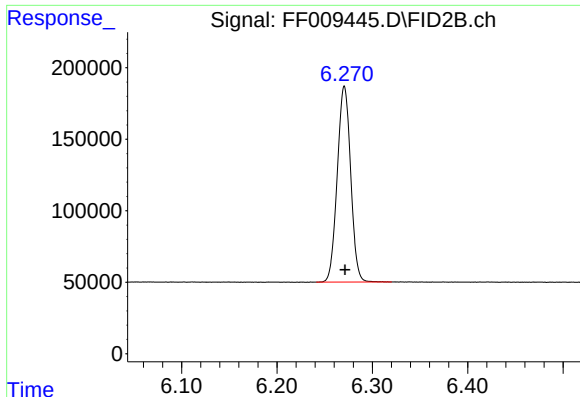

#3 N-DODECANE


R.T.: 6.271 min
Delta R.T.: 0.000 min
Response: 1335129
Conc: 9.23 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

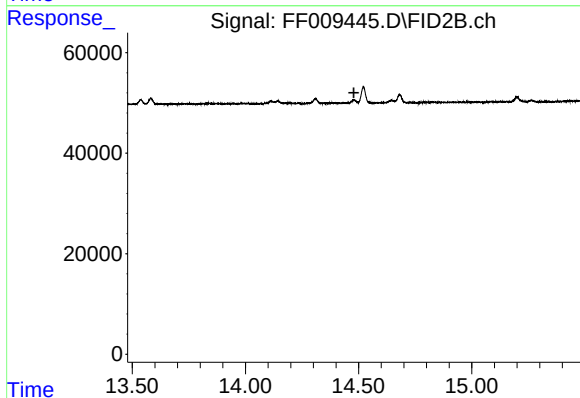

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

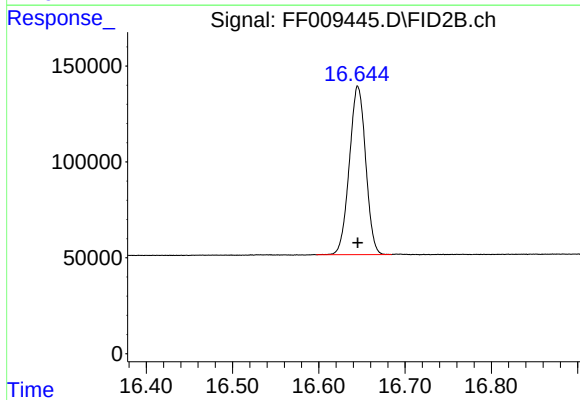

#12 N-OCTACOSANE

R.T.: 16.645 min
Delta R.T.: 0.000 min
Response: 1154115
Conc: 9.69 ug/ml