

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121523\
 Data File : FF013871.D
 Signal(s) : FID2B.ch
 Acq On : 15 Dec 2023 11:14
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 15 22:35:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
 Quant Title :
 QLast Update : Tue Dec 05 11:16:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.967	2117066	17.915 ug/ml
Target Compounds			
18) N-TETRACONTANE	22.074f	275368	3.526 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121523\
Data File : FF013871.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2023 11:14
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 15 22:35:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

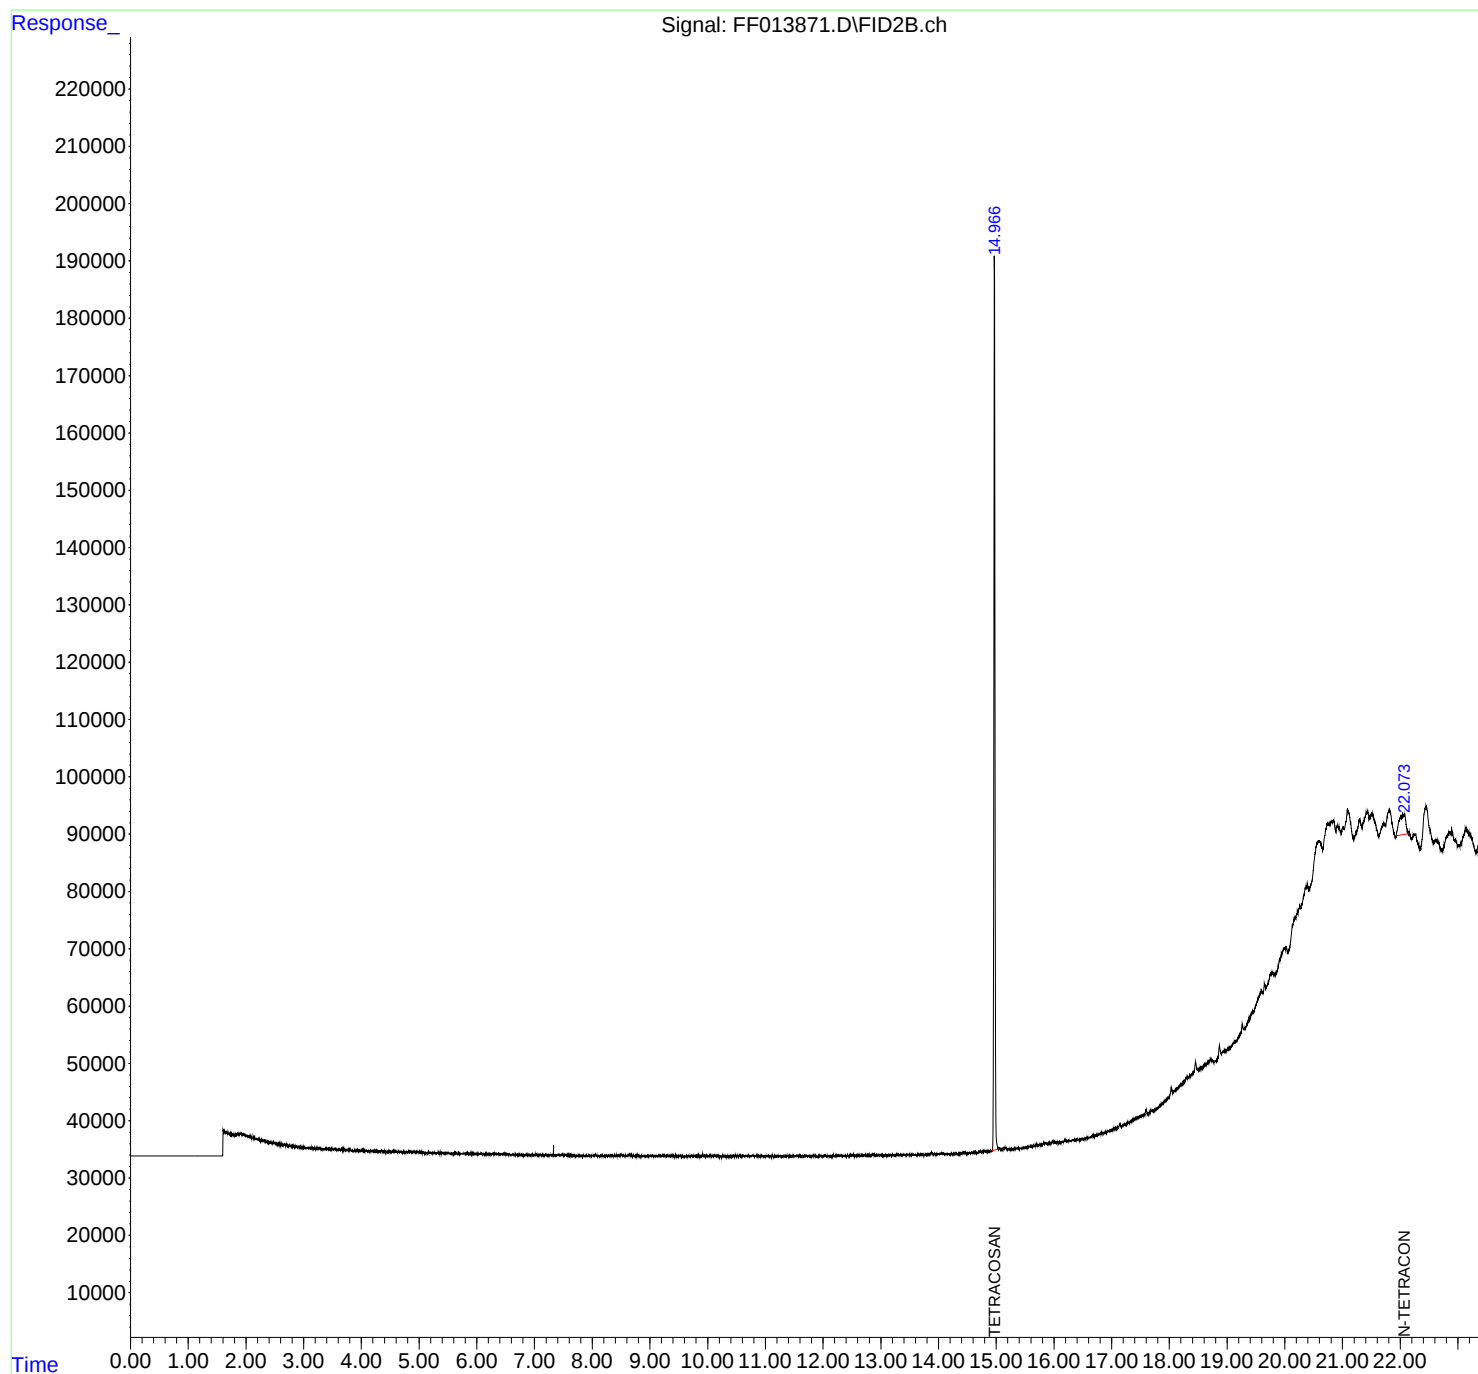


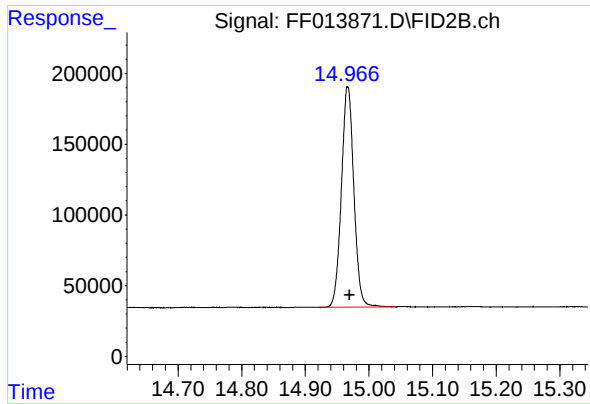

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.967 min
Delta R.T.: -0.003 min
Response: 2117066
Conc: 17.92 ug/ml

Instrument :
FID_F
ClientSampleId :

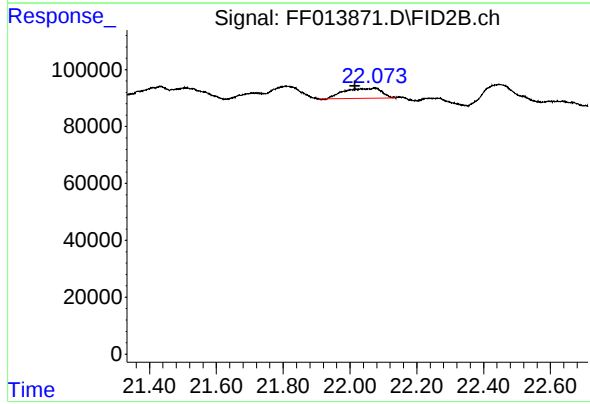

#18 N-TETRACONTANE

R.T.: 22.074 min
Delta R.T.: 0.059 min
Response: 275368
Conc: 3.53 ug/ml