

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121523\  
Data File : FF013880.D  
Signal(s) : FID2B.ch  
Acq On : 15 Dec 2023 17:03  
Operator : YP\AJ  
Sample : PB157845BL  
Misc :  
ALS Vial : 65 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 15 22:36:26 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120523.M  
Quant Title :  
QLast Update : Tue Dec 05 11:16:50 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.969 | 2015250  | 17.054 ug/ml |
| Target Compounds              |        |          |              |
| 13) N-TRIACONTANE             | 18.037 | 47948    | 0.409 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.862 | 48446    | 0.427 ug/ml  |
| 15) N-TETRATRIACONTANE        | 19.622 | 115861   | 1.182 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.399 | 55296    | 0.687 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121523\  
Data File : FF013880.D  
Signal(s) : FID2B.ch  
Acq On : 15 Dec 2023 17:03  
Operator : YP\AJ  
Sample : PB157845BL  
Misc :  
ALS Vial : 65 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 15 22:36:26 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120523.M  
Quant Title :  
QLast Update : Tue Dec 05 11:16:50 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

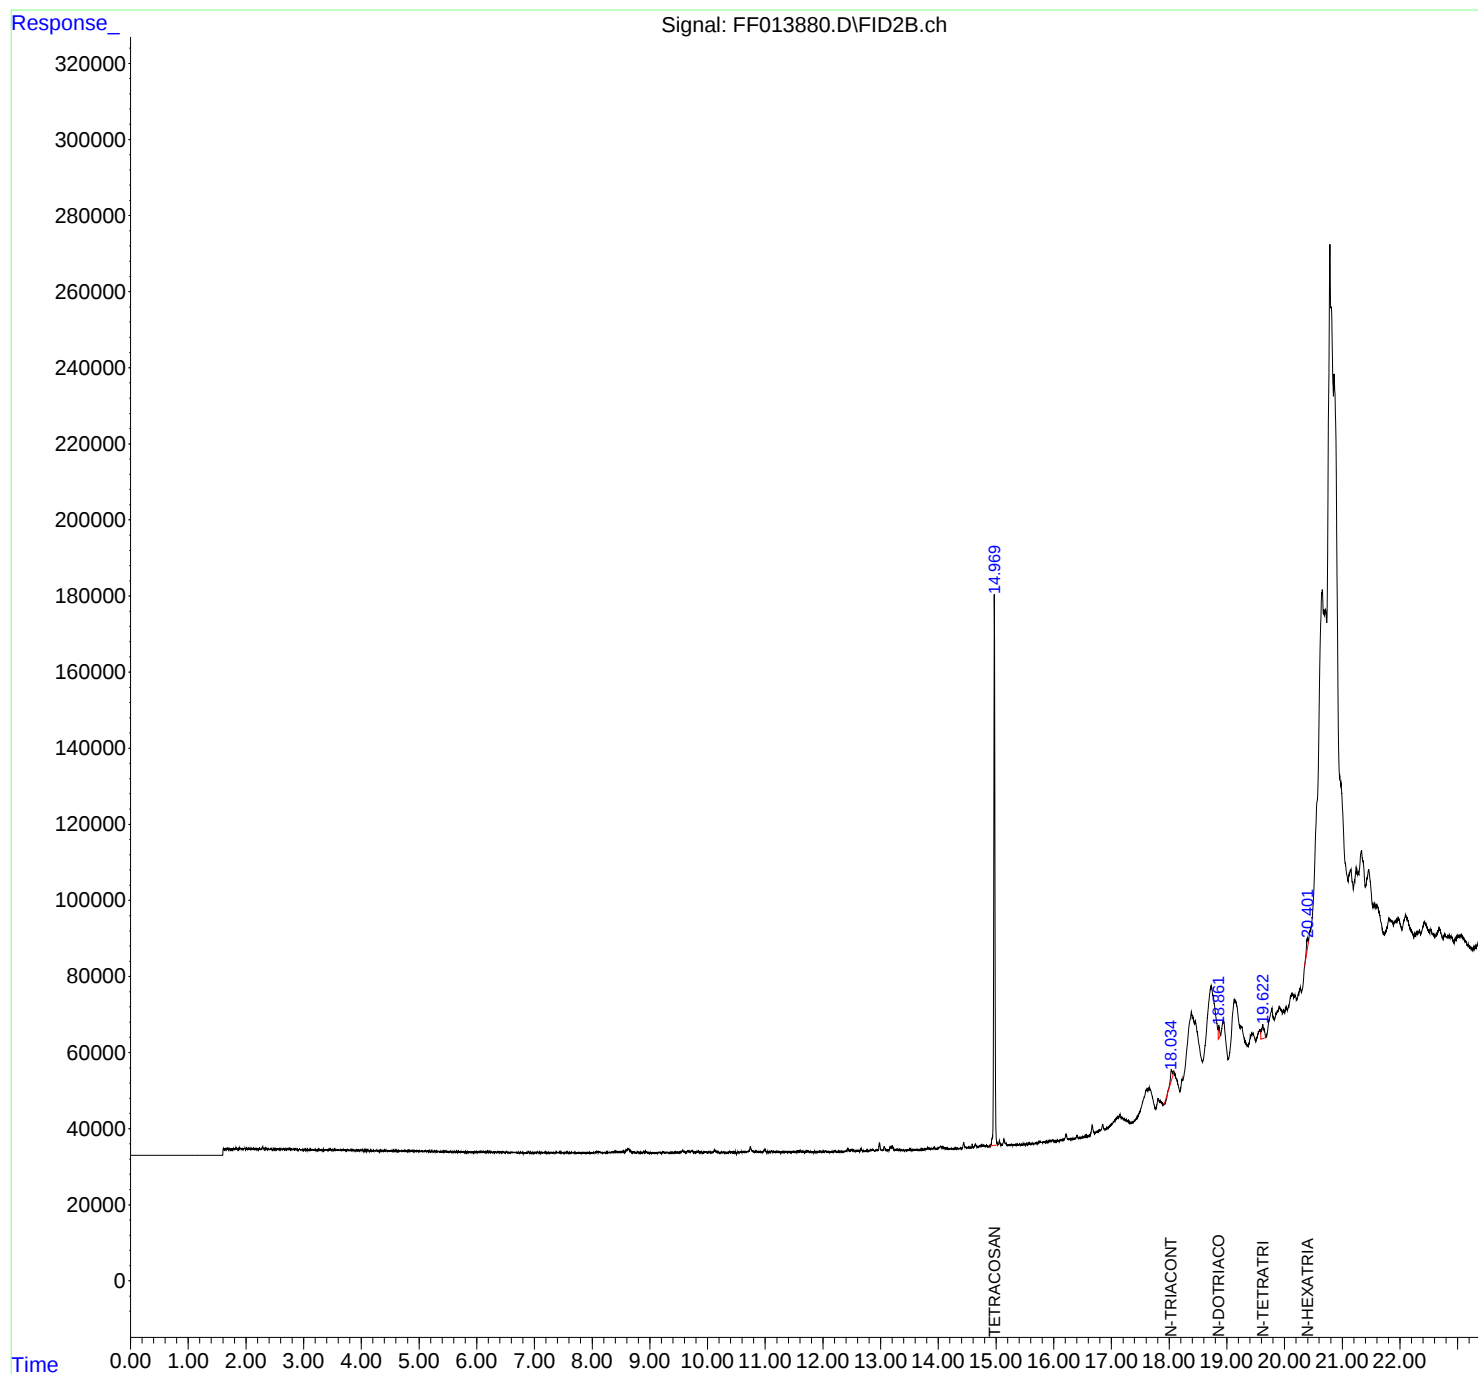


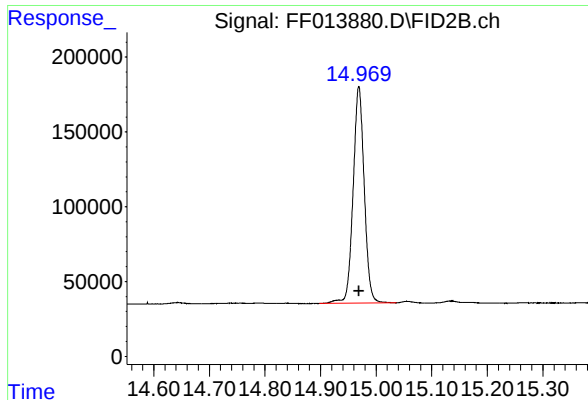

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.969 min  
Delta R.T.: 0.000 min  
Response: 2015250  
Conc: 17.05 ug/ml

Instrument : FID\_F  
ClientSampleId :

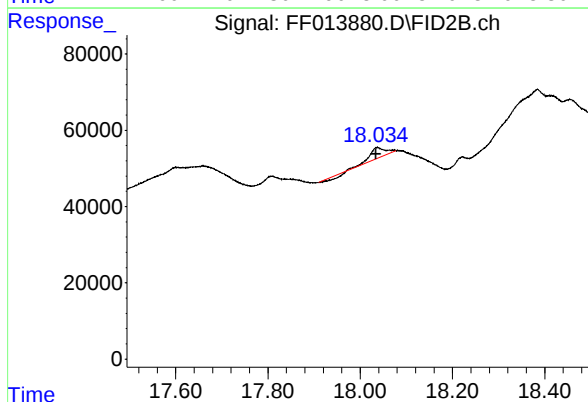


#13 N-TRIACONTANE

R.T.: 18.037 min  
Delta R.T.: 0.003 min  
Response: 47948  
Conc: 0.41 ug/ml

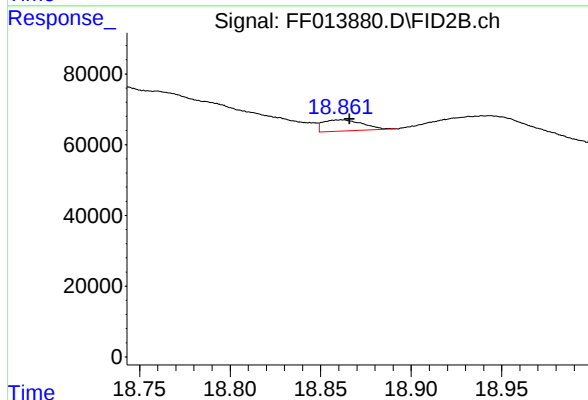


#14 N-DOTRIACONTANE

R.T.: 18.862 min  
Delta R.T.: -0.005 min  
Response: 48446  
Conc: 0.43 ug/ml

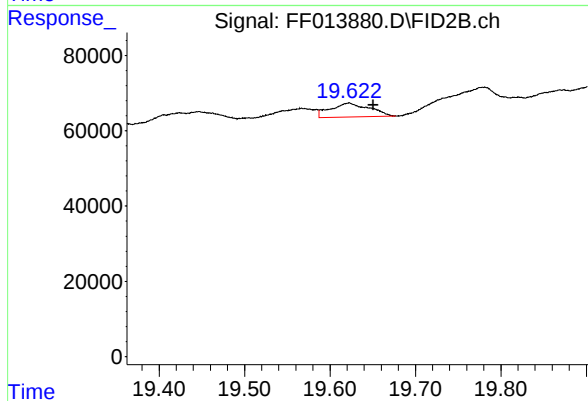

#15 N-TETRATRIACONTANE

R.T.: 19.622 min  
Delta R.T.: -0.028 min  
Response: 115861  
Conc: 1.18 ug/ml

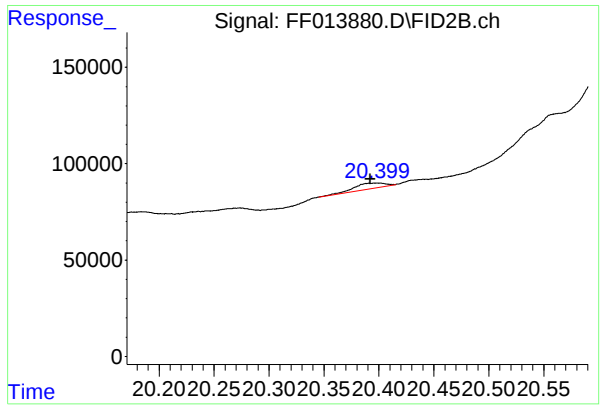

#16 N-HEXATRIACONTANE

R.T.: 20.399 min  
Delta R.T.: 0.007 min  
Response: 55296  
Conc: 0.69 ug/ml

Instrument :  
FID\_F  
ClientSampleId :