

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121523\
 Data File : FF013874.D
 Signal(s) : FID2B.ch
 Acq On : 15 Dec 2023 14:03
 Operator : YP\AJ
 Sample : 05853-01
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SOUTH-WALL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/18/2023
 Supervised By :Ankita Jodhani 12/18/2023

Integration File: autoint1.e
 Quant Time: Dec 15 22:35:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
 Quant Title :
 QLast Update : Tue Dec 05 11:16:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.967	1716867	14.529 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121523\
Data File : FF013874.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2023 14:03
Operator : YP\AJ
Sample : 05853-01
Misc :
ALS Vial : 61 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
SOUTH-WALL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/18/2023
Supervised By :Ankita Jodhani 12/18/2023

Integration File: autoint1.e
Quant Time: Dec 15 22:35:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

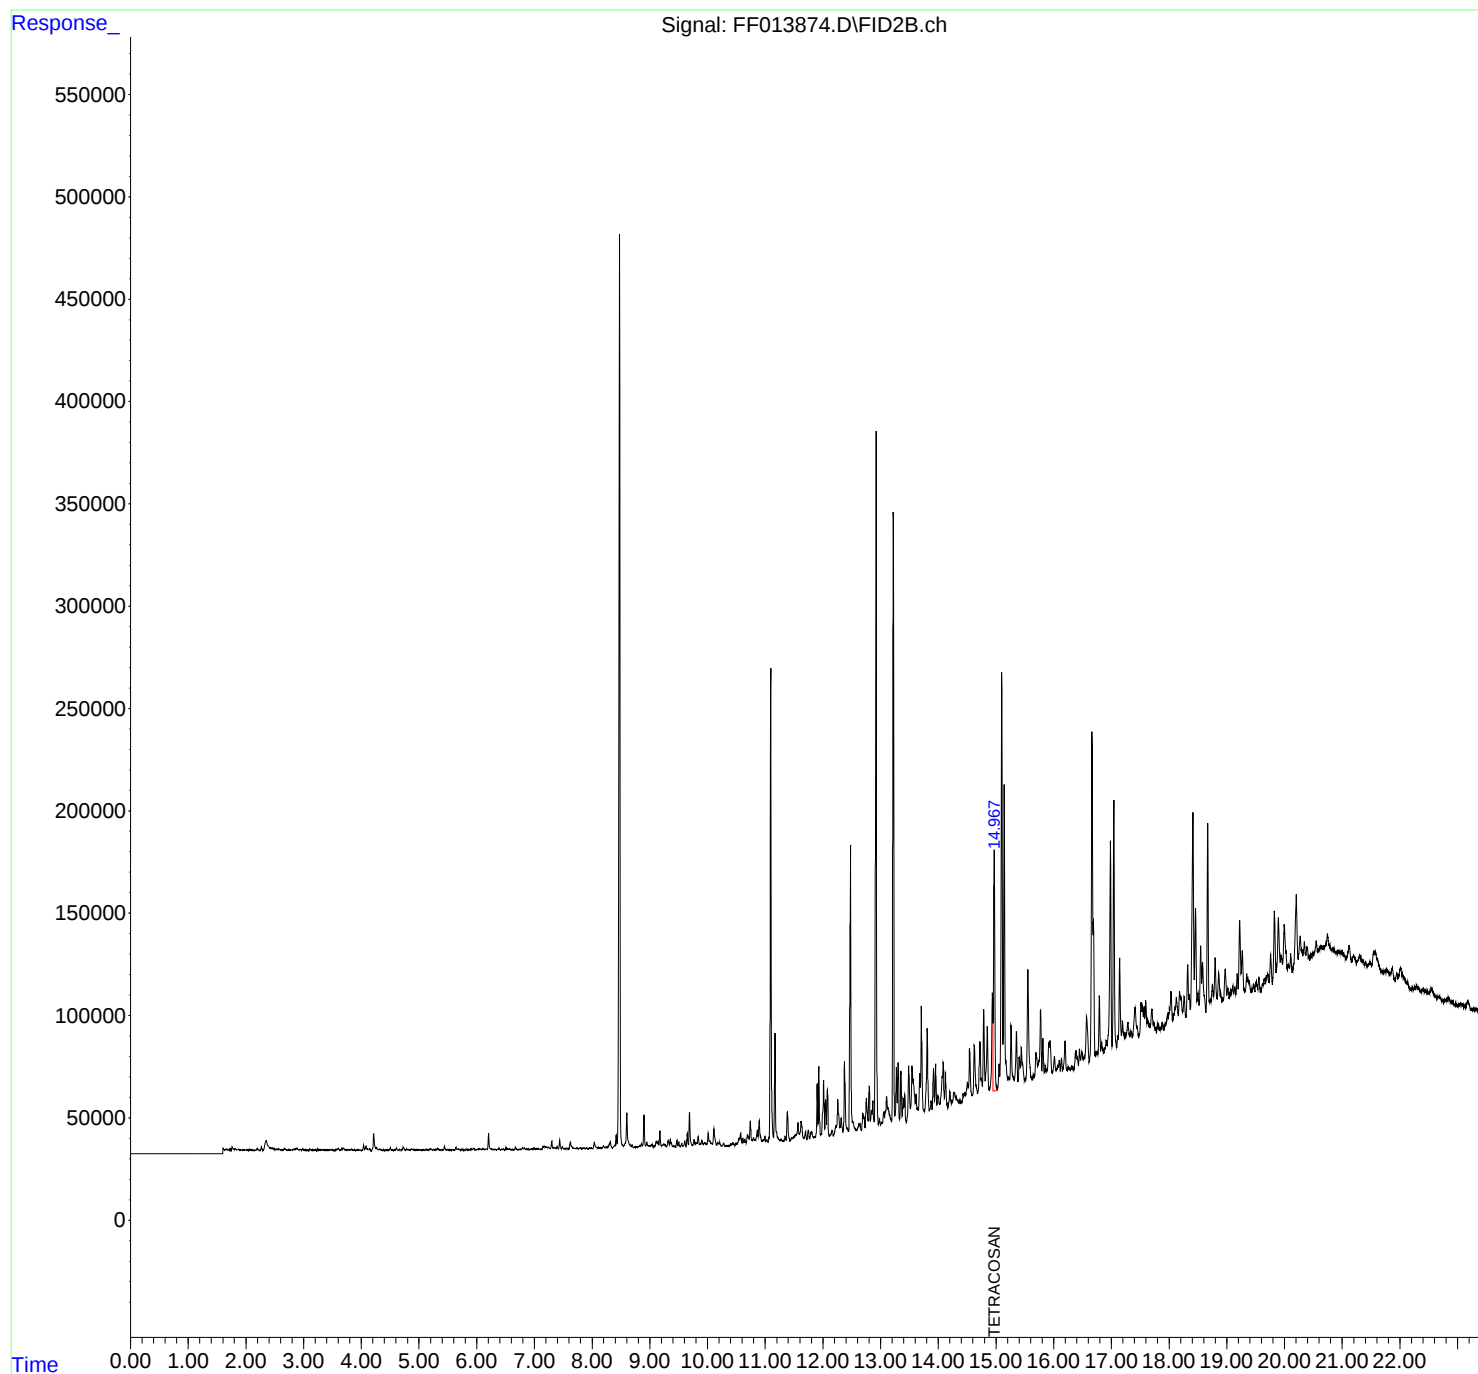

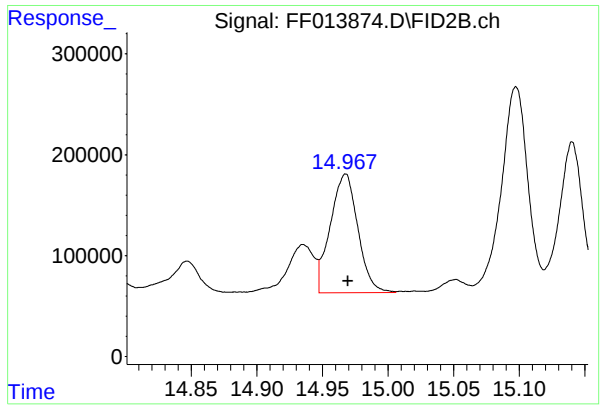

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.967 min
Delta R.T.: -0.002 min
Response: 1716867
Conc: 14.53 ug/ml

Instrument :

FID_F

ClientSampleId :

SOUTH-WALL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 12/18/2023

Supervised By :Ankita Jodhani 12/18/2023