

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121523\
Data File : FF013877.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2023 15:36
Operator : YP\AJ
Sample : 05862-02 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FL-06-20231213-13.0-13.5

Integration File: autoint1.e
Quant Time: Dec 15 22:35:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.976	1050455	8.889 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121523\
Data File : FF013877.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2023 15:36
Operator : YP\AJ
Sample : 05862-02 10X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
FL-06-20231213-13.0-13.5

Integration File: autoint1.e
Quant Time: Dec 15 22:35:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

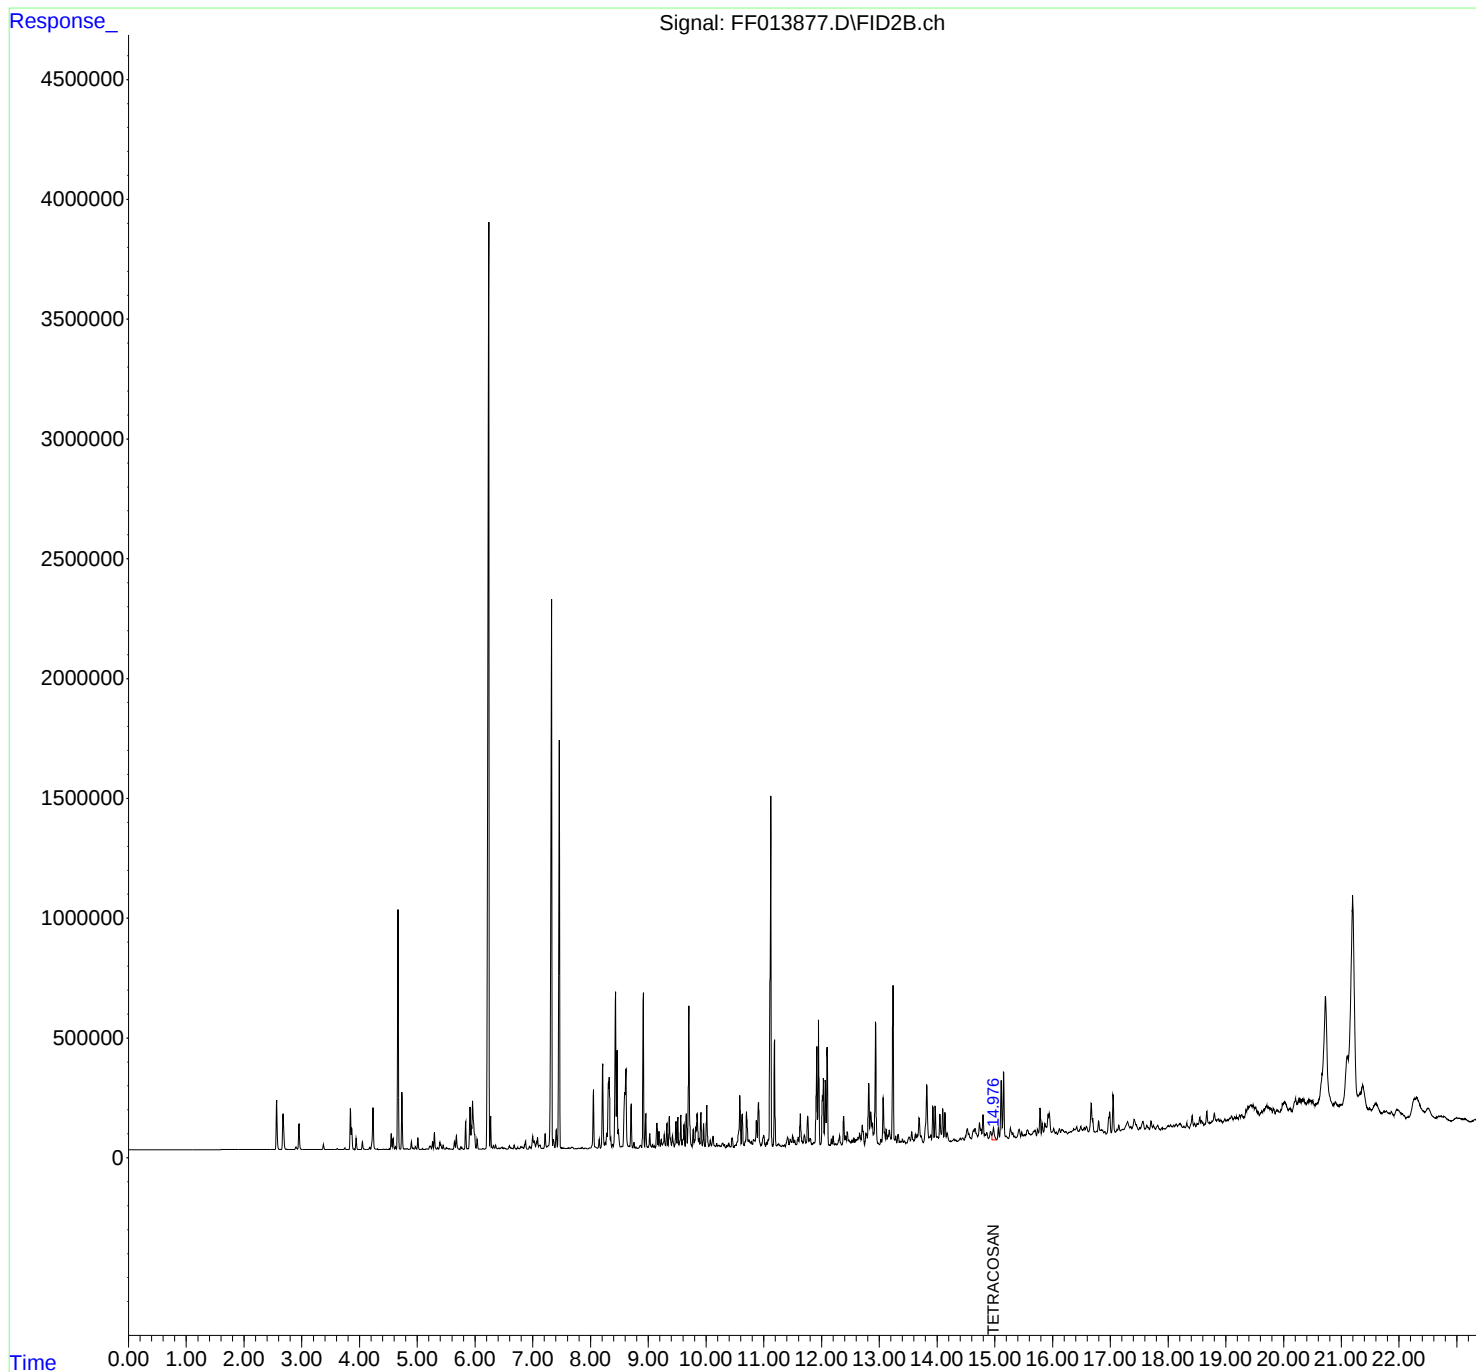

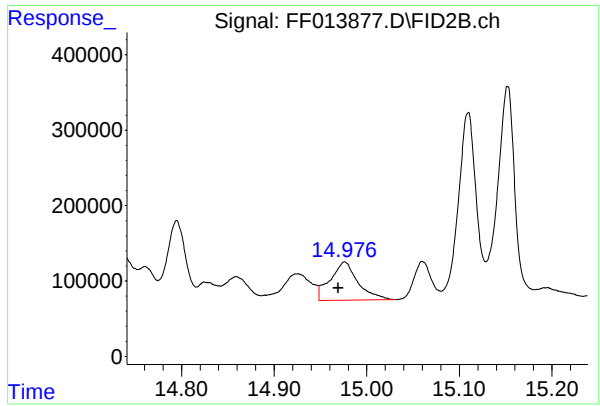

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.976 min
Delta R.T.: 0.007 min
Response: 1050455
Conc: 8.89 ug/ml

Instrument :
FID_F
ClientSampleId :
FL-06-20231213-13.0-13.5