

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121523\
Data File : FF013878.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2023 16:05
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/19/2024
Supervised By :Sohil Jodhani 01/19/2024

Integration File: autoint1.e
Quant Time: Dec 28 02:45:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.970	1871657	15.839 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121523\
Data File : FF013878.D
Signal(s) : FID2B.ch
Acq On : 15 Dec 2023 16:05
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1


Instrument :
FID_F
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/19/2024
Supervised By :Sohil Jodhani 01/19/2024

Integration File: autoint1.e
Quant Time: Dec 28 02:45:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

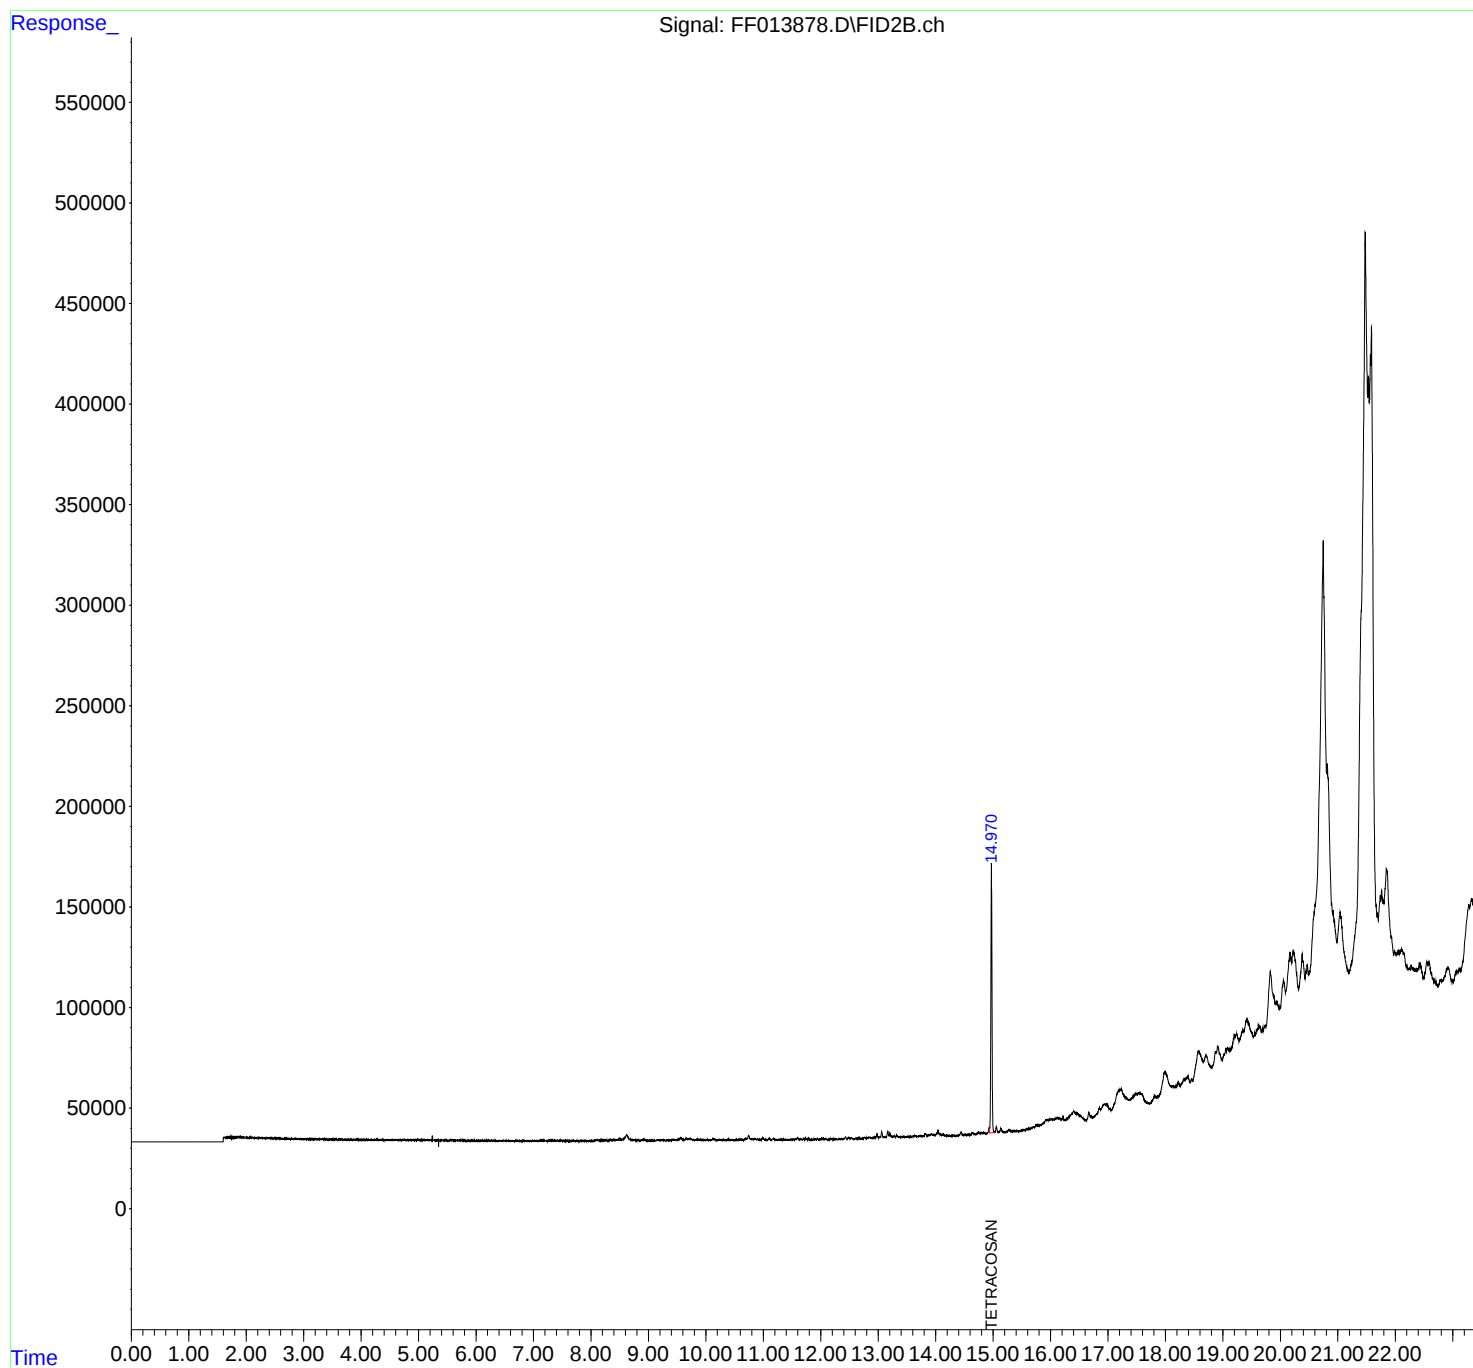

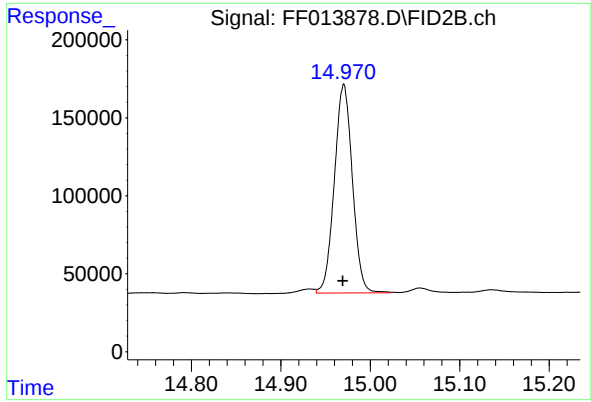

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.970 min
Delta R.T.: 0.000 min
Response: 1871657
Conc: 15.84 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/19/2024
Supervised By :Sohil Jodhani 01/19/2024