

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121523\  
 Data File : FF013883.D  
 Signal(s) : FID2B.ch  
 Acq On : 15 Dec 2023 18:31  
 Operator : YP\AJ  
 Sample : 05862-12  
 Misc :  
 ALS Vial : 68 Sample Multiplier: 1

Instrument :  
 FID\_F  
 ClientSampleId :  
 WC-LIQUIDS-20231213-01

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 12/18/2023  
 Supervised By :Ankita Jodhani 12/18/2023

Integration File: autoint1.e  
 Quant Time: Dec 15 22:36:52 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120523.M  
 Quant Title :  
 QLast Update : Tue Dec 05 11:16:50 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.962 | 9253793  | 78.308 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121523\  
Data File : FF013883.D  
Signal(s) : FID2B.ch  
Acq On : 15 Dec 2023 18:31  
Operator : YP\AJ  
Sample : 05862-12  
Misc :  
ALS Vial : 68 Sample Multiplier: 1


Instrument :  
FID\_F  
ClientSampleId :  
WC-LIQUIDS-20231213-01


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/18/2023  
Supervised By :Ankita Jodhani 12/18/2023

Integration File: autoint1.e  
Quant Time: Dec 15 22:36:52 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120523.M  
Quant Title :  
QLast Update : Tue Dec 05 11:16:50 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

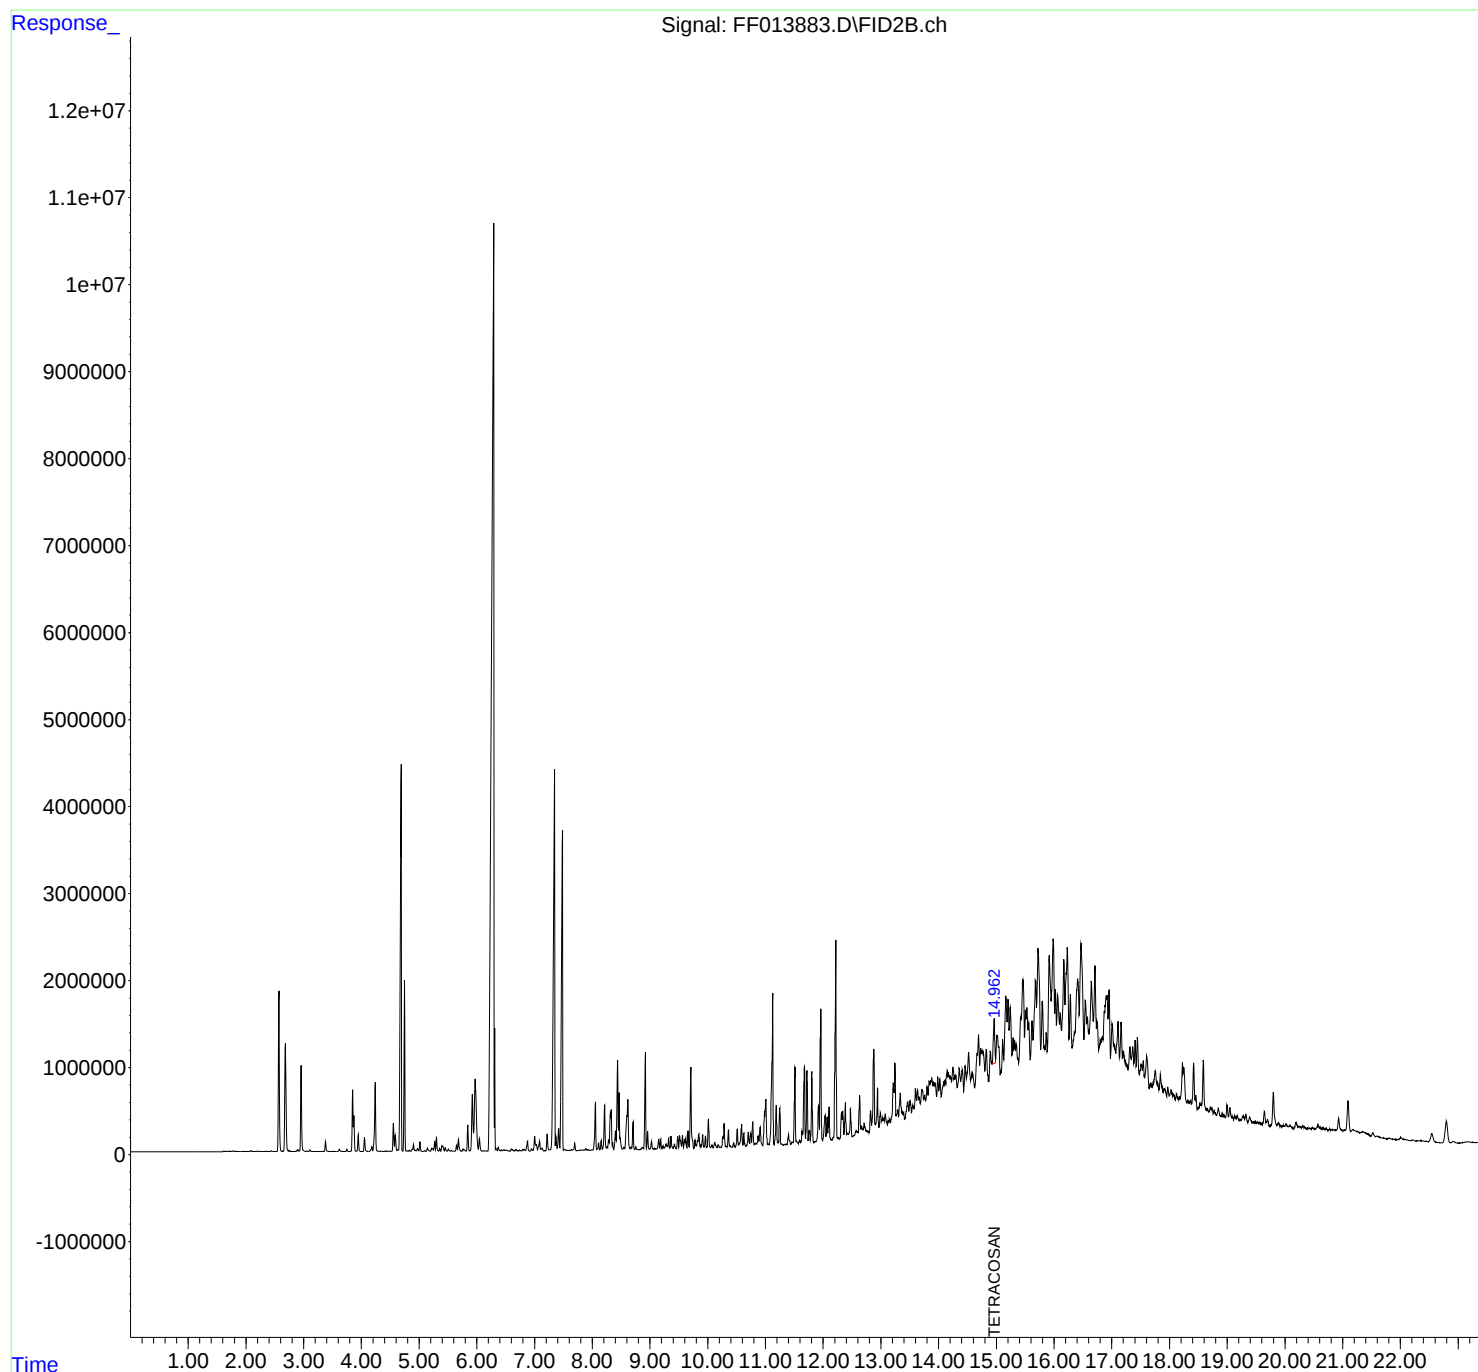

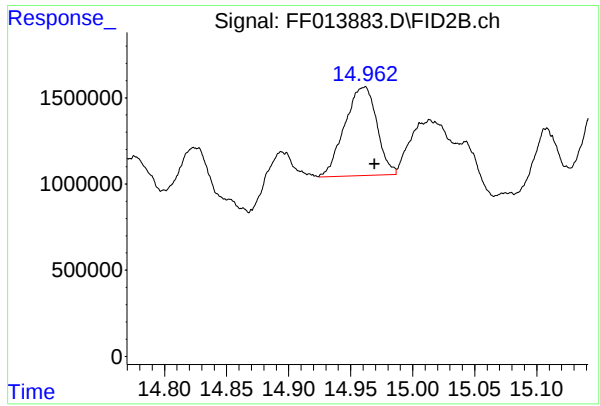

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.962 min  
Delta R.T.: -0.008 min  
Response: 9253793  
Conc: 78.31 ug/ml

Instrument :  
FID\_F  
ClientSampleId :  
WC-LIQUIDS-20231213-01

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 12/18/2023  
Supervised By :Ankita Jodhani 12/18/2023