

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
 Data File : FF009449.D
 Signal(s) : FID2B.ch
 Acq On : 16 Dec 2021 09:49
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 14:28:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
7) N-EICOSANE	12.379	107177	0.756 ug/ml
8) N-DOCOSANE	13.579	107535	0.789 ug/ml
10) N-TETRACOSANE	14.678	85064	0.646 ug/ml
11) N-HEXACOSANE	15.696	90593	0.725 ug/ml
12) N-OCTACOSANE	16.644	169479	1.423 ug/ml
13) N-TRIACONTANE	17.526	471337	4.115 ug/ml
14) N-DOTRIACONTANE	18.358	606677	5.551 ug/ml
15) N-TETRATRIACONTANE	19.139	466704	4.406 ug/ml
16) N-HEXATRIACONTANE	19.876	330404	3.299 ug/ml
17) N-OCTATRIACONTANE	20.584	152252	1.551 ug/ml
18) N-TETRACONTANE	21.415	206738	2.047 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009449.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 09:49
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 14:28:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

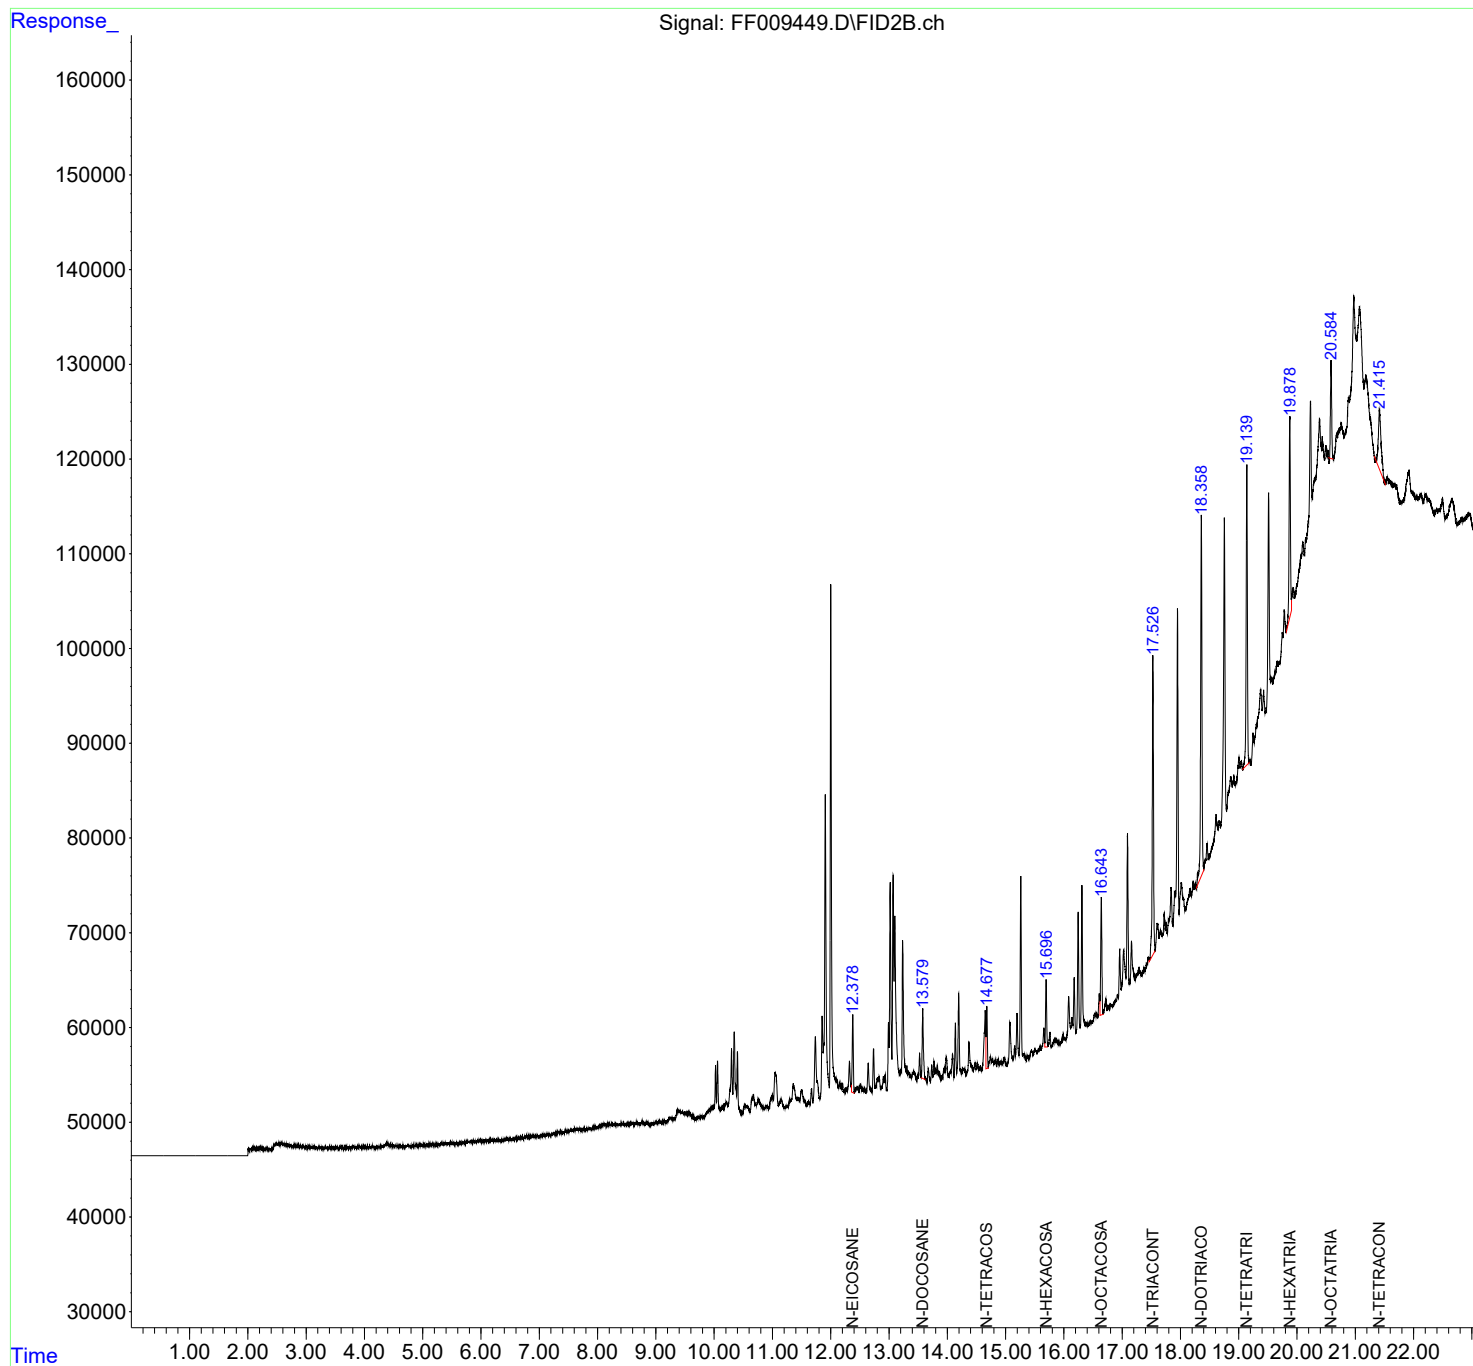


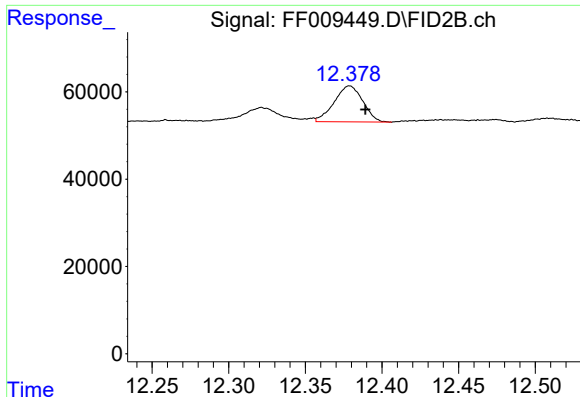

#7 N-EICOSANE


R.T.: 12.379 min
Delta R.T.: -0.010 min
Response: 107177
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :

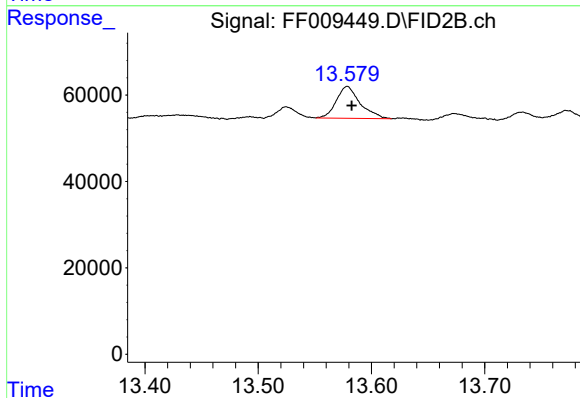


#8 N-DOCOSANE

R.T.: 13.579 min
Delta R.T.: -0.004 min
Response: 107535
Conc: 0.79 ug/ml

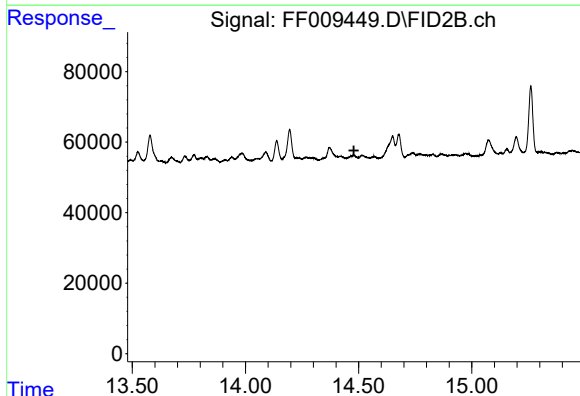


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

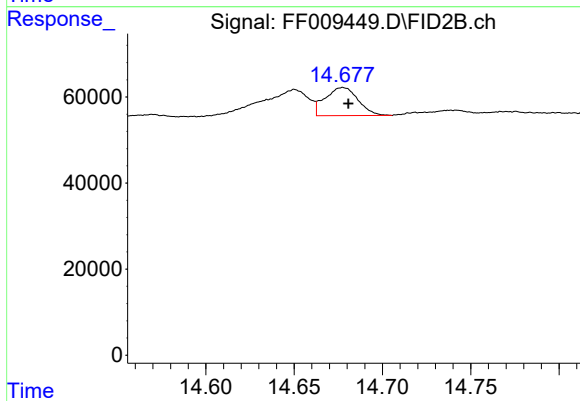

#10 N-TETRACOSANE


R.T.: 14.678 min
Delta R.T.: -0.003 min
Response: 85064
Conc: 0.65 ug/ml

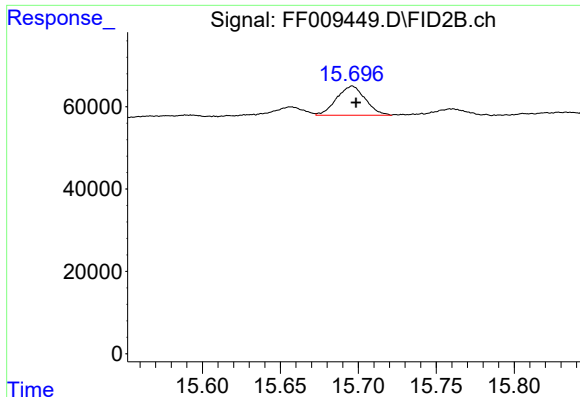

#11 N-HEXACOSANE


R.T.: 15.696 min
Delta R.T.: -0.002 min
Response: 90593
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

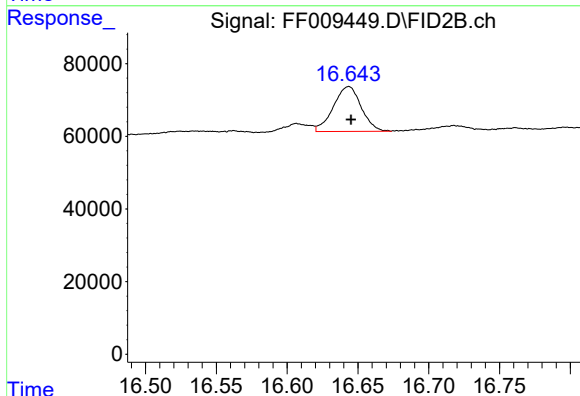


#12 N-OCTACOSANE

R.T.: 16.644 min
Delta R.T.: -0.001 min
Response: 169479
Conc: 1.42 ug/ml

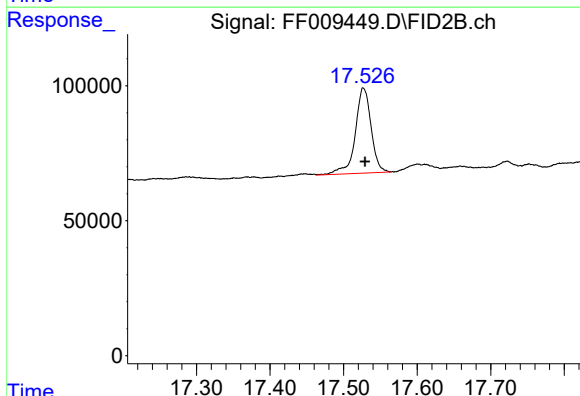


#13 N-TRIACONTANE

R.T.: 17.526 min
Delta R.T.: -0.003 min
Response: 471337
Conc: 4.11 ug/ml

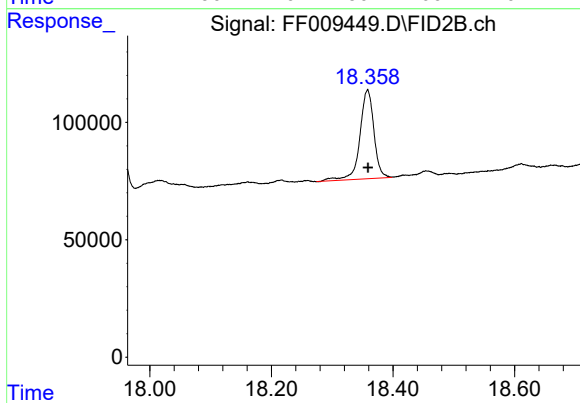

#14 N-DOTRIACONTANE


R.T.: 18.358 min
Delta R.T.: 0.000 min
Response: 606677
Conc: 5.55 ug/ml

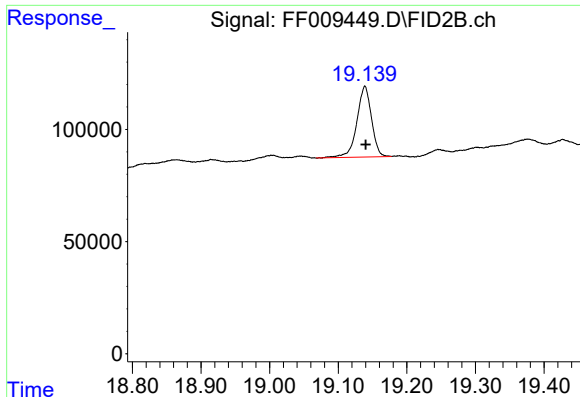

#15 N-TETRATRIACONTANE


R.T.: 19.139 min
Delta R.T.: -0.001 min
Response: 466704
Conc: 4.41 ug/ml

Instrument :
FID_F
ClientSampleId :

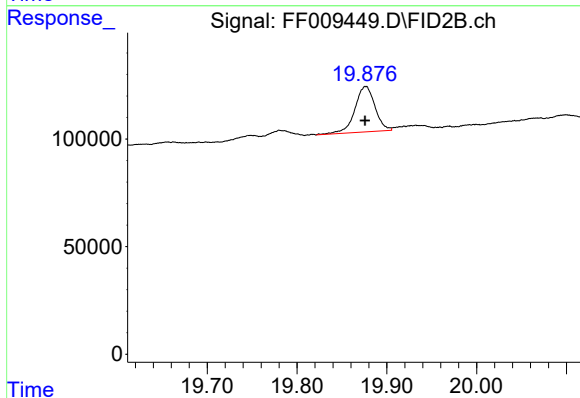


#16 N-HEXATRIACONTANE

R.T.: 19.876 min
Delta R.T.: 0.000 min
Response: 330404
Conc: 3.30 ug/ml

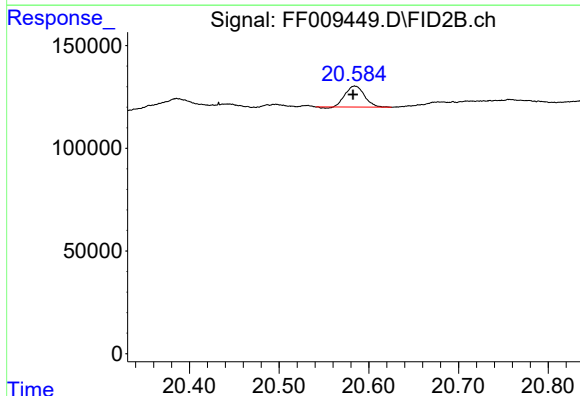

#17 N-OCTATRIACONTANE

R.T.: 20.584 min
Delta R.T.: 0.002 min
Response: 152252
Conc: 1.55 ug/ml

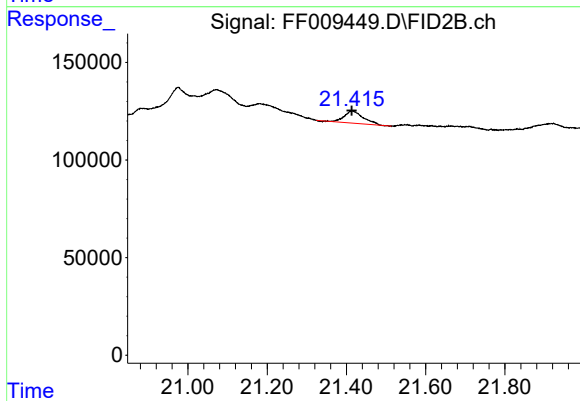

#18 N-TETRACONTANE

R.T.: 21.415 min
Delta R.T.: 0.002 min
Response: 206738
Conc: 2.05 ug/ml