

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
 Data File : FF009453.D
 Signal(s) : FID2B.ch
 Acq On : 16 Dec 2021 11:51
 Operator : AJ\MA
 Sample : M5074-02
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 14:28:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.481	1951497	16.846 ug/ml
Target Compounds			
4) N-TETRADECANE	8.055	93249	0.641 ug/ml
7) N-EICOSANE	12.390	56468	0.398 ug/ml
8) N-DOCOSANE	13.605	55096	0.404 ug/ml
10) N-TETRACOSANE	14.656	365018	2.772 ug/ml
11) N-HEXACOSANE	15.762f	43852	0.351 ug/ml
12) N-OCTACOSANE	16.655	165875	1.393 ug/ml
13) N-TRIACONTANE	17.532	199143	1.739 ug/ml
14) N-DOTRIACONTANE	18.357	294645	2.696 ug/ml
15) N-TETRATRIACONTANE	19.164	215674	2.036 ug/ml
16) N-HEXATRIACONTANE	19.875	49026	0.489 ug/ml
17) N-OCTATRIACONTANE	20.589	10319	0.105 ug/ml
18) N-TETRACONTANE	21.420	9310	0.092 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009453.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 11:51
Operator : AJ\MA
Sample : M5074-02
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 14:28:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

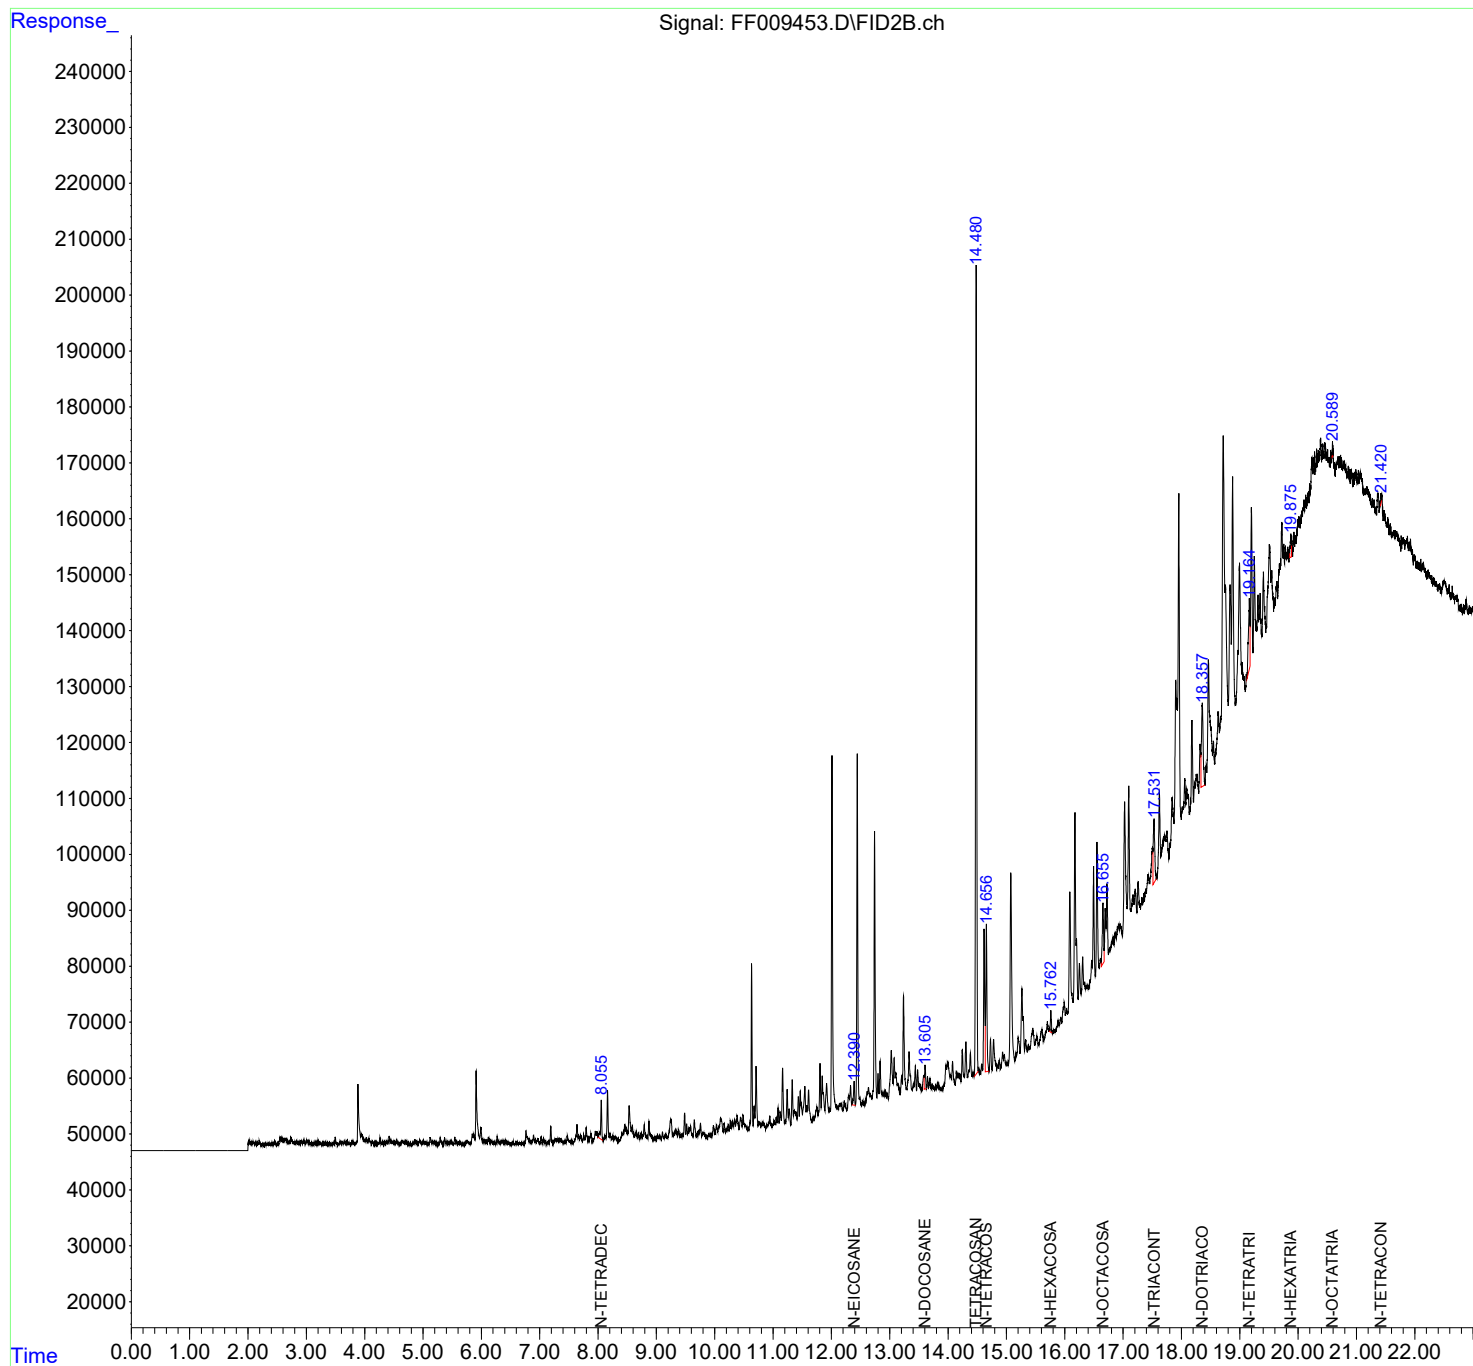


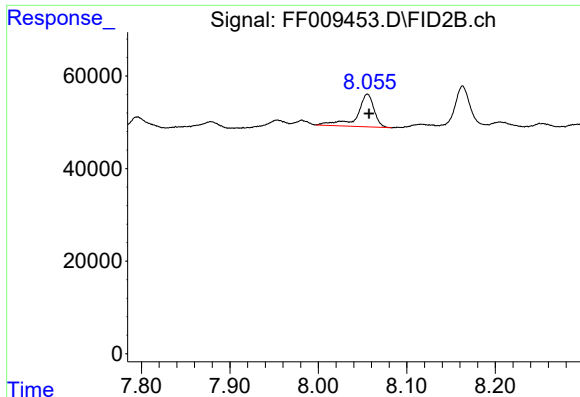

#4 N-TETRADECANE


R.T.: 8.055 min
Delta R.T.: -0.002 min
Response: 93249
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

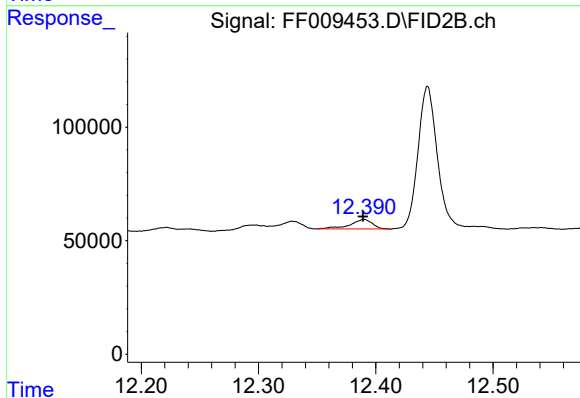


#7 N-EICOSANE

R.T.: 12.390 min
Delta R.T.: 0.000 min
Response: 56468
Conc: 0.40 ug/ml

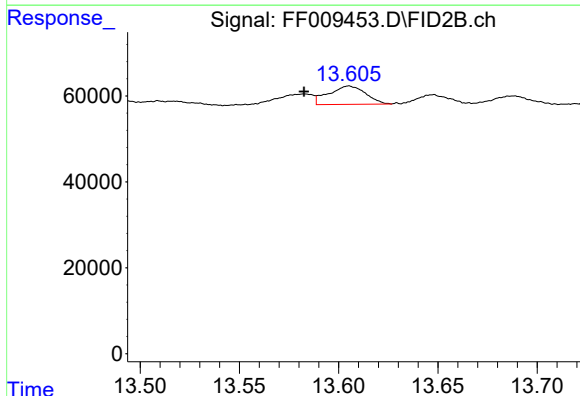


#8 N-DOCOSANE

R.T.: 13.605 min
Delta R.T.: 0.023 min
Response: 55096
Conc: 0.40 ug/ml

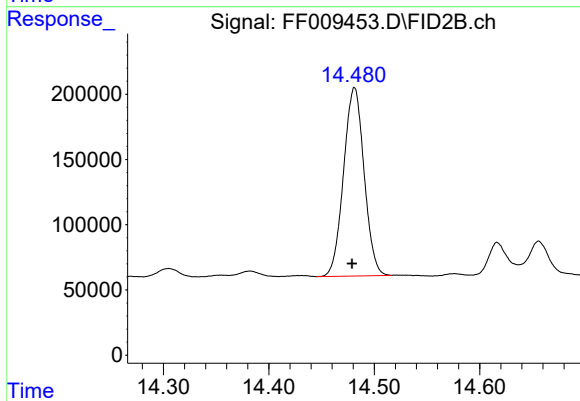

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.481 min
Delta R.T.: 0.002 min
Response: 1951497
Conc: 16.85 ug/ml

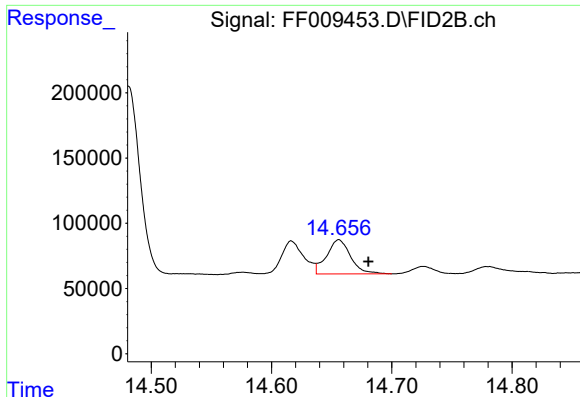

#10 N-TETRACOSANE


R.T.: 14.656 min
Delta R.T.: -0.025 min
Response: 365018
Conc: 2.77 ug/ml

Instrument :
FID_F
ClientSampleId :

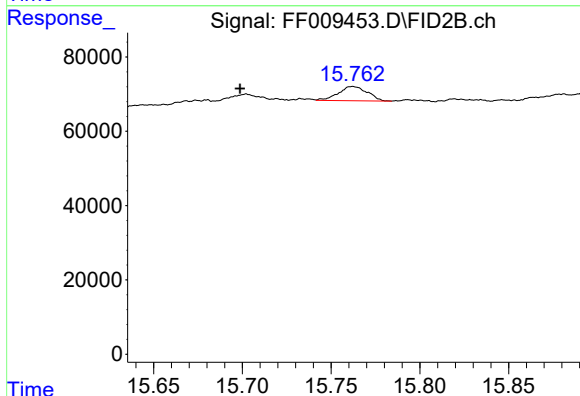


#11 N-HEXACOSANE

R.T.: 15.762 min
Delta R.T.: 0.064 min
Response: 43852
Conc: 0.35 ug/ml

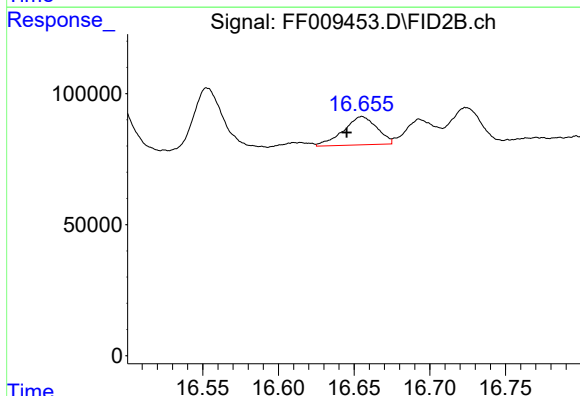


#12 N-OCTACOSANE

R.T.: 16.655 min
Delta R.T.: 0.010 min
Response: 165875
Conc: 1.39 ug/ml

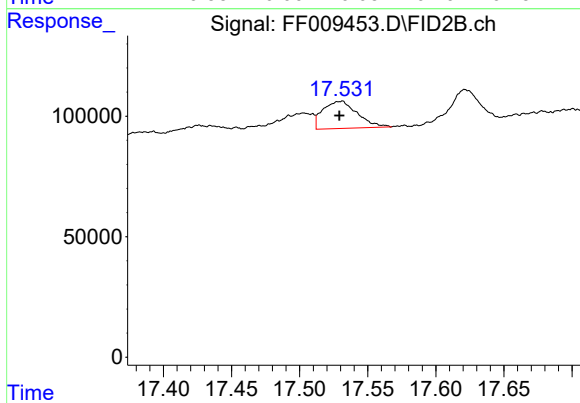

#13 N-TRIACONTANE


R.T.: 17.532 min
Delta R.T.: 0.002 min
Response: 199143
Conc: 1.74 ug/ml

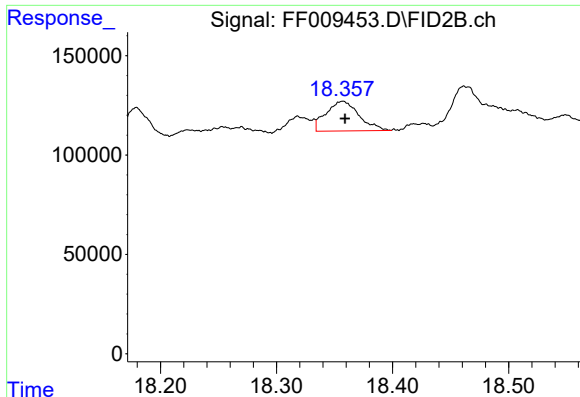

#14 N-DOTRIACONTANE


R.T.: 18.357 min
Delta R.T.: -0.002 min
Response: 294645
Conc: 2.70 ug/ml

Instrument :
FID_F
ClientSampleId :

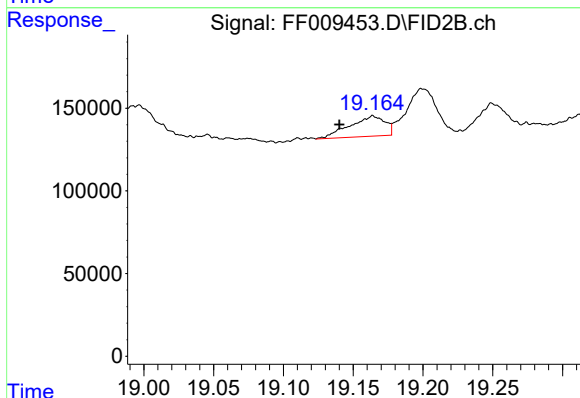


#15 N-TETRATRIACONTANE

R.T.: 19.164 min
Delta R.T.: 0.024 min
Response: 215674
Conc: 2.04 ug/ml

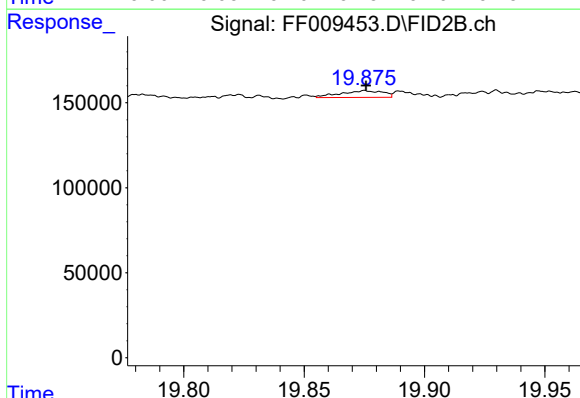


#16 N-HEXATRIACONTANE

R.T.: 19.875 min
Delta R.T.: 0.000 min
Response: 49026
Conc: 0.49 ug/ml

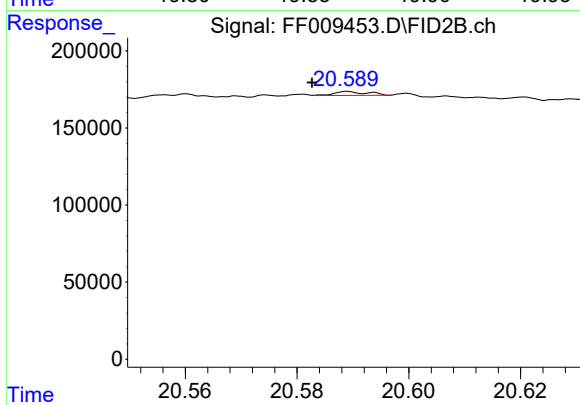

#17 N-OCTATRIACONTANE

R.T.: 20.589 min
Delta R.T.: 0.007 min
Response: 10319
Conc: 0.11 ug/ml

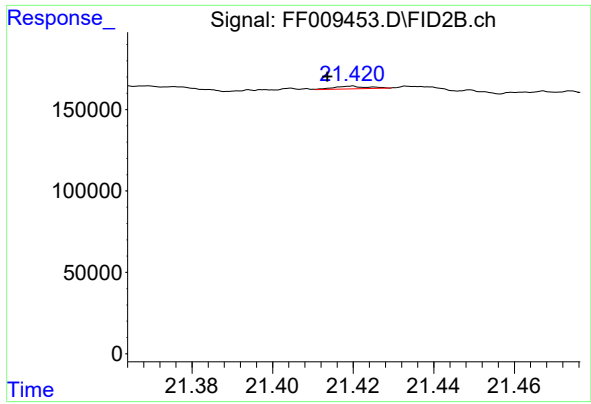

#18 N-TETRACONTANE

R.T.: 21.420 min
Delta R.T.: 0.006 min
Response: 9310
Conc: 0.09 ug/ml

Instrument :
FID_F
ClientSampleId :