

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
 Data File : FF009454.D
 Signal(s) : FID2B.ch
 Acq On : 16 Dec 2021 12:22
 Operator : AJ\MA
 Sample : M5074-04
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 14:28:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.482	1558692	13.456 ug/ml
Target Compounds			
4) N-TETRADECANE	8.056	62281	0.428 ug/ml
6) N-OCTADECANE	11.086	38262	0.265 ug/ml
7) N-EICOSANE	12.390	41690	0.294 ug/ml
10) N-TETRACOSANE	14.658	236285	1.795 ug/ml
11) N-HEXACOSANE	15.706	31631	0.253 ug/ml
12) N-OCTACOSANE	16.656	136506	1.146 ug/ml
13) N-TRIACONTANE	17.531	194498	1.698 ug/ml
14) N-DOTRIACONTANE	18.360	242626	2.220 ug/ml
15) N-TETRATRIACONTANE	19.141	31026	0.293 ug/ml
16) N-HEXATRIACONTANE	19.870	15093	0.151 ug/ml
17) N-OCTATRIACONTANE	20.593	42895	0.437 ug/ml
18) N-TETRACONTANE	21.439	94105	0.932 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009454.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 12:22
Operator : AJ\MA
Sample : M5074-04
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 14:28:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

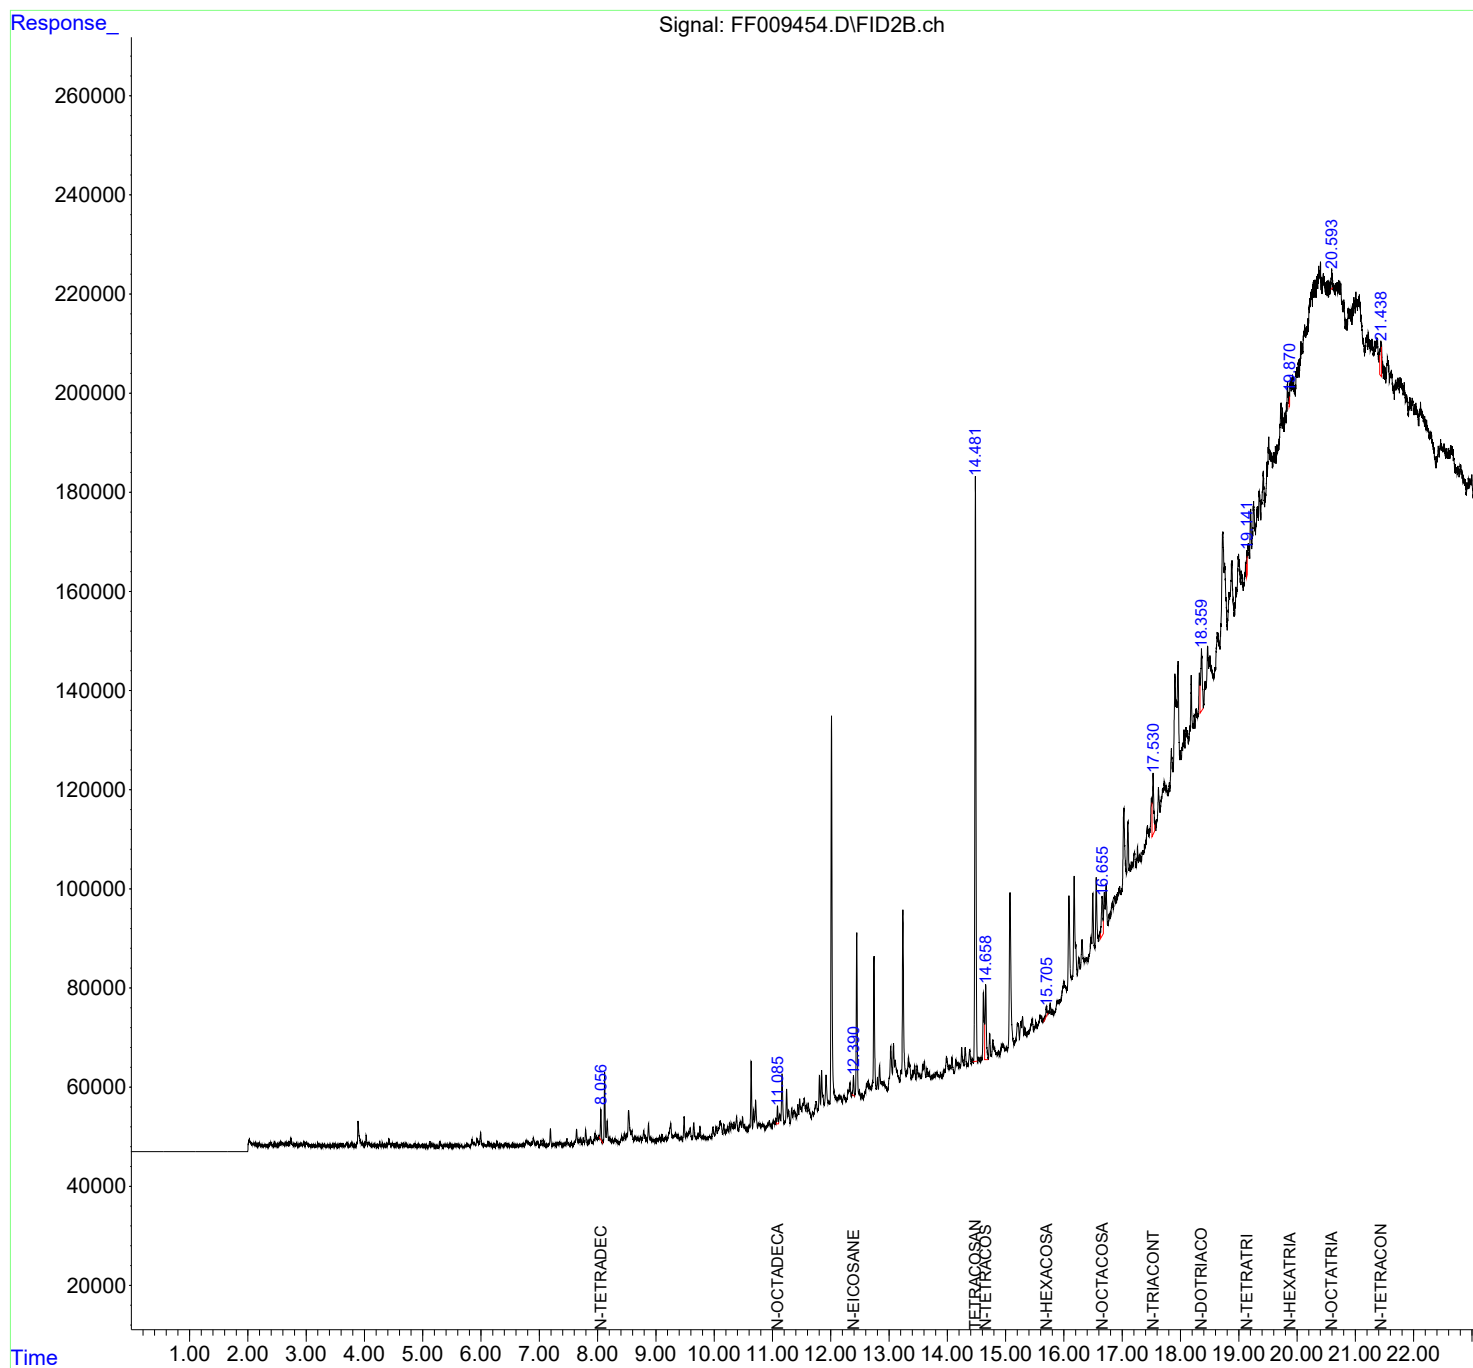


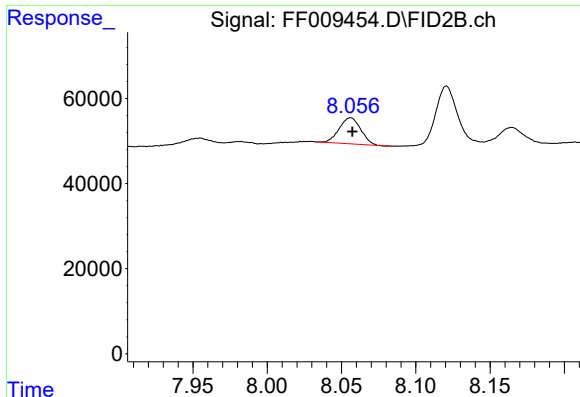

#4 N-TETRADECANE


R.T.: 8.056 min
Delta R.T.: -0.001 min
Response: 62281
Conc: 0.43 ug/ml

Instrument :
FID_F
ClientSampleId :

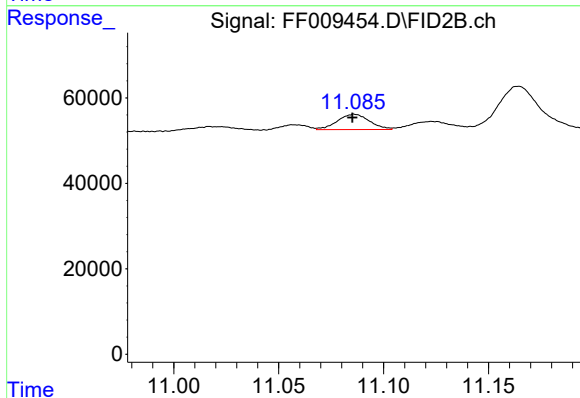


#6 N-OCTADECANE

R.T.: 11.086 min
Delta R.T.: 0.000 min
Response: 38262
Conc: 0.27 ug/ml

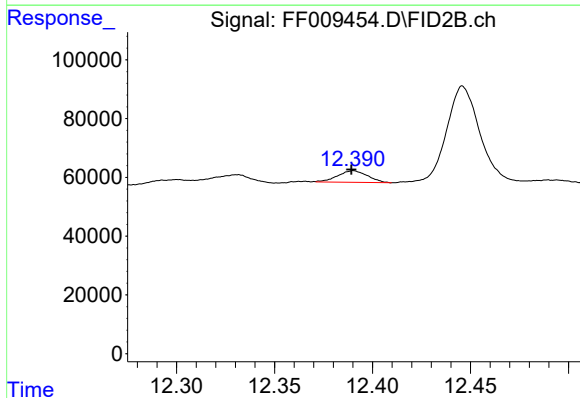


#7 N-EICOSANE

R.T.: 12.390 min
Delta R.T.: 0.001 min
Response: 41690
Conc: 0.29 ug/ml

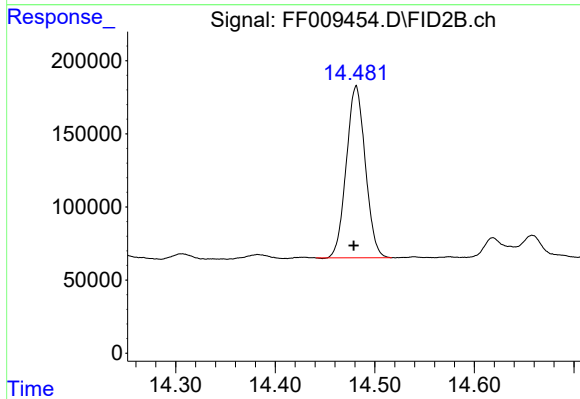

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.482 min
Delta R.T.: 0.002 min
Response: 1558692
Conc: 13.46 ug/ml

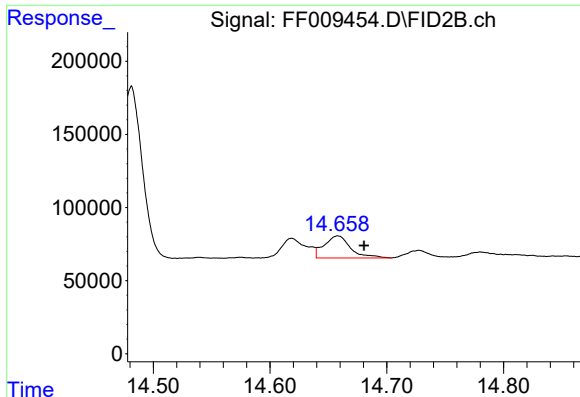

#10 N-TETRACOSANE


R.T.: 14.658 min
Delta R.T.: -0.023 min
Response: 236285
Conc: 1.79 ug/ml

Instrument :
FID_F
ClientSampleId :

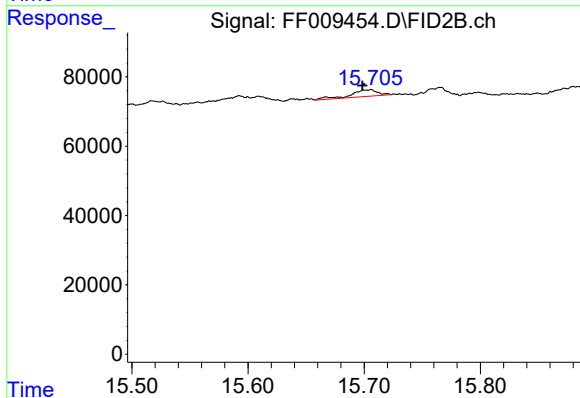


#11 N-HEXACOSANE

R.T.: 15.706 min
Delta R.T.: 0.007 min
Response: 31631
Conc: 0.25 ug/ml

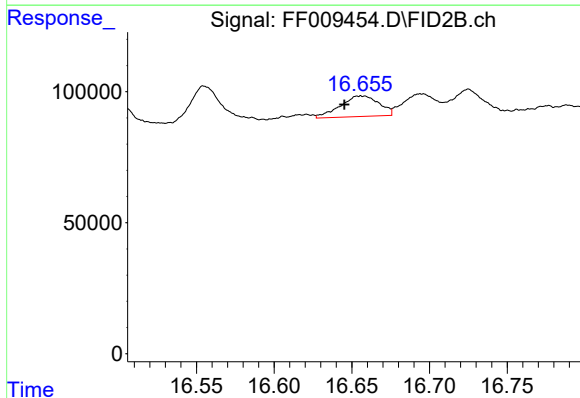


#12 N-OCTACOSANE

R.T.: 16.656 min
Delta R.T.: 0.011 min
Response: 136506
Conc: 1.15 ug/ml

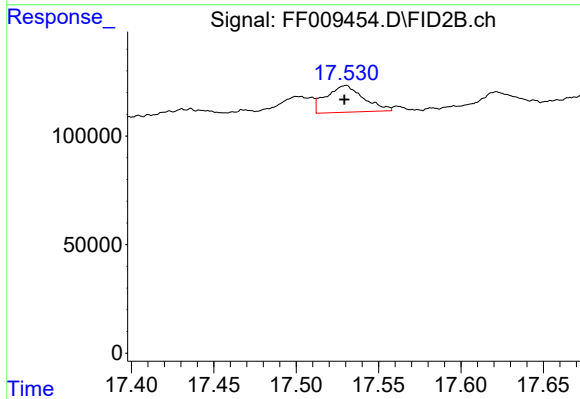

#13 N-TRIACONTANE


R.T.: 17.531 min
Delta R.T.: 0.001 min
Response: 194498
Conc: 1.70 ug/ml

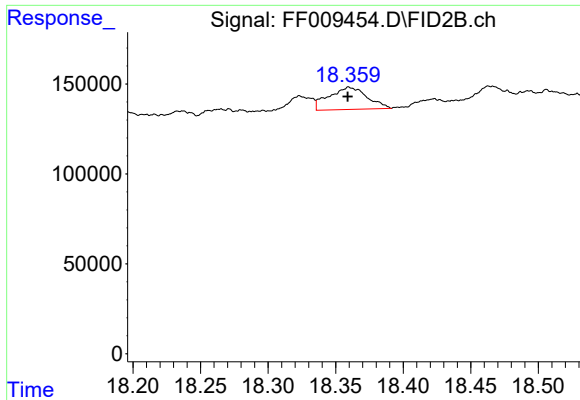

#14 N-DOTRIACONTANE


R.T.: 18.360 min
Delta R.T.: 0.000 min
Response: 242626
Conc: 2.22 ug/ml

Instrument :
FID_F
ClientSampleId :

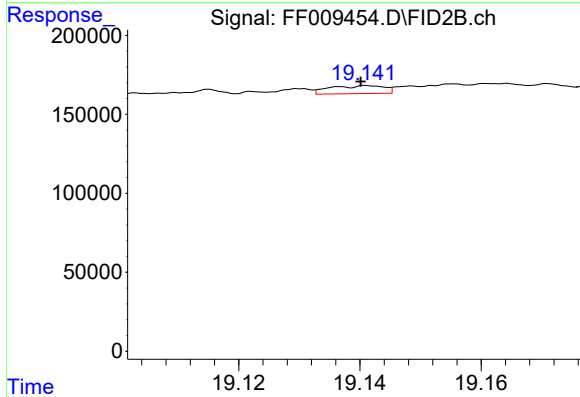


#15 N-TETRATRIACONTANE

R.T.: 19.141 min
Delta R.T.: 0.001 min
Response: 31026
Conc: 0.29 ug/ml

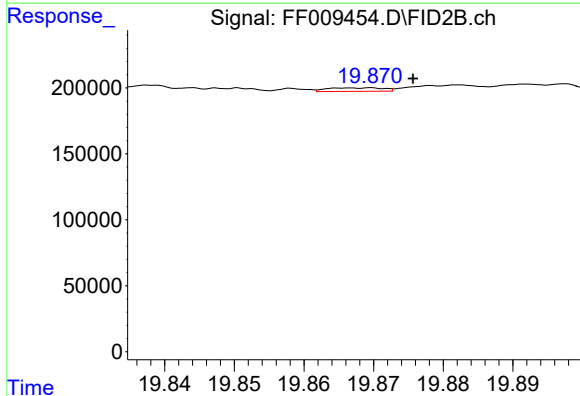


#16 N-HEXATRIACONTANE

R.T.: 19.870 min
Delta R.T.: -0.006 min
Response: 15093
Conc: 0.15 ug/ml

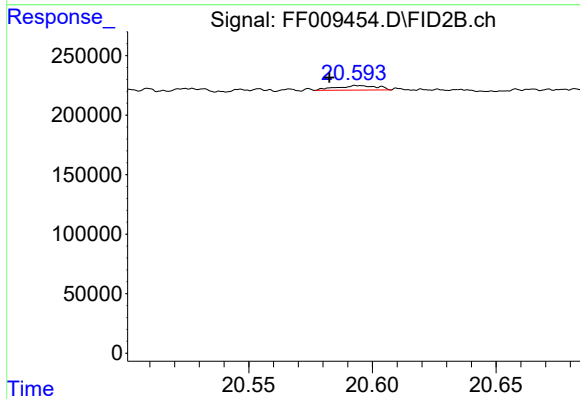

#17 N-OCTATRIACONTANE

R.T.: 20.593 min
Delta R.T.: 0.011 min
Response: 42895
Conc: 0.44 ug/ml

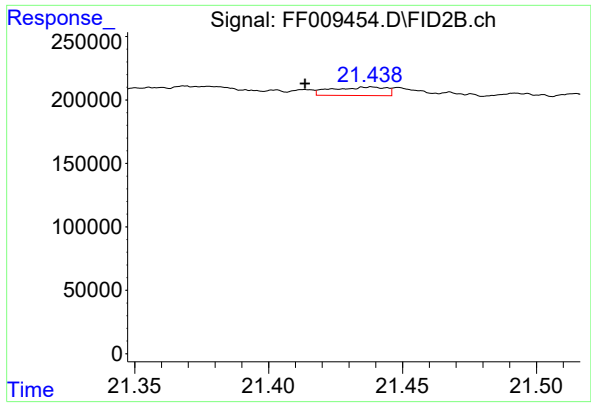

#18 N-TETRACONTANE

R.T.: 21.439 min
Delta R.T.: 0.025 min
Response: 94105
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :