

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
 Data File : FF009458.D
 Signal(s) : FID2B.ch
 Acq On : 16 Dec 2021 14:25
 Operator : AJ\MA
 Sample : PB141445BL
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 17 00:59:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.482	2791330	24.096 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.533	53635	0.468 ug/ml
14) N-DOTRIACONTANE	18.360	77063	0.705 ug/ml
15) N-TETRATRIACONTANE	19.141	77128	0.728 ug/ml
16) N-HEXATRIACONTANE	19.879	50908	0.508 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009458.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 14:25
Operator : AJ\MA
Sample : PB141445BL
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 17 00:59:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

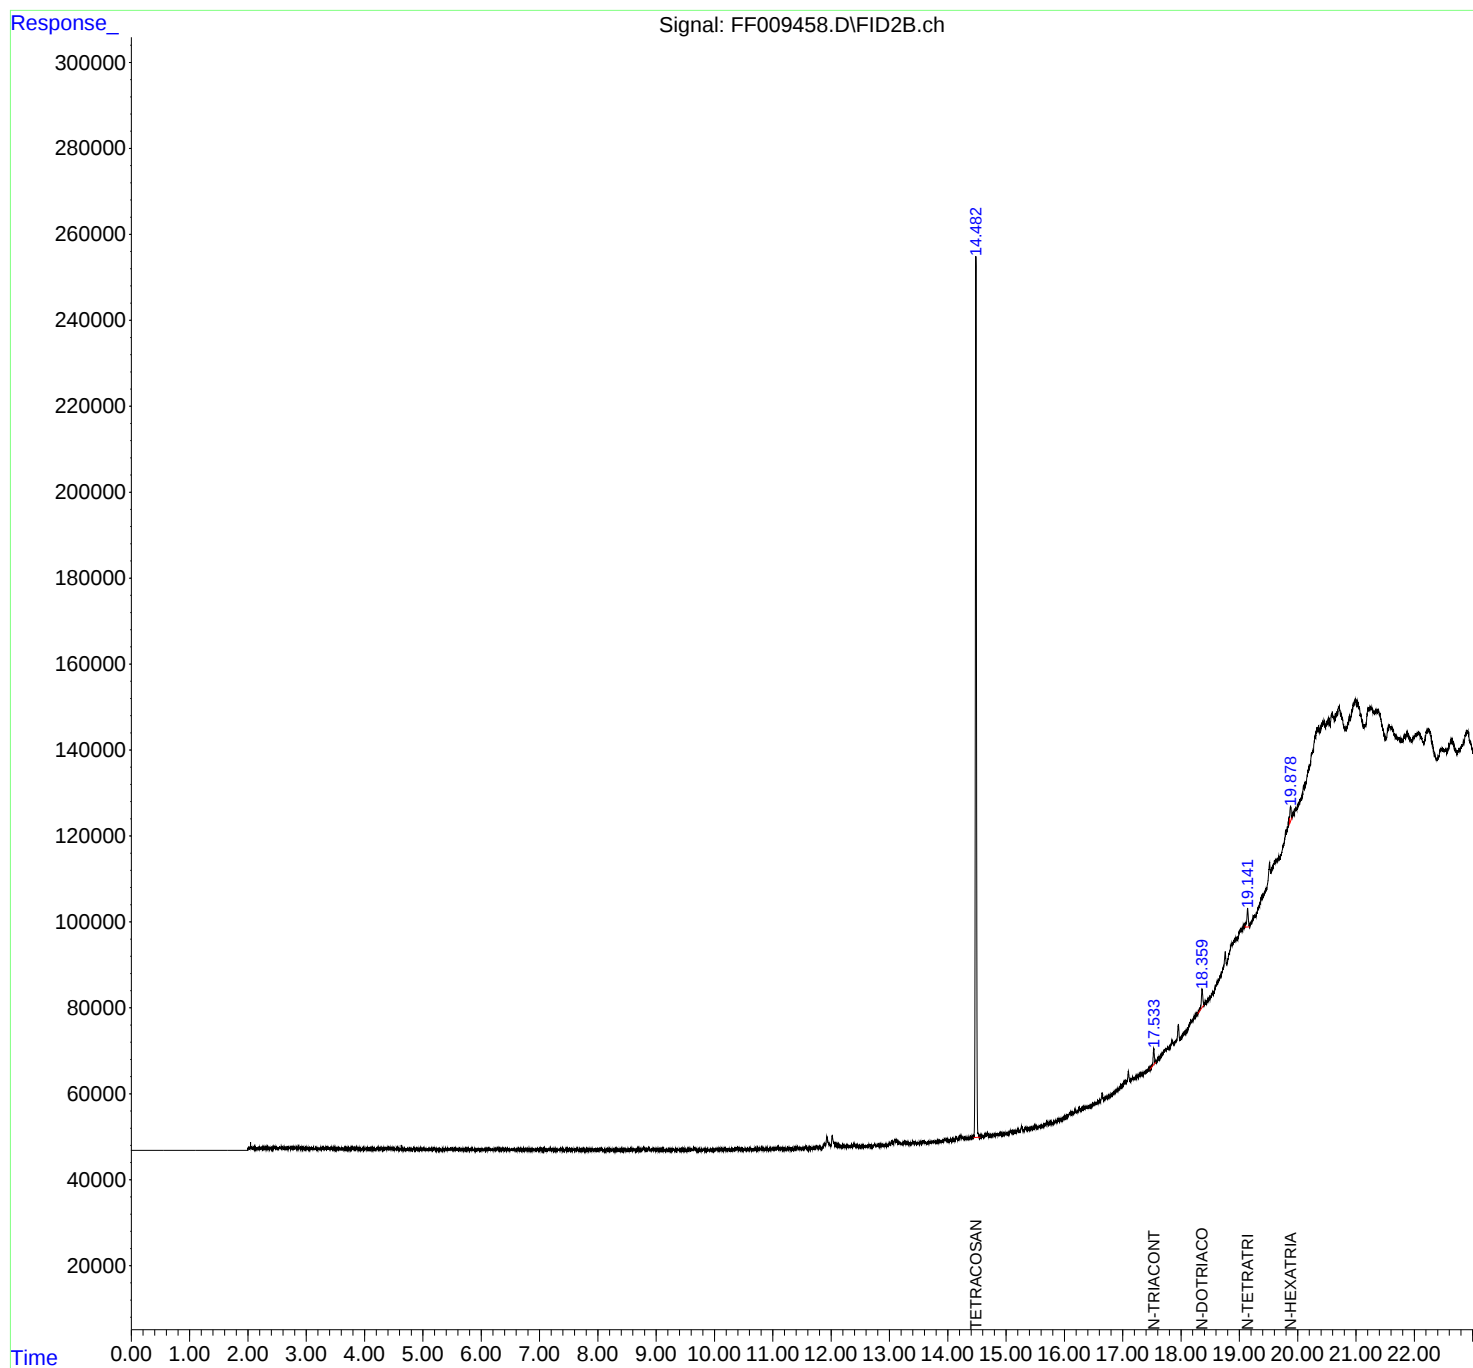


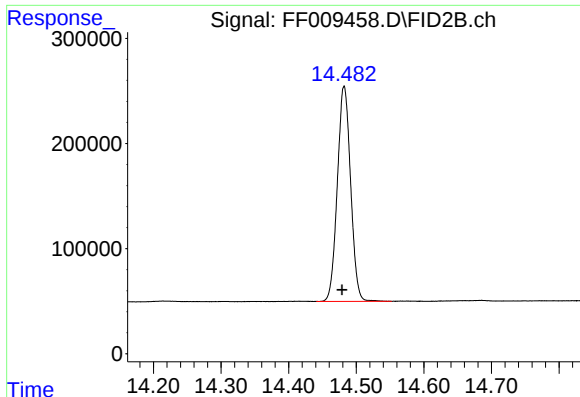

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.482 min
Delta R.T.: 0.003 min
Response: 2791330
Conc: 24.10 ug/ml

Instrument :
FID_F
ClientSampleId :

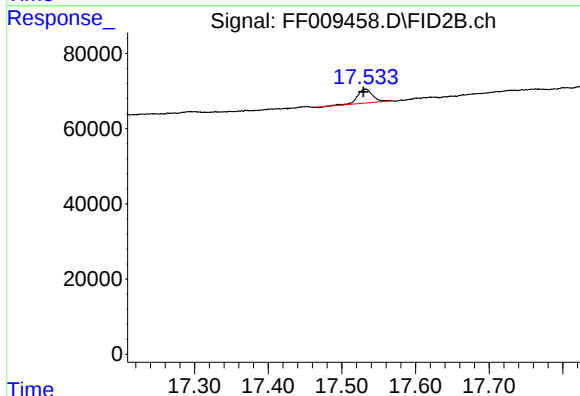


#13 N-TRIACONTANE

R.T.: 17.533 min
Delta R.T.: 0.004 min
Response: 53635
Conc: 0.47 ug/ml

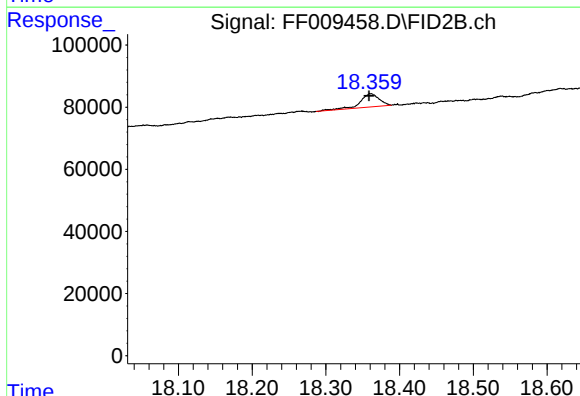


#14 N-DOTRIACONTANE

R.T.: 18.360 min
Delta R.T.: 0.000 min
Response: 77063
Conc: 0.71 ug/ml

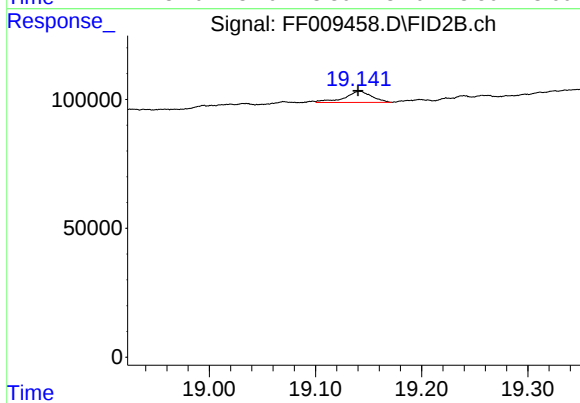

#15 N-TETRATRIACONTANE

R.T.: 19.141 min
Delta R.T.: 0.001 min
Response: 77128
Conc: 0.73 ug/ml

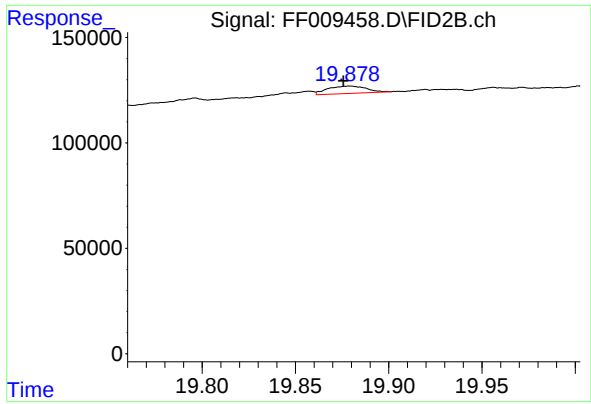

#16 N-HEXATRIACONTANE

R.T.: 19.879 min
Delta R.T.: 0.003 min
Response: 50908
Conc: 0.51 ug/ml

Instrument :

FID_F

ClientSampleId :