

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009461.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 15:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 17 01:00:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.480	2089829	18.041 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.360	27610	0.253 ug/ml
16) N-HEXATRIACONTANE	19.884	18786	0.188 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009461.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 15:58
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 17 01:00:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

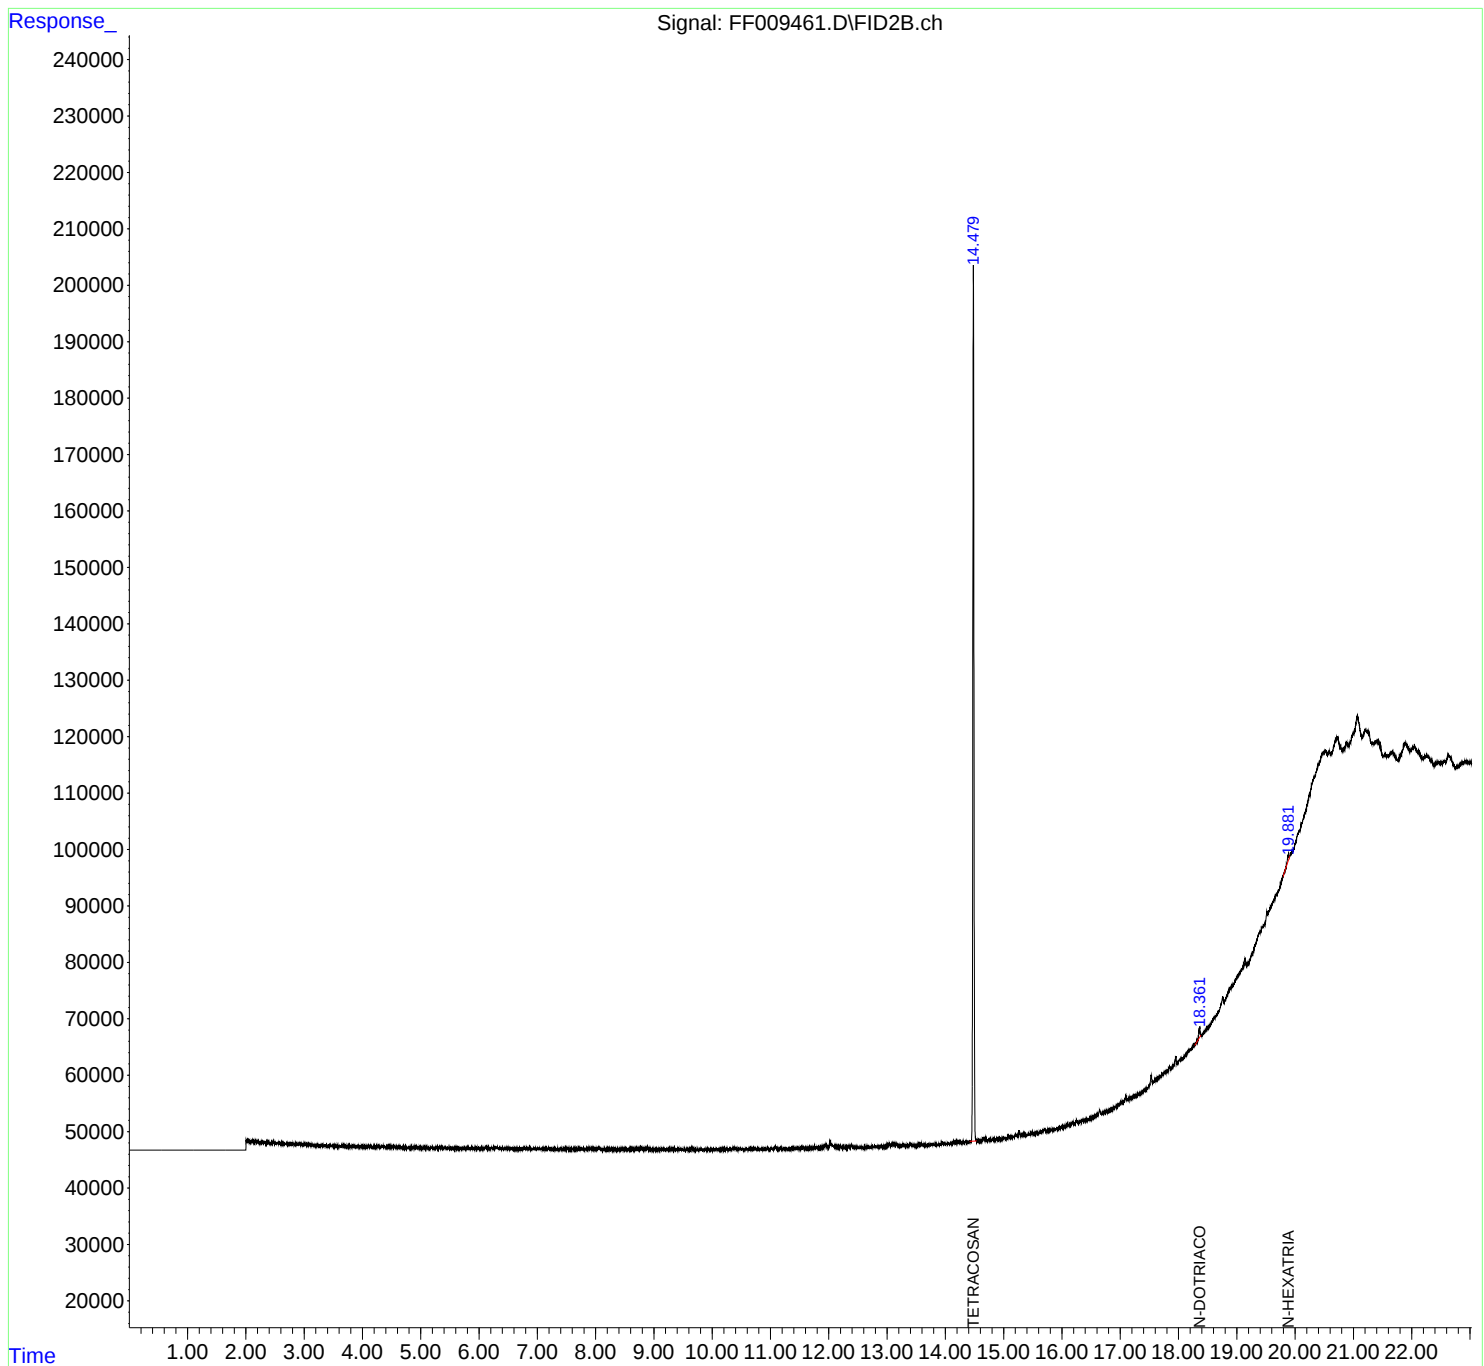


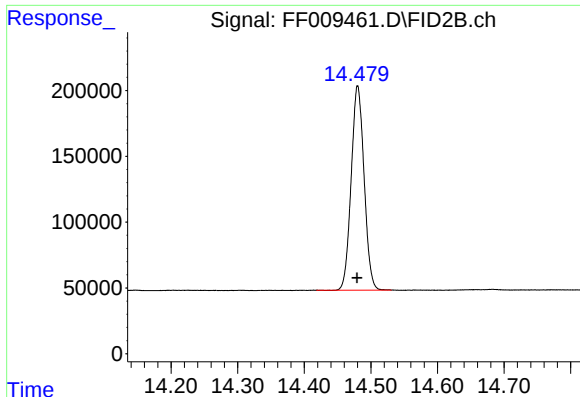

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.480 min
Delta R.T.: 0.001 min
Response: 2089829
Conc: 18.04 ug/ml

Instrument :
FID_F
ClientSampleId :

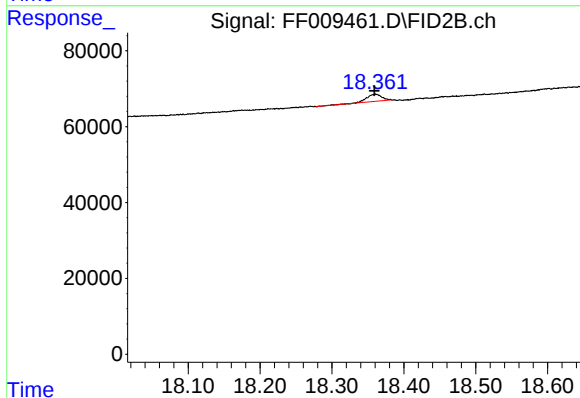

#14 N-DOTRIACONTANE

R.T.: 18.360 min
Delta R.T.: 0.001 min
Response: 27610
Conc: 0.25 ug/ml

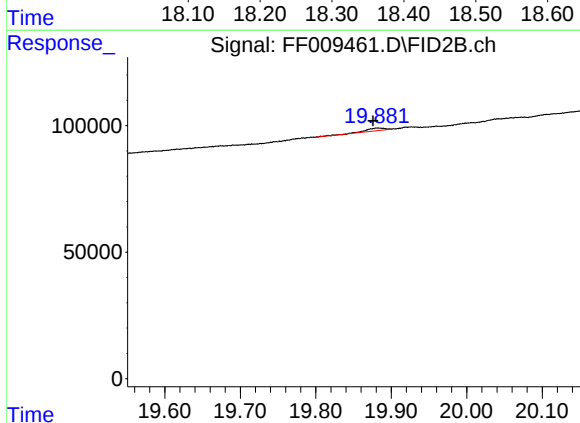

#16 N-HEXATRIACONTANE

R.T.: 19.884 min
Delta R.T.: 0.008 min
Response: 18786
Conc: 0.19 ug/ml