

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
 Data File : FF009467.D
 Signal(s) : FID2B.ch
 Acq On : 16 Dec 2021 19:03
 Operator : AJ\MA
 Sample : M5064-04
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 17 01:02:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.479	1212230	10.465 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.644	56832	0.477 ug/ml
13) N-TRIACONTANE	17.527	76009	0.664 ug/ml
14) N-DOTRIACONTANE	18.359	193516	1.771 ug/ml
15) N-TETRATRIACONTANE	19.139	60449	0.571 ug/ml
16) N-HEXATRIACONTANE	19.876	56818	0.567 ug/ml
18) N-TETRACONTANE	21.449	544978	5.396 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009467.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 19:03
Operator : AJ\MA
Sample : M5064-04
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 17 01:02:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

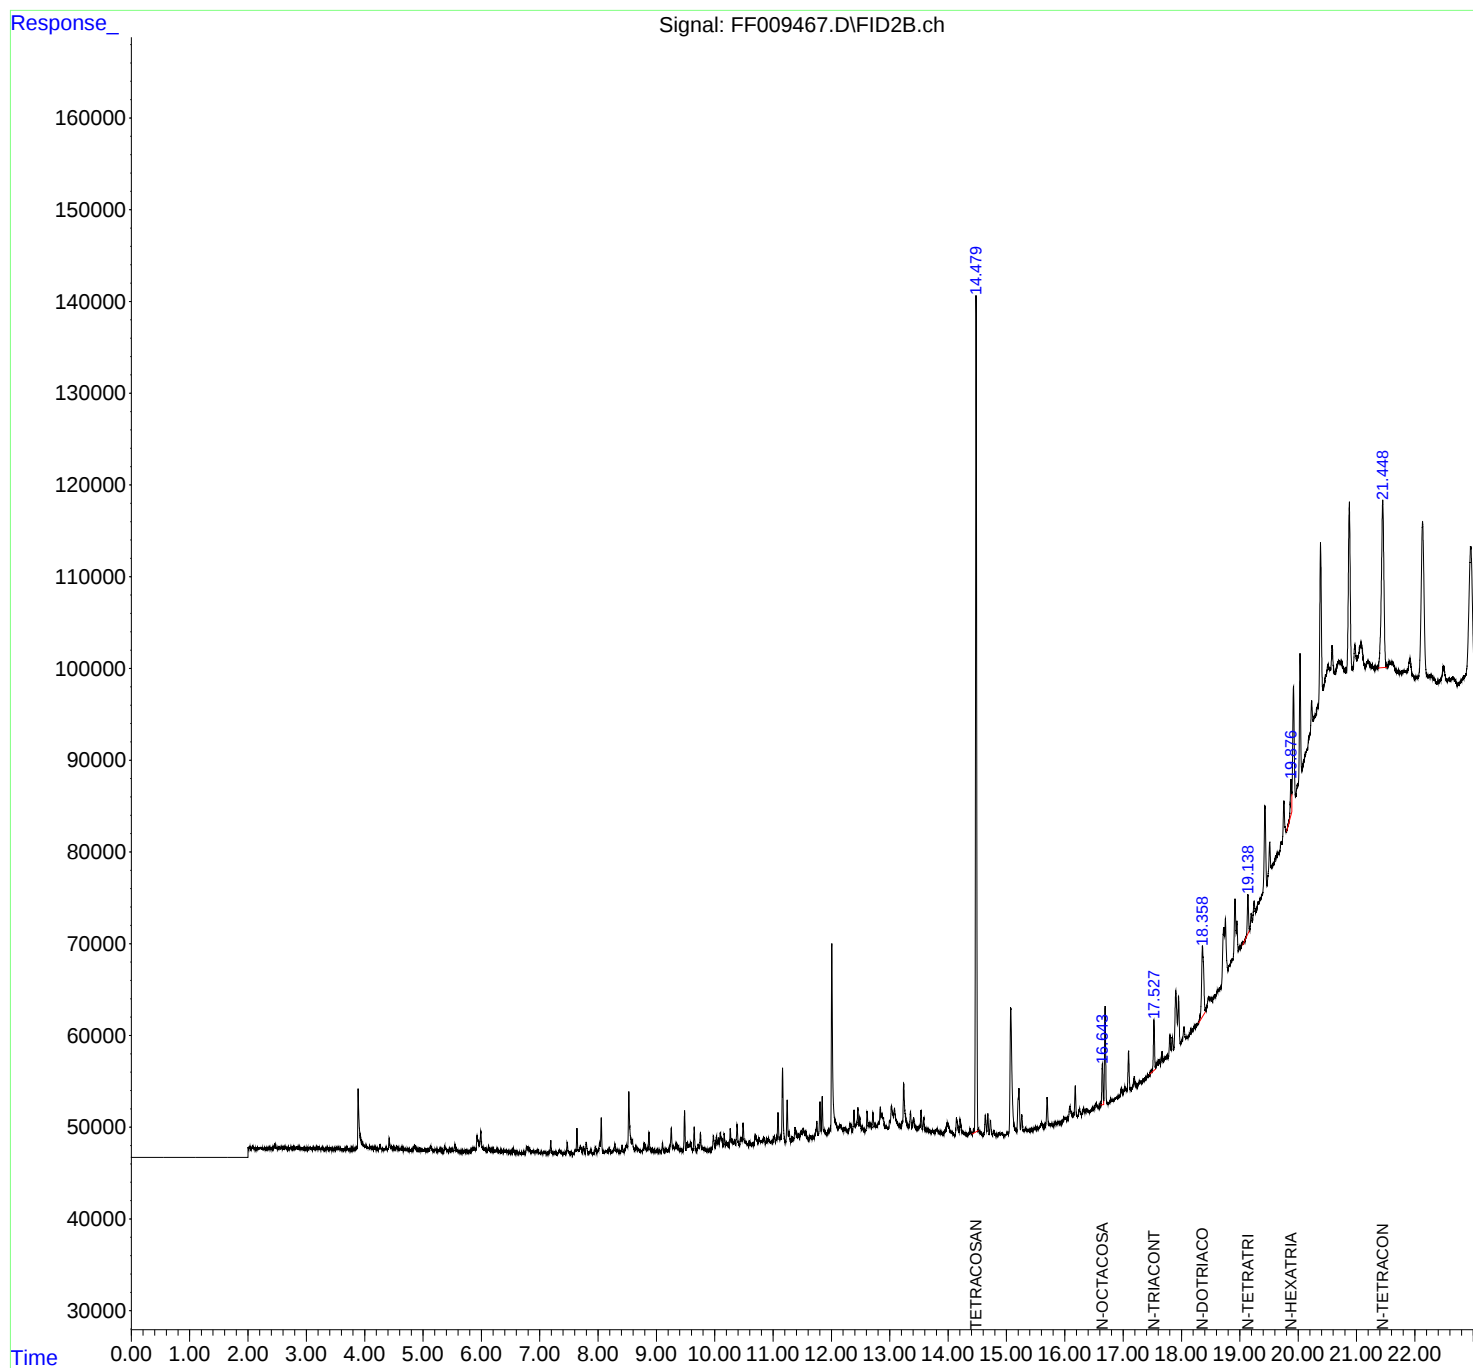


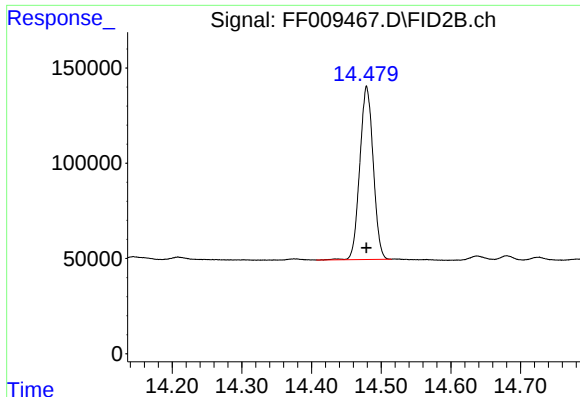

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.479 min
Delta R.T.: 0.000 min
Response: 1212230
Conc: 10.46 ug/ml

Instrument :
FID_F
ClientSampleId :

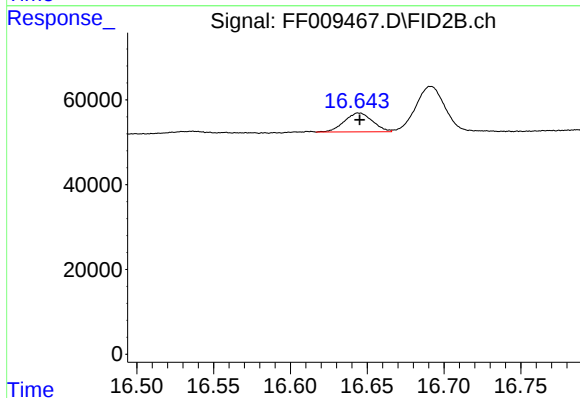


#12 N-OCTACOSANE

R.T.: 16.644 min
Delta R.T.: -0.001 min
Response: 56832
Conc: 0.48 ug/ml

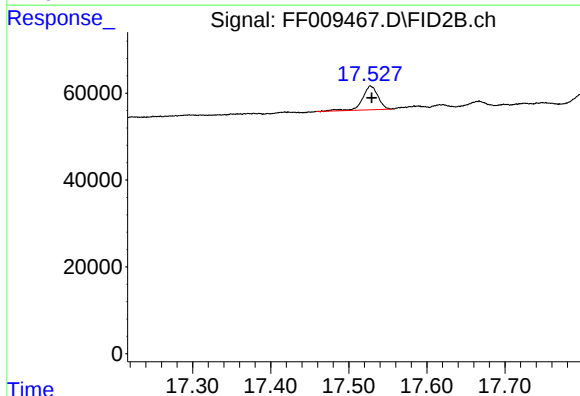


#13 N-TRIACONTANE

R.T.: 17.527 min
Delta R.T.: -0.002 min
Response: 76009
Conc: 0.66 ug/ml

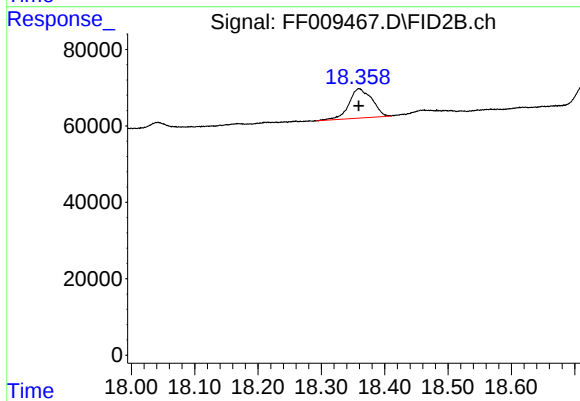

#14 N-DOTRIACONTANE


R.T.: 18.359 min
Delta R.T.: 0.000 min
Response: 193516
Conc: 1.77 ug/ml

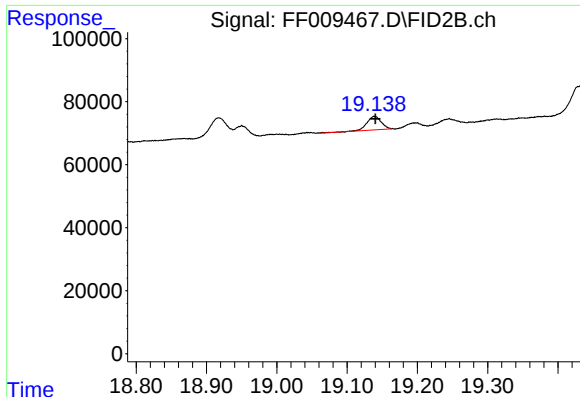

#15 N-TETRATRIACONTANE


R.T.: 19.139 min
Delta R.T.: -0.002 min
Response: 60449
Conc: 0.57 ug/ml

Instrument :
FID_F
ClientSampleId :

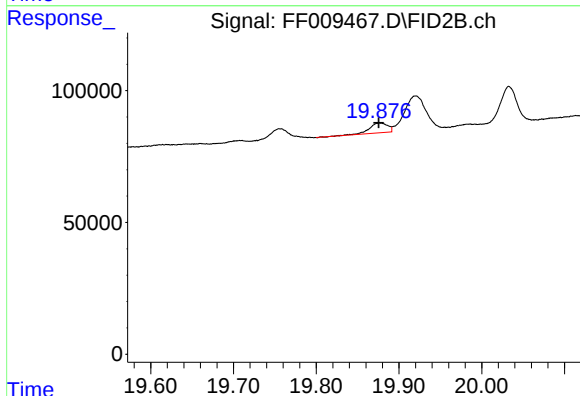

#16 N-HEXATRIACONTANE

R.T.: 19.876 min
Delta R.T.: 0.000 min
Response: 56818
Conc: 0.57 ug/ml

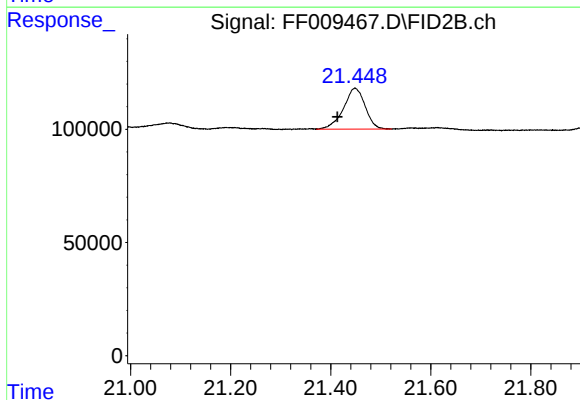

#18 N-TETRACONTANE

R.T.: 21.449 min
Delta R.T.: 0.035 min
Response: 544978
Conc: 5.40 ug/ml