

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
 Data File : FF009464.D
 Signal(s) : FID2B.ch
 Acq On : 16 Dec 2021 17:31
 Operator : AJ\MA
 Sample : M5064-02MS
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SASP2-121-1-(5-10)MS

Integration File: Sample.e
 Quant Time: Dec 17 01:01:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.480	2048276	17.682 ug/ml
Target Compounds			
2) N-DECANE	4.262	2796023	19.611 ug/ml
3) N-DODECANE	6.270	2844901	19.672 ug/ml
4) N-TETRADECANE	8.057	2929117	20.146 ug/ml
5) N-HEXADECANE	9.650	2753234	19.170 ug/ml
6) N-OCTADECANE	11.086	2834826	19.641 ug/ml
7) N-EICOSANE	12.391	2752324	19.421 ug/ml
8) N-DOCOSANE	13.585	2615137	19.192 ug/ml
10) N-TETRACOSANE	14.683	2493199	18.935 ug/ml
11) N-HEXACOSANE	15.700	2382388	19.062 ug/ml
12) N-OCTACOSANE	16.646	2325062	19.526 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009464.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 17:31
Operator : AJ\MA
Sample : M5064-02MS
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-121-1-(5-10)MS

Integration File: Sample.e
Quant Time: Dec 17 01:01:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

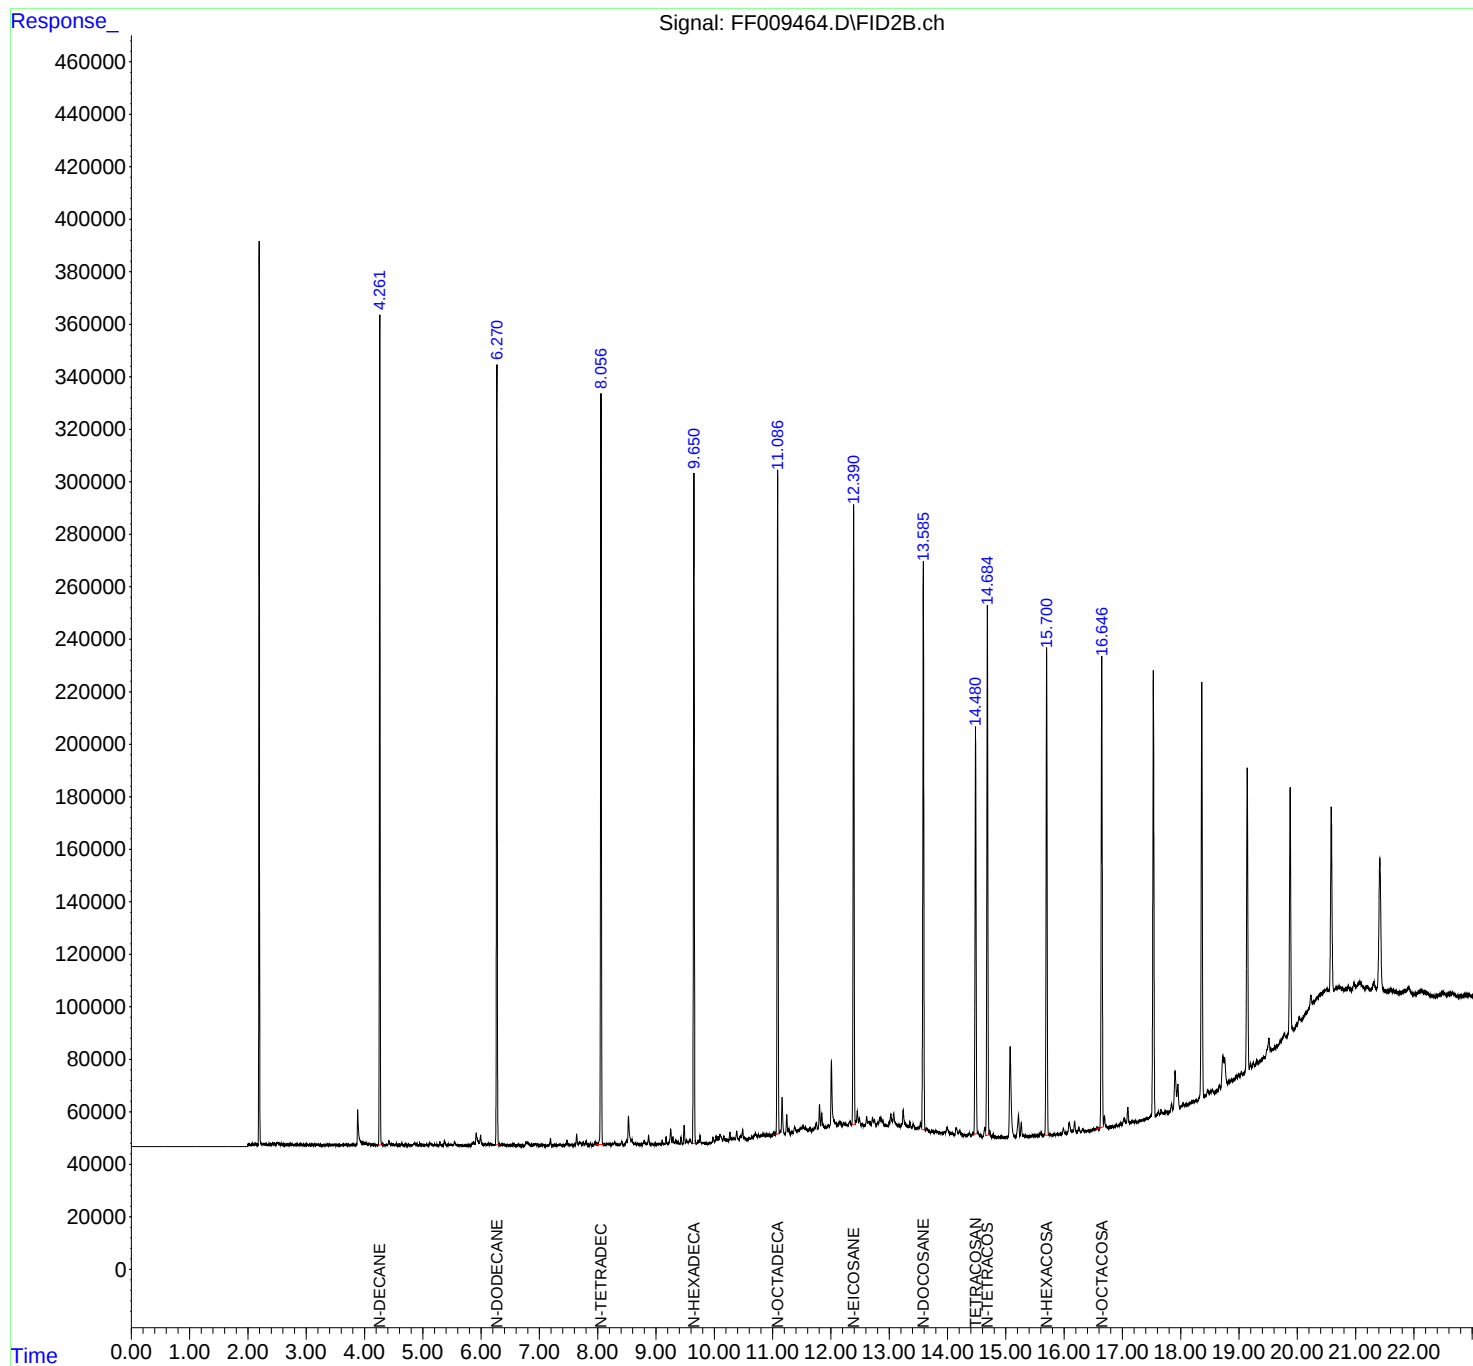


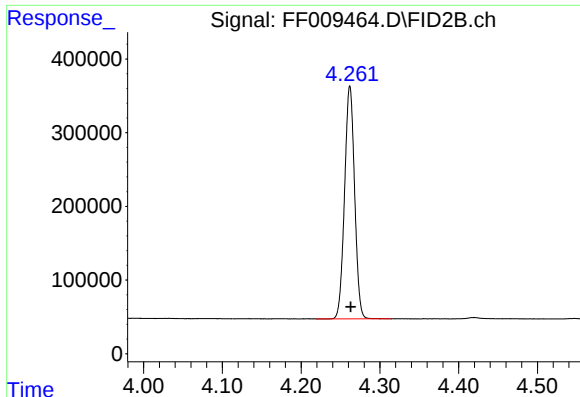

#2 N-DECANE


R.T.: 4.262 min
Delta R.T.: -0.001 min
Response: 2796023
Conc: 19.61 ug/ml

Instrument :
FID_F
ClientSampleId :
SASP2-121-1-(5-10)MS

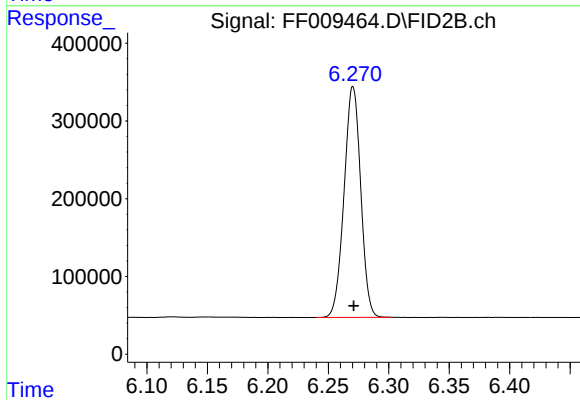


#3 N-DODECANE

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 2844901
Conc: 19.67 ug/ml

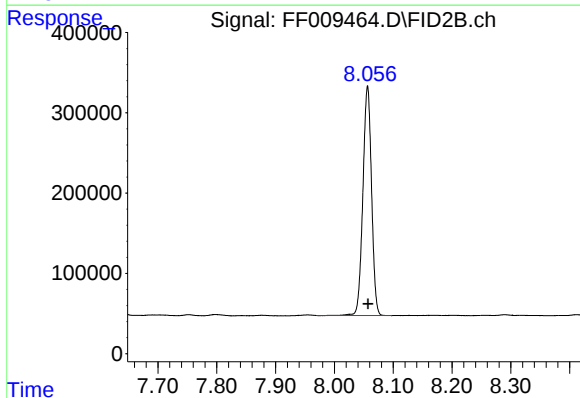


#4 N-TETRADECANE

R.T.: 8.057 min
Delta R.T.: 0.000 min
Response: 2929117
Conc: 20.15 ug/ml

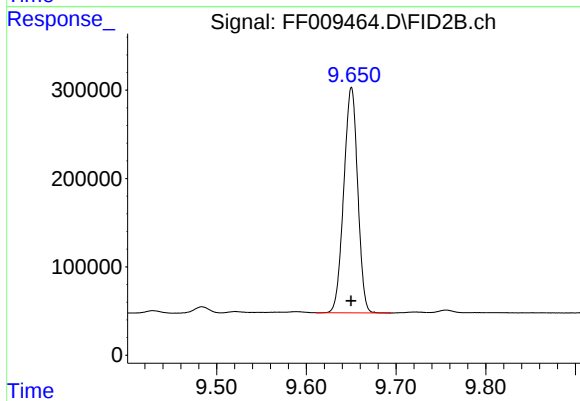

#5 N-HEXADECANE


R.T.: 9.650 min
Delta R.T.: 0.000 min
Response: 2753234
Conc: 19.17 ug/ml

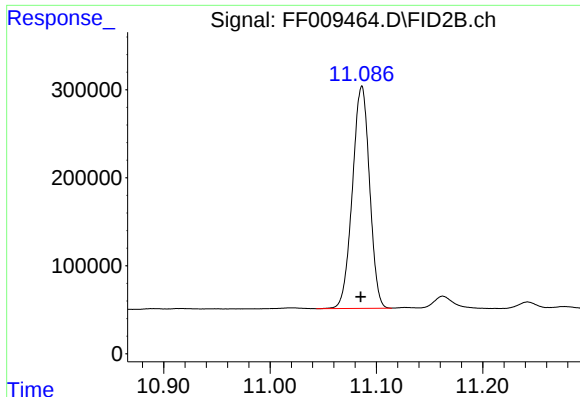

#6 N-OCTADECANE


R.T.: 11.086 min
Delta R.T.: 0.001 min
Response: 2834826
Conc: 19.64 ug/ml

Instrument :
FID_F
ClientSampleId :
SASP2-121-1-(5-10)MS

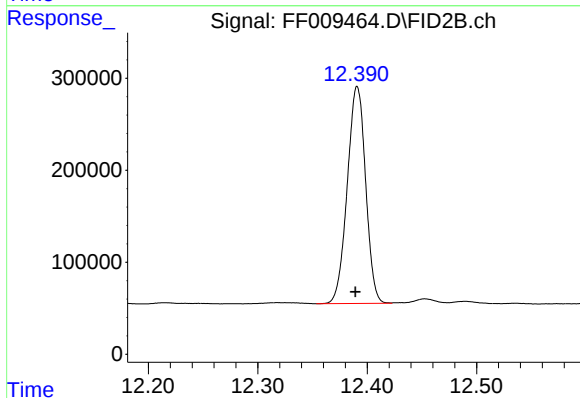


#7 N-EICOSANE

R.T.: 12.391 min
Delta R.T.: 0.002 min
Response: 2752324
Conc: 19.42 ug/ml

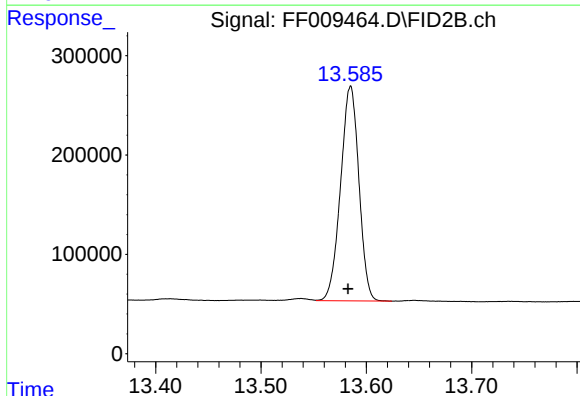


#8 N-DOCOSANE

R.T.: 13.585 min
Delta R.T.: 0.003 min
Response: 2615137
Conc: 19.19 ug/ml

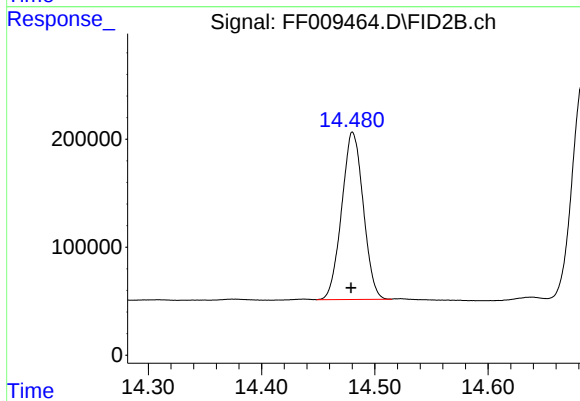

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.480 min
Delta R.T.: 0.001 min
Response: 2048276
Conc: 17.68 ug/ml

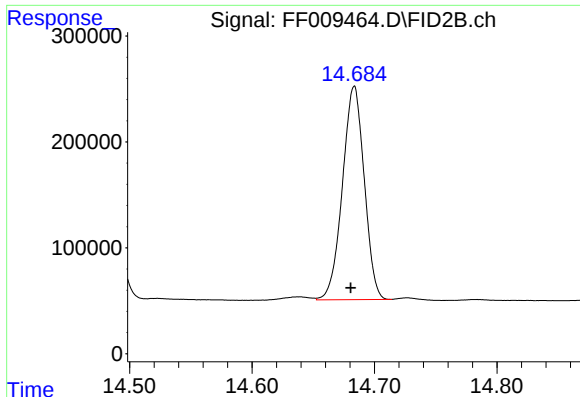

#10 N-TETRACOSANE


R.T.: 14.683 min
Delta R.T.: 0.003 min
Response: 2493199
Conc: 18.94 ug/ml

Instrument :
FID_F
ClientSampleId :
SASP2-121-1-(5-10)MS

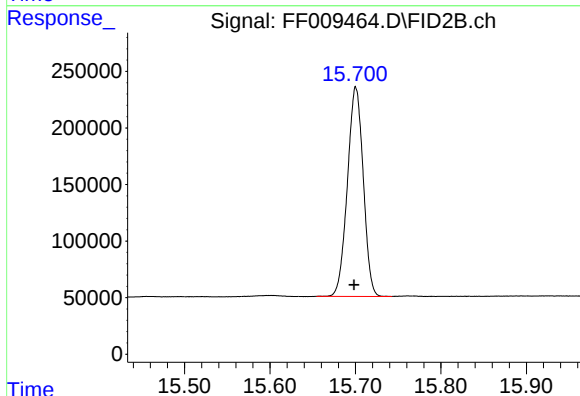

#11 N-HEXACOSANE

R.T.: 15.700 min
Delta R.T.: 0.002 min
Response: 2382388
Conc: 19.06 ug/ml

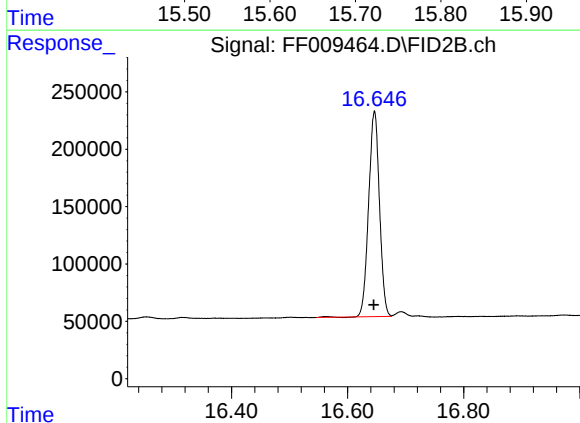

#12 N-OCTACOSANE

R.T.: 16.646 min
Delta R.T.: 0.001 min
Response: 2325062
Conc: 19.53 ug/ml