

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009467.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 19:03
Operator : AJ\MA
Sample : M5064-04
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-121-1-(17-32)

Integration File: Sample.e
Quant Time: Dec 17 01:02:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.479	1212230	10.465 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009467.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 19:03
Operator : AJ\MA
Sample : M5064-04
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-121-1-(17-32)

Integration File: Sample.e
Quant Time: Dec 17 01:02:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

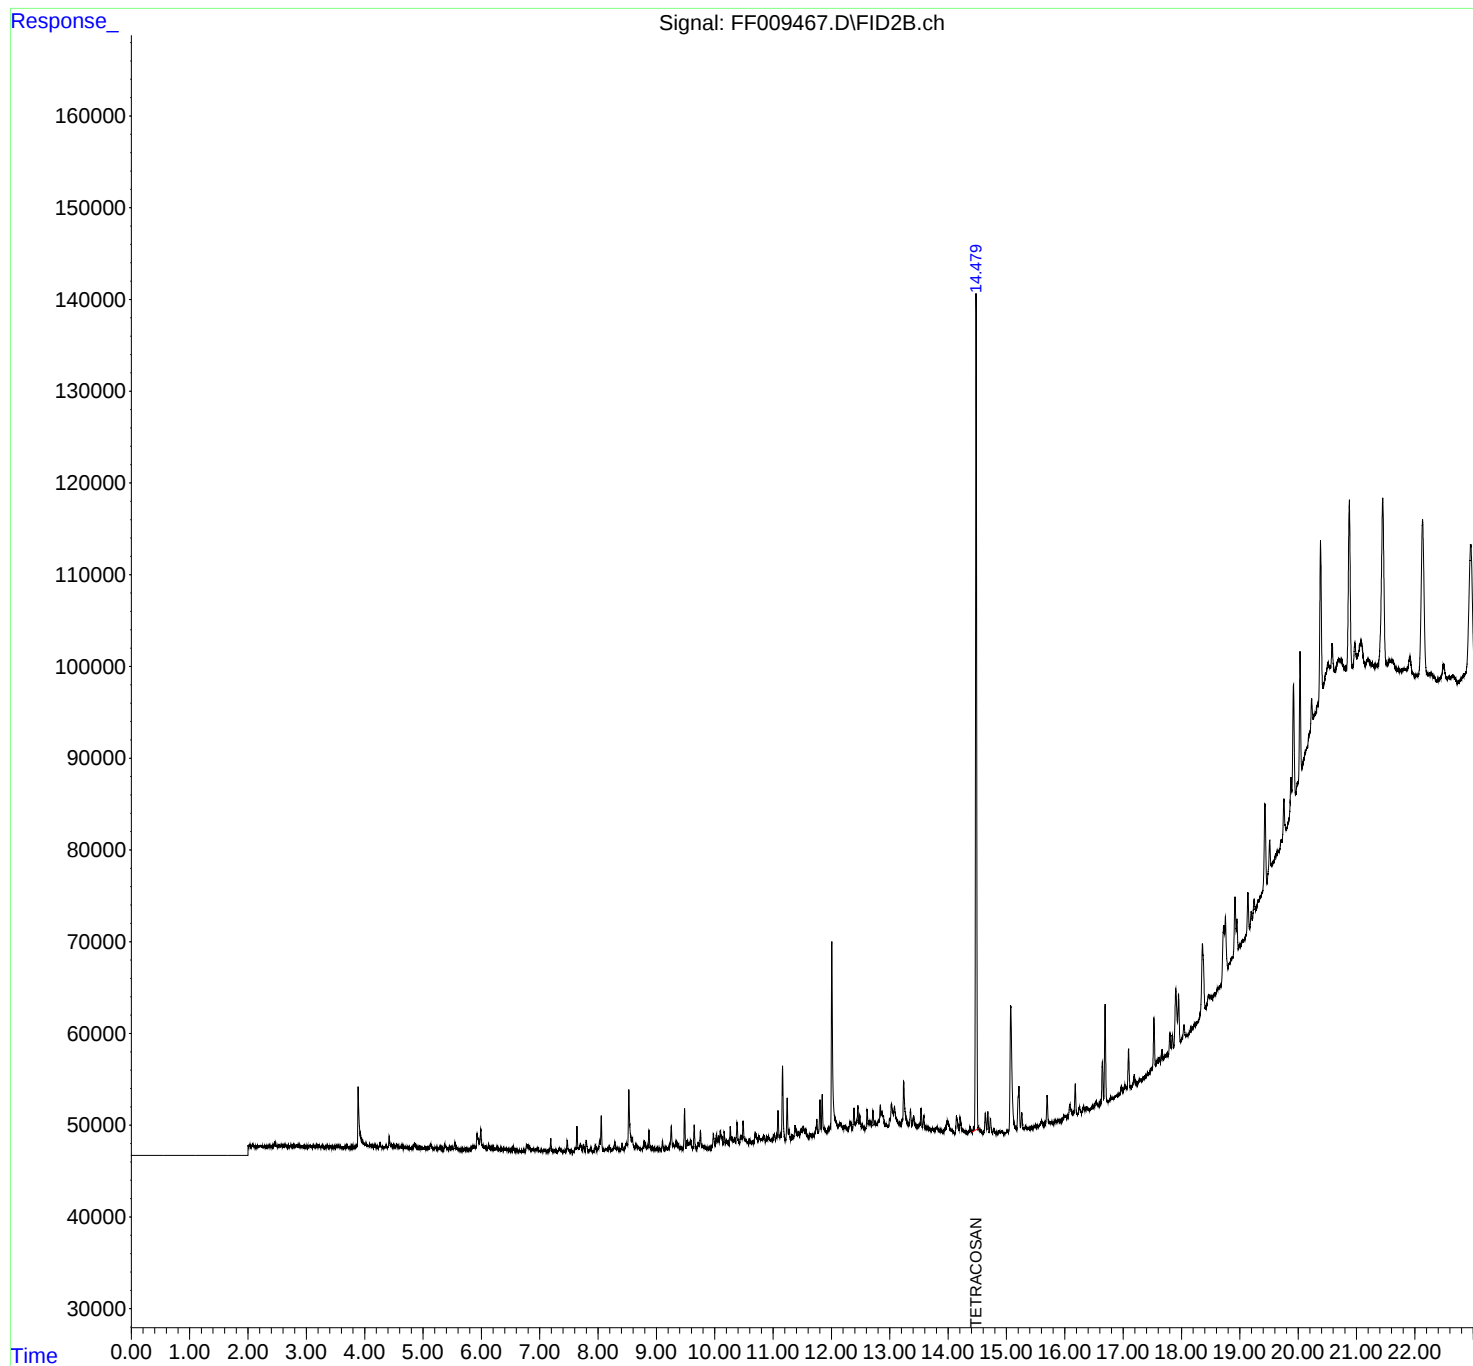

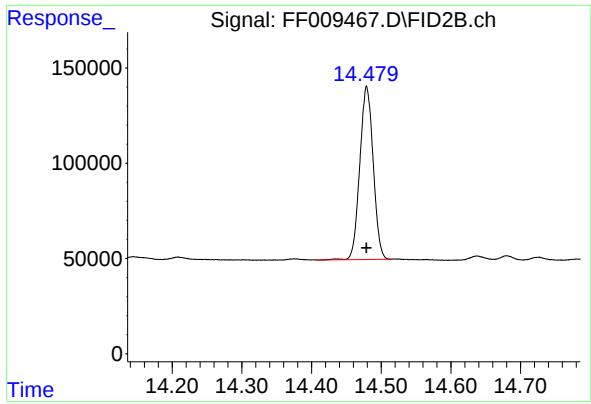

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.479 min
Delta R.T.: 0.000 min
Response: 1212230
Conc: 10.46 ug/ml

Instrument :
FID_F
ClientSampleId :
SASP2-121-1-(17-32)