

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009472.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 21:36
Operator : AJ\MA
Sample : M5082-03
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-121-1(65-77.7)

Integration File: Sample.e
Quant Time: Dec 17 01:03:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.477	1912326	16.508 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121621\
Data File : FF009472.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2021 21:36
Operator : AJ\MA
Sample : M5082-03
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SASP2-121-1(65-77.7)

Integration File: Sample.e
Quant Time: Dec 17 01:03:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

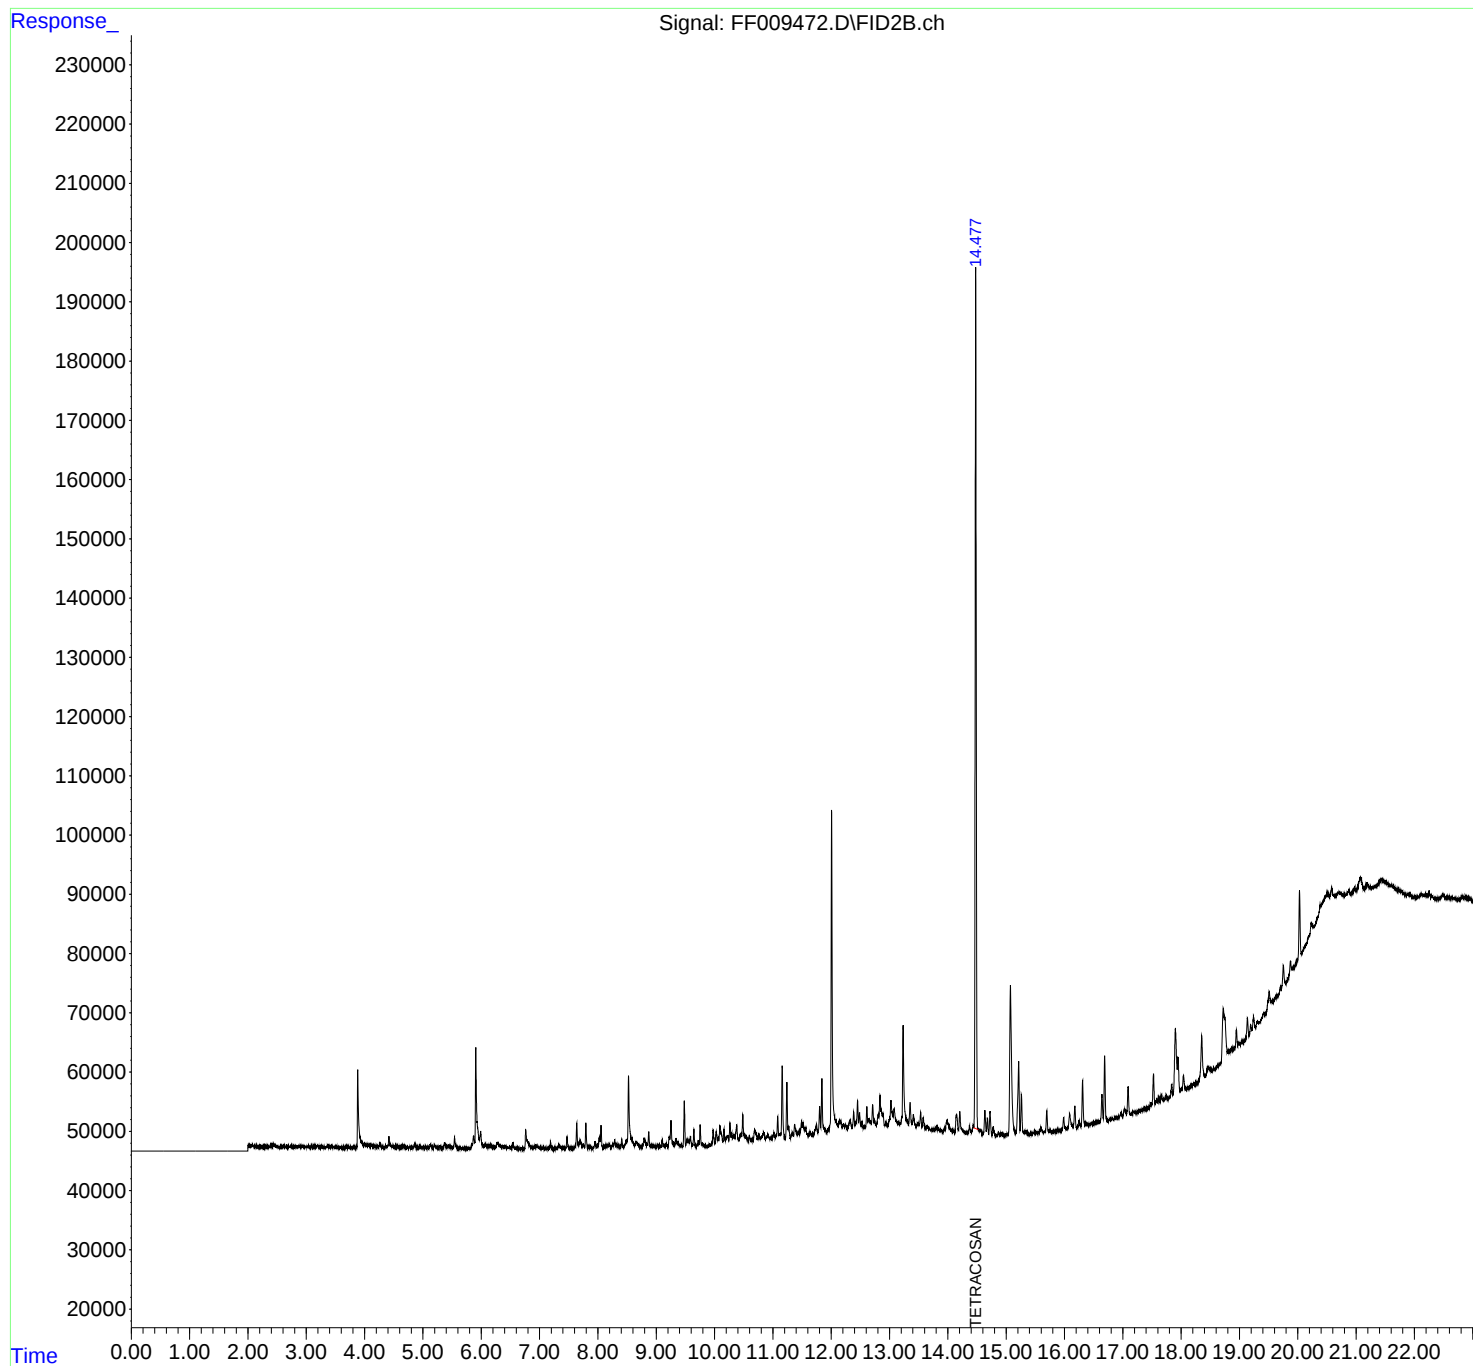

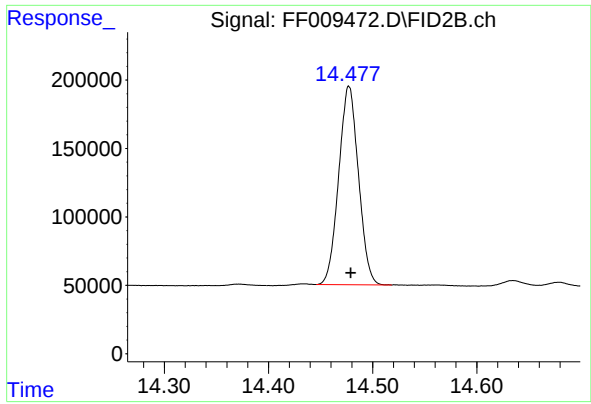

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.477 min
Delta R.T.: -0.002 min
Response: 1912326
Conc: 16.51 ug/ml

Instrument :
FID_F
ClientSampleId :
SASP2-121-1(65-77.7)