

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121622\
 Data File : FF011828.D
 Signal(s) : FID2B.ch
 Acq On : 16 Dec 2022 10:54
 Operator : YP\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 17:39:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
 Quant Title :
 QLast Update : Tue Dec 06 04:24:35 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.771	3372789	24.423 ug/ml
12) N-OCTACOSANE	17.223	3094404	25.104 ug/ml
13) N-TRIACONTANE	18.109	348146	2.874 ug/ml
14) N-DOTRIACONTANE	18.942	464490	3.860 ug/ml
15) N-TETRATRIACONTANE	19.725	397903	3.358 ug/ml
16) N-HEXATRIACONTANE	20.465	299287	2.573 ug/ml
17) N-OCTATRIACONTANE	21.204	328940	2.722 ug/ml
18) N-TETRACONTANE	22.127	469746	3.601 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121622\
Data File : FF011828.D
Signal(s) : FID2B.ch
Acq On : 16 Dec 2022 10:54
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 17:39:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120522.M
Quant Title :
QLast Update : Tue Dec 06 04:24:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

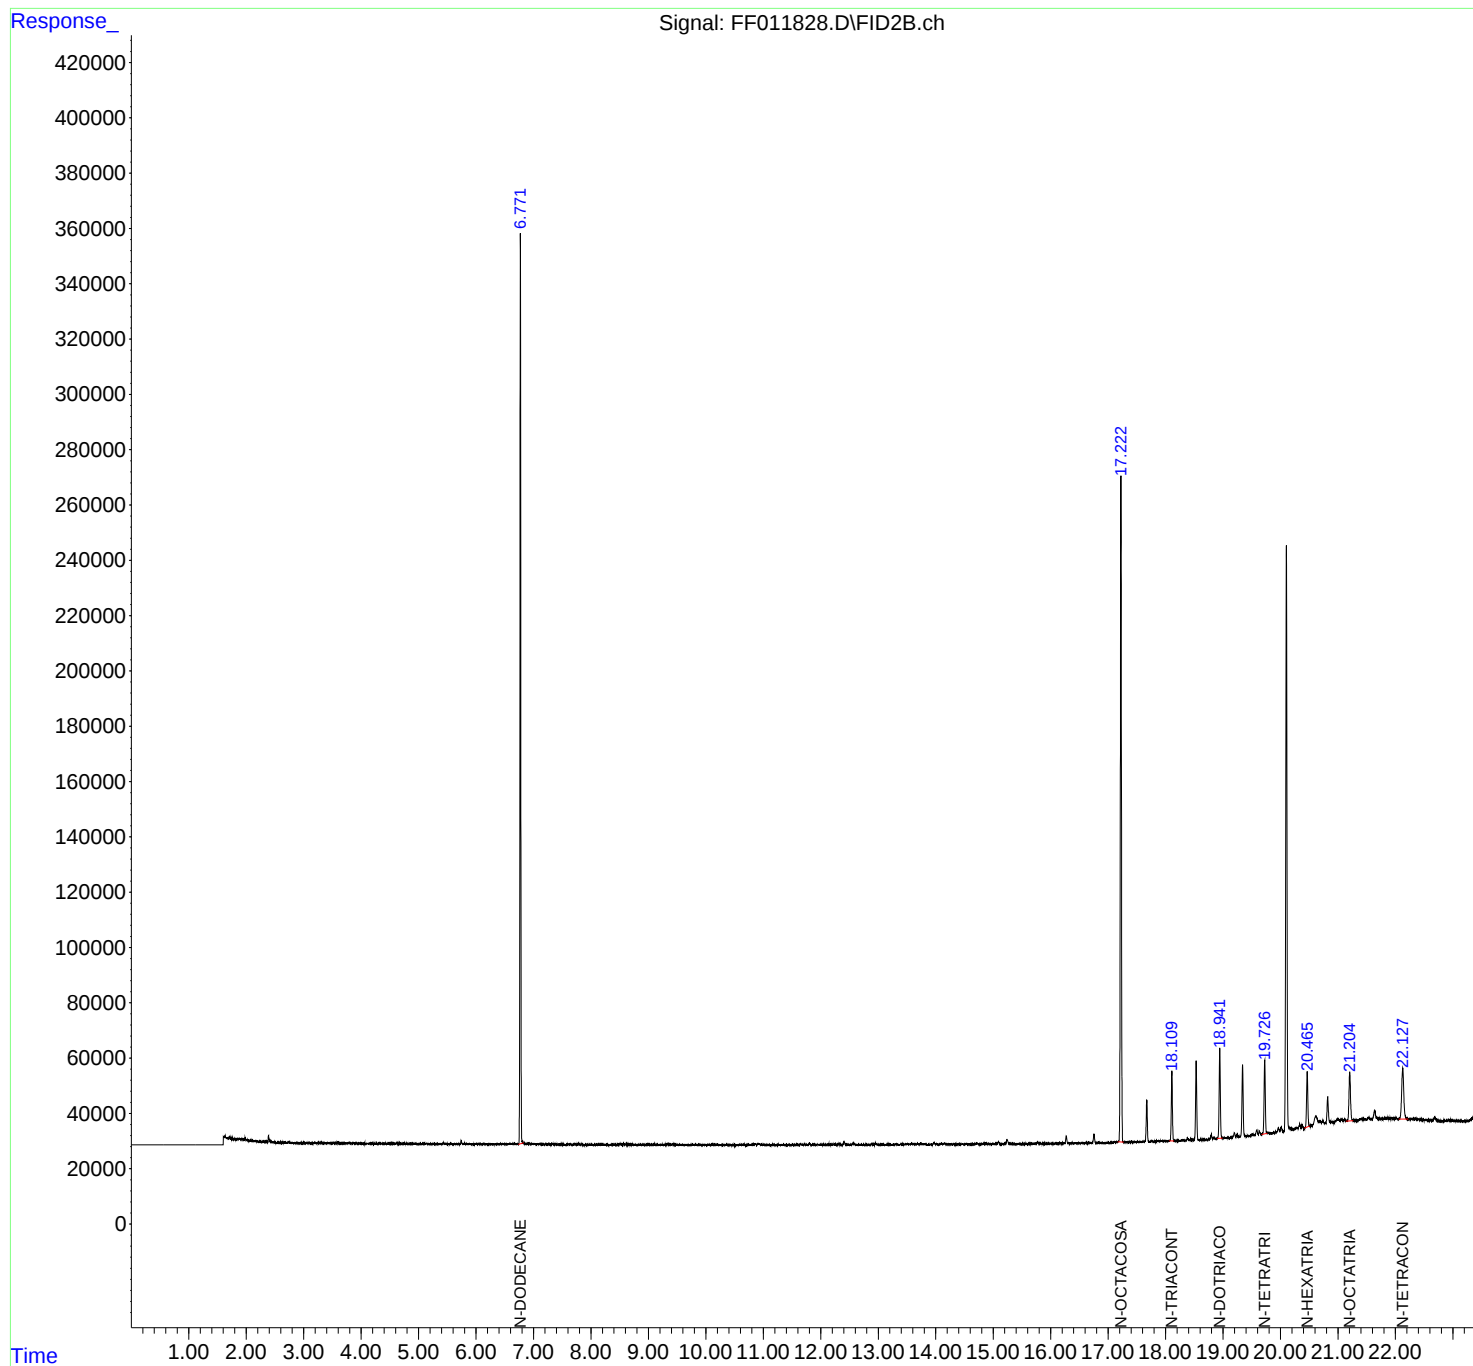


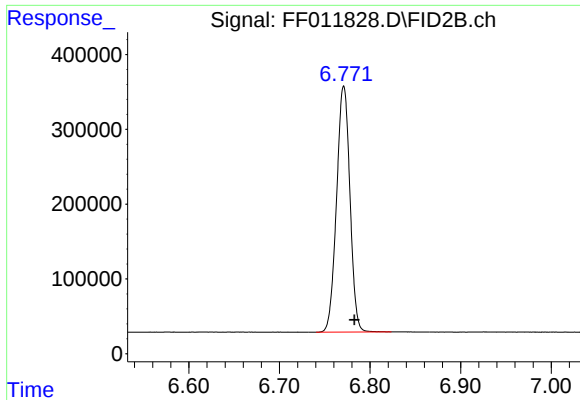

#3 N-DODECANE


R.T.: 6.771 min
Delta R.T.: -0.012 min
Response: 3372789
Conc: 24.42 ug/ml

Instrument :
FID_F
ClientSampleId :

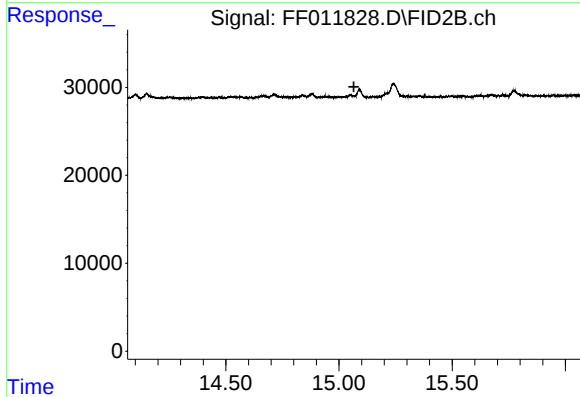


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.066 min
Response: 0
Conc: N.D.

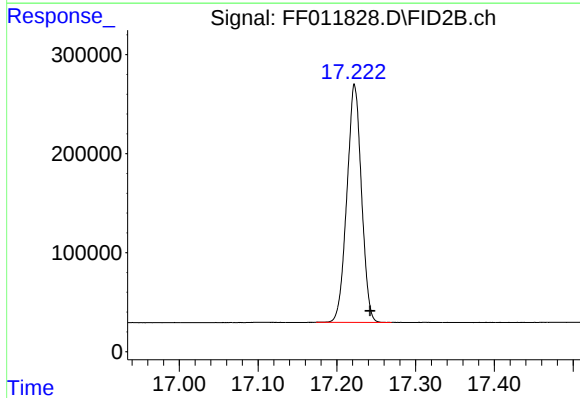


#12 N-OCTACOSANE

R.T.: 17.223 min
Delta R.T.: -0.020 min
Response: 3094404
Conc: 25.10 ug/ml

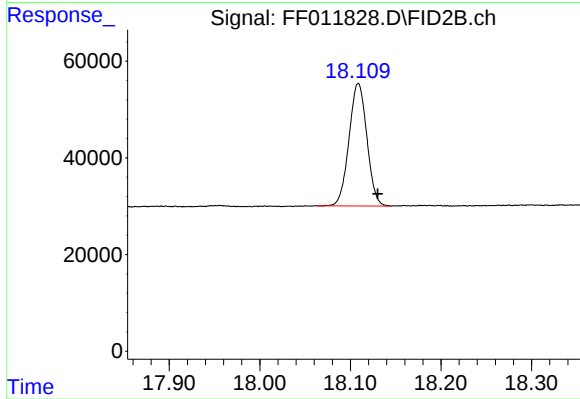

#13 N-TRIACONTANE


R.T.: 18.109 min
Delta R.T.: -0.022 min
Response: 348146
Conc: 2.87 ug/ml

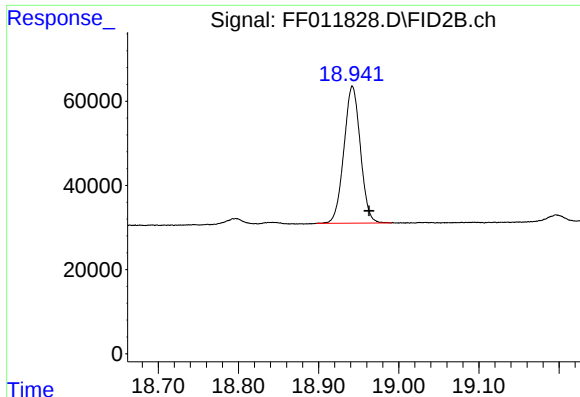

#14 N-DOTRIACONTANE


R.T.: 18.942 min
Delta R.T.: -0.021 min
Response: 464490
Conc: 3.86 ug/ml

Instrument :
FID_F
ClientSampleId :

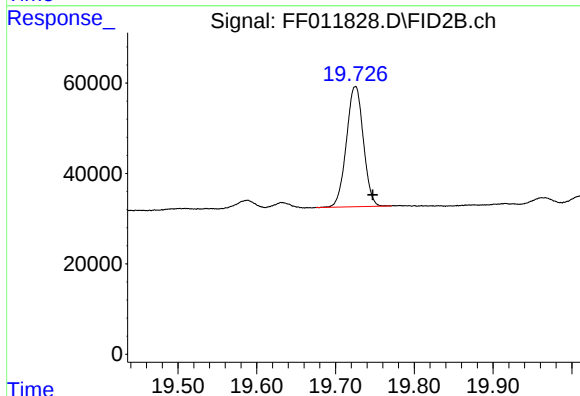


#15 N-TETRATRIACONTANE

R.T.: 19.725 min
Delta R.T.: -0.022 min
Response: 397903
Conc: 3.36 ug/ml

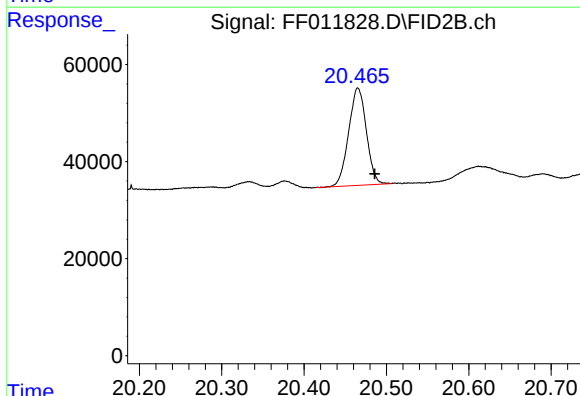


#16 N-HEXATRIACONTANE

R.T.: 20.465 min
Delta R.T.: -0.021 min
Response: 299287
Conc: 2.57 ug/ml

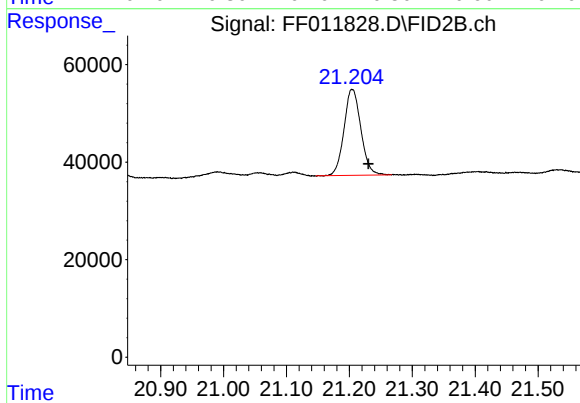

#17 N-OCTATRIACONTANE

R.T.: 21.204 min
Delta R.T.: -0.026 min
Response: 328940
Conc: 2.72 ug/ml

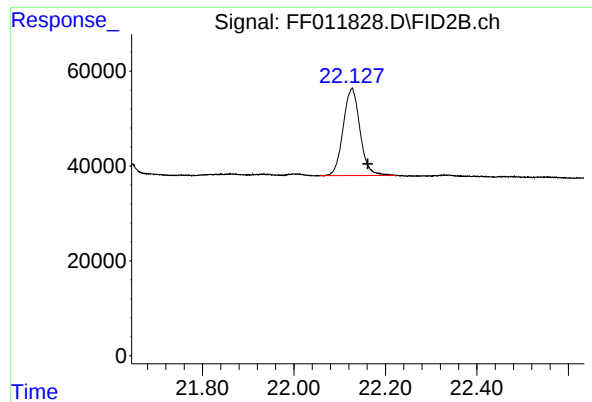

#18 N-TETRACONTANE

R.T.: 22.127 min
Delta R.T.: -0.034 min
Response: 469746
Conc: 3.60 ug/ml

Instrument :

FID_F

ClientSampleId :