

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF121718\
 Data File : FF003032.D
 Signal(s) : FID2B.ch
 Acq On : 17 Dec 2018 12:07
 Operator : AJ\SJ
 Sample : J6425-07
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 17 14:15:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.637	2061083	15.876 ug/ml
Target Compounds				
2)	N-DECANE	4.304f	174362	1.113 ug/ml
3)	N-DODECANE	6.374	813588	5.123 ug/ml
4)	N-TETRADECANE	8.177	475195	2.965 ug/ml
5)	N-HEXADECANE	9.782	625068	3.903 ug/ml
6)	N-OCTADECANE	11.233	1109671	7.005 ug/ml
7)	N-EICOSANE	12.596f	698272	4.527 ug/ml
10)	N-TETRACOSANE	14.817	156257	1.081 ug/ml
12)	N-OCTACOSANE	16.817	147090	1.098 ug/ml
13)	N-TRIACONTANE	17.706	175386	1.369 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF121718\
Data File : FF003032.D
Signal(s) : FID2B.ch
Acq On : 17 Dec 2018 12:07
Operator : AJ\SJ
Sample : J6425-07
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 17 14:15:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

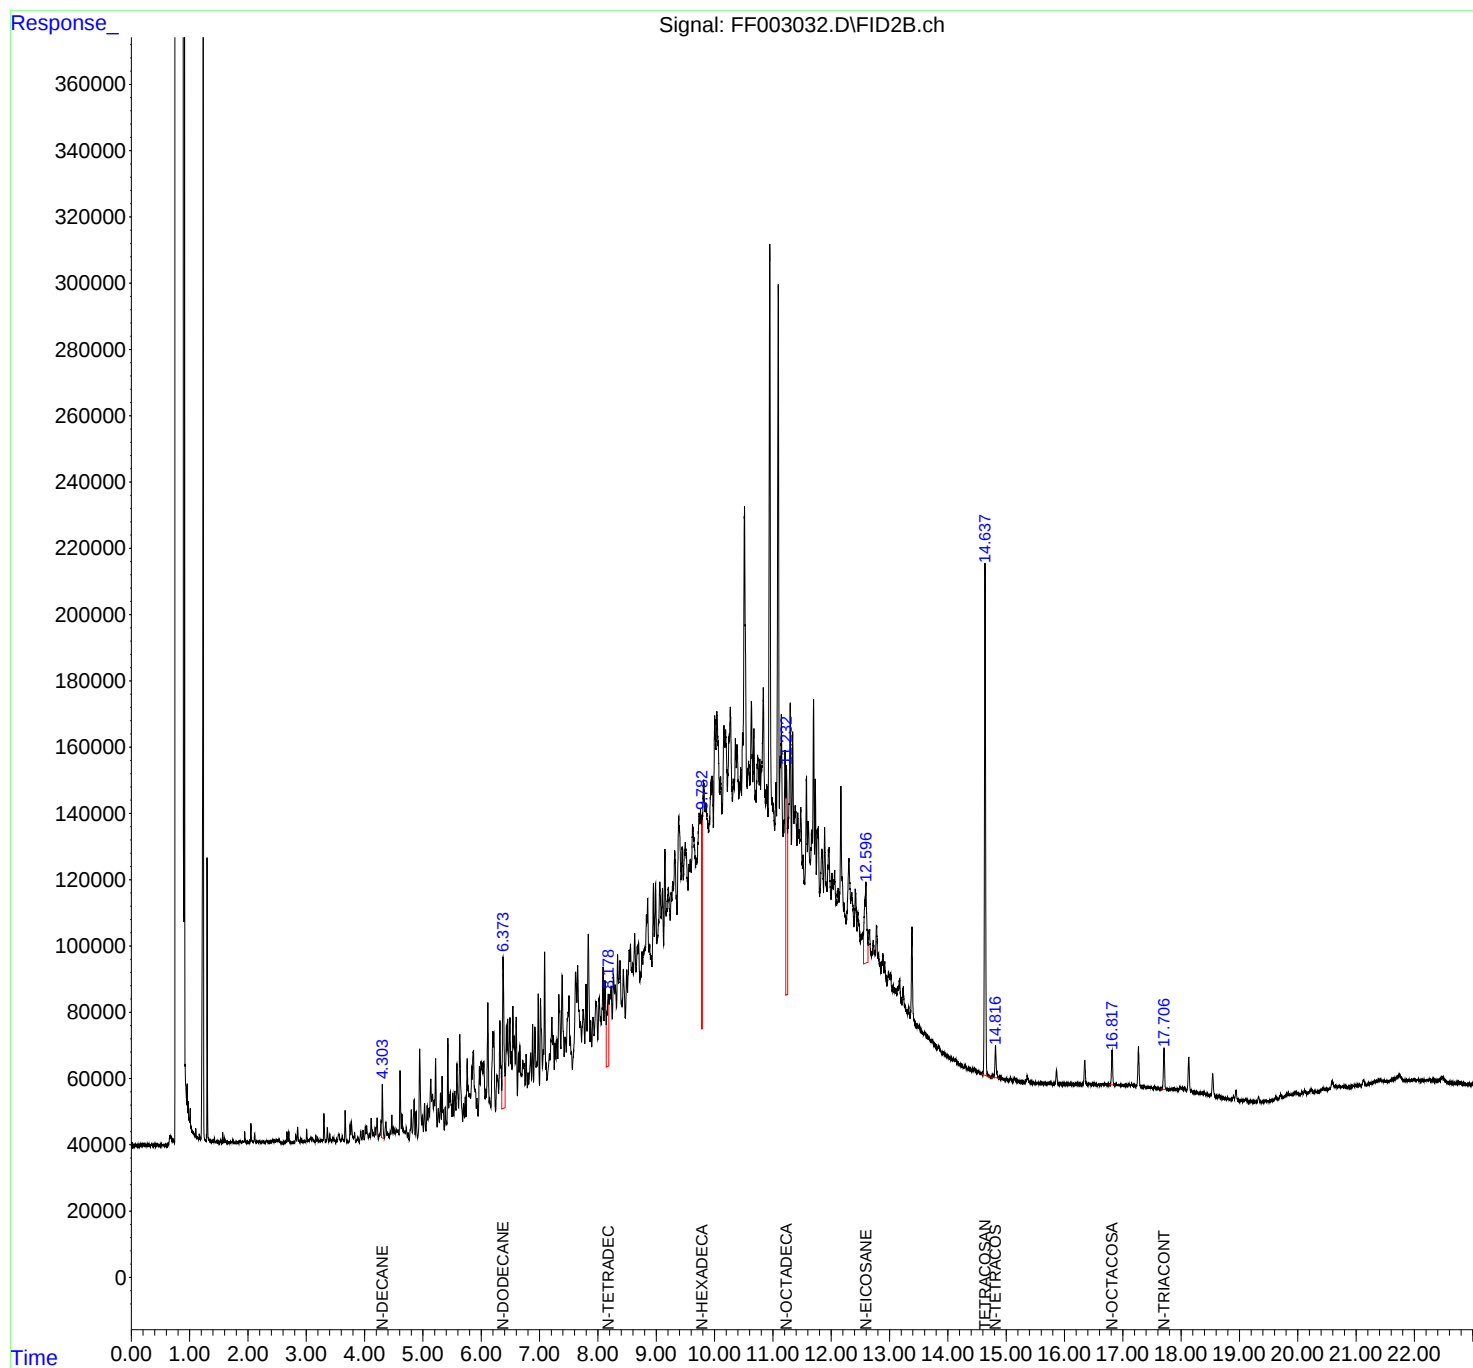

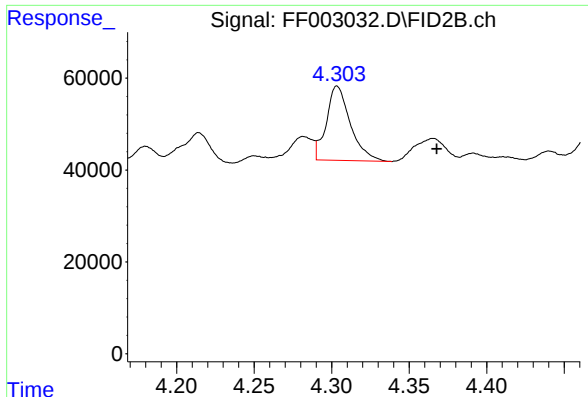


#2 N-DECANE

R.T.: 4.304 min
Delta R.T.: -0.064 min
Response: 174362
Conc: 1.11 ug/ml

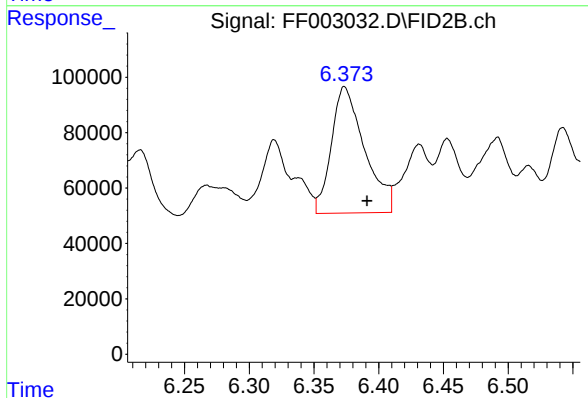


#3 N-DODECANE

R.T.: 6.374 min
Delta R.T.: -0.017 min
Response: 813588
Conc: 5.12 ug/ml

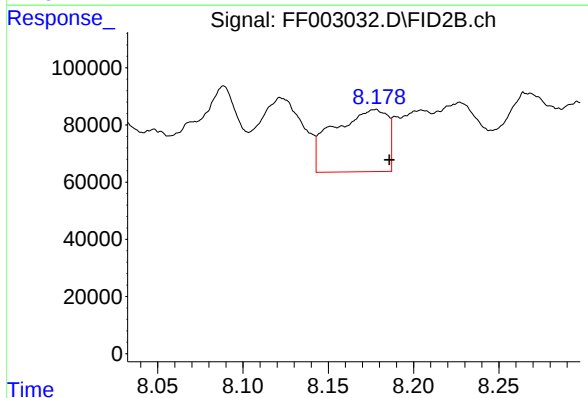


#4 N-TETRADECANE

R.T.: 8.177 min
Delta R.T.: -0.008 min
Response: 475195
Conc: 2.96 ug/ml

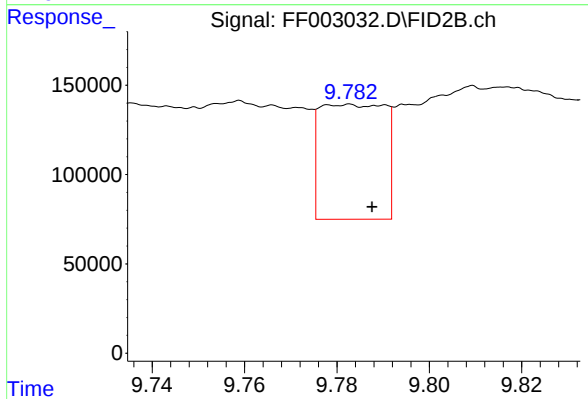


#5 N-HEXADECANE

R.T.: 9.782 min
Delta R.T.: -0.005 min
Response: 625068
Conc: 3.90 ug/ml

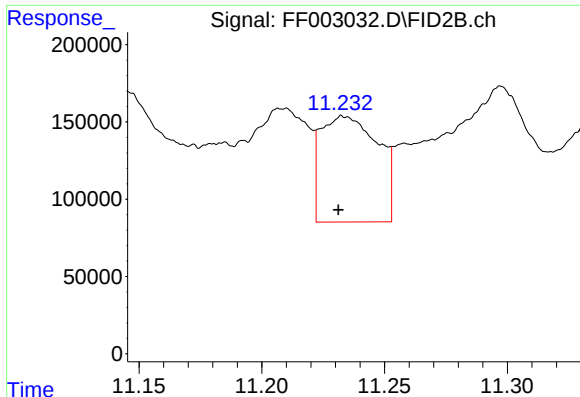


#6 N-OCTADECANE

R.T.: 11.233 min
Delta R.T.: 0.002 min
Response: 1109671
Conc: 7.00 ug/ml

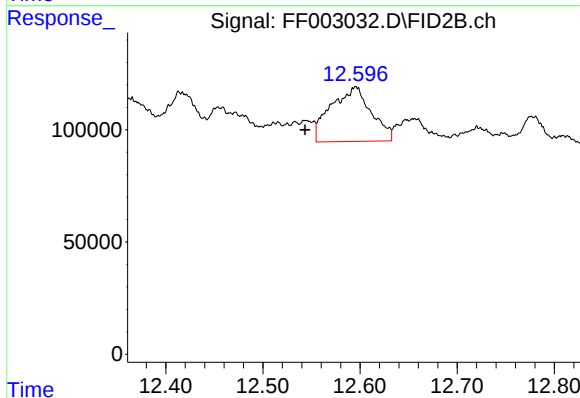


#7 N-EICOSANE

R.T.: 12.596 min
Delta R.T.: 0.052 min
Response: 698272
Conc: 4.53 ug/ml

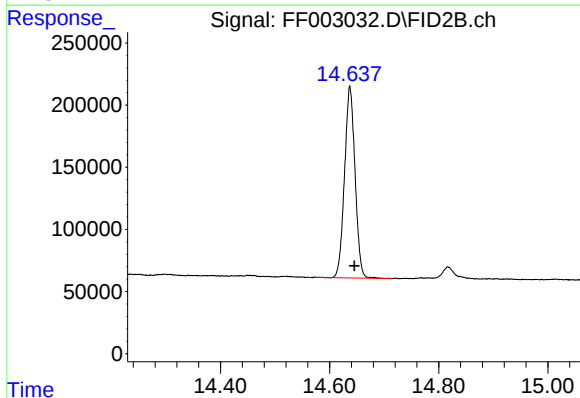


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.637 min
Delta R.T.: -0.008 min
Response: 2061083
Conc: 15.88 ug/ml

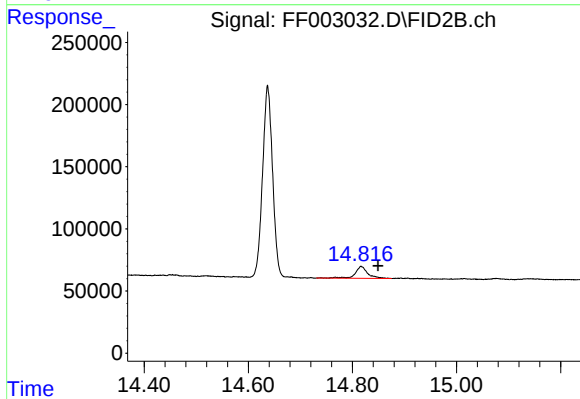


#10 N-TETRACOSANE

R.T.: 14.817 min
Delta R.T.: -0.033 min
Response: 156257
Conc: 1.08 ug/ml

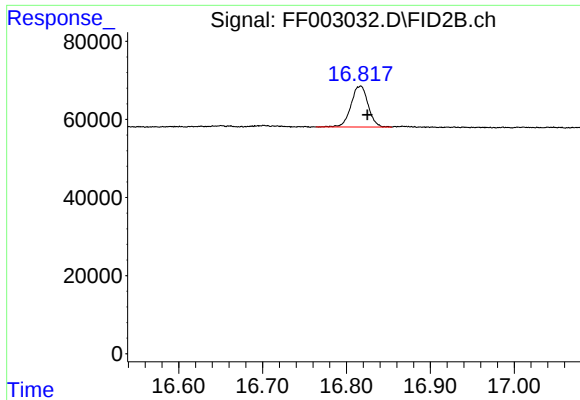

#12 N-OCTACOSANE

R.T.: 16.817 min
Delta R.T.: -0.008 min
Response: 147090
Conc: 1.10 ug/ml

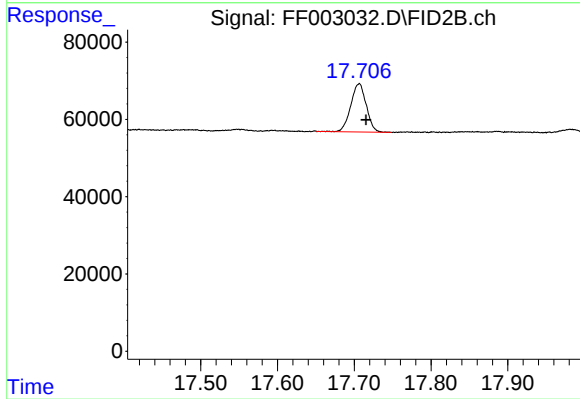

#13 N-TRIACONTANE

R.T.: 17.706 min
Delta R.T.: -0.009 min
Response: 175386
Conc: 1.37 ug/ml