

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121819\
 Data File : FF006044.D
 Signal(s) : FID2B.ch
 Acq On : 18 Dec 2019 15:22
 Operator : DD\AJ
 Sample : K6300-01
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 19 00:28:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	2681916	18.460 ug/ml
Target Compounds			
4) N-TETRADECANE	8.260	106191	0.626 ug/ml
10) N-TETRACOSANE	14.833	381228	2.284 ug/ml
11) N-HEXACOSANE	15.851	500004	3.105 ug/ml
12) N-OCTACOSANE	16.798	365171	2.381 ug/ml
13) N-TRIACONTANE	17.681	248750	1.715 ug/ml
14) N-DOTRIACONTANE	18.511	169451	1.220 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121819\
Data File : FF006044.D
Signal(s) : FID2B.ch
Acq On : 18 Dec 2019 15:22
Operator : DD\AJ
Sample : K6300-01
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 19 00:28:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

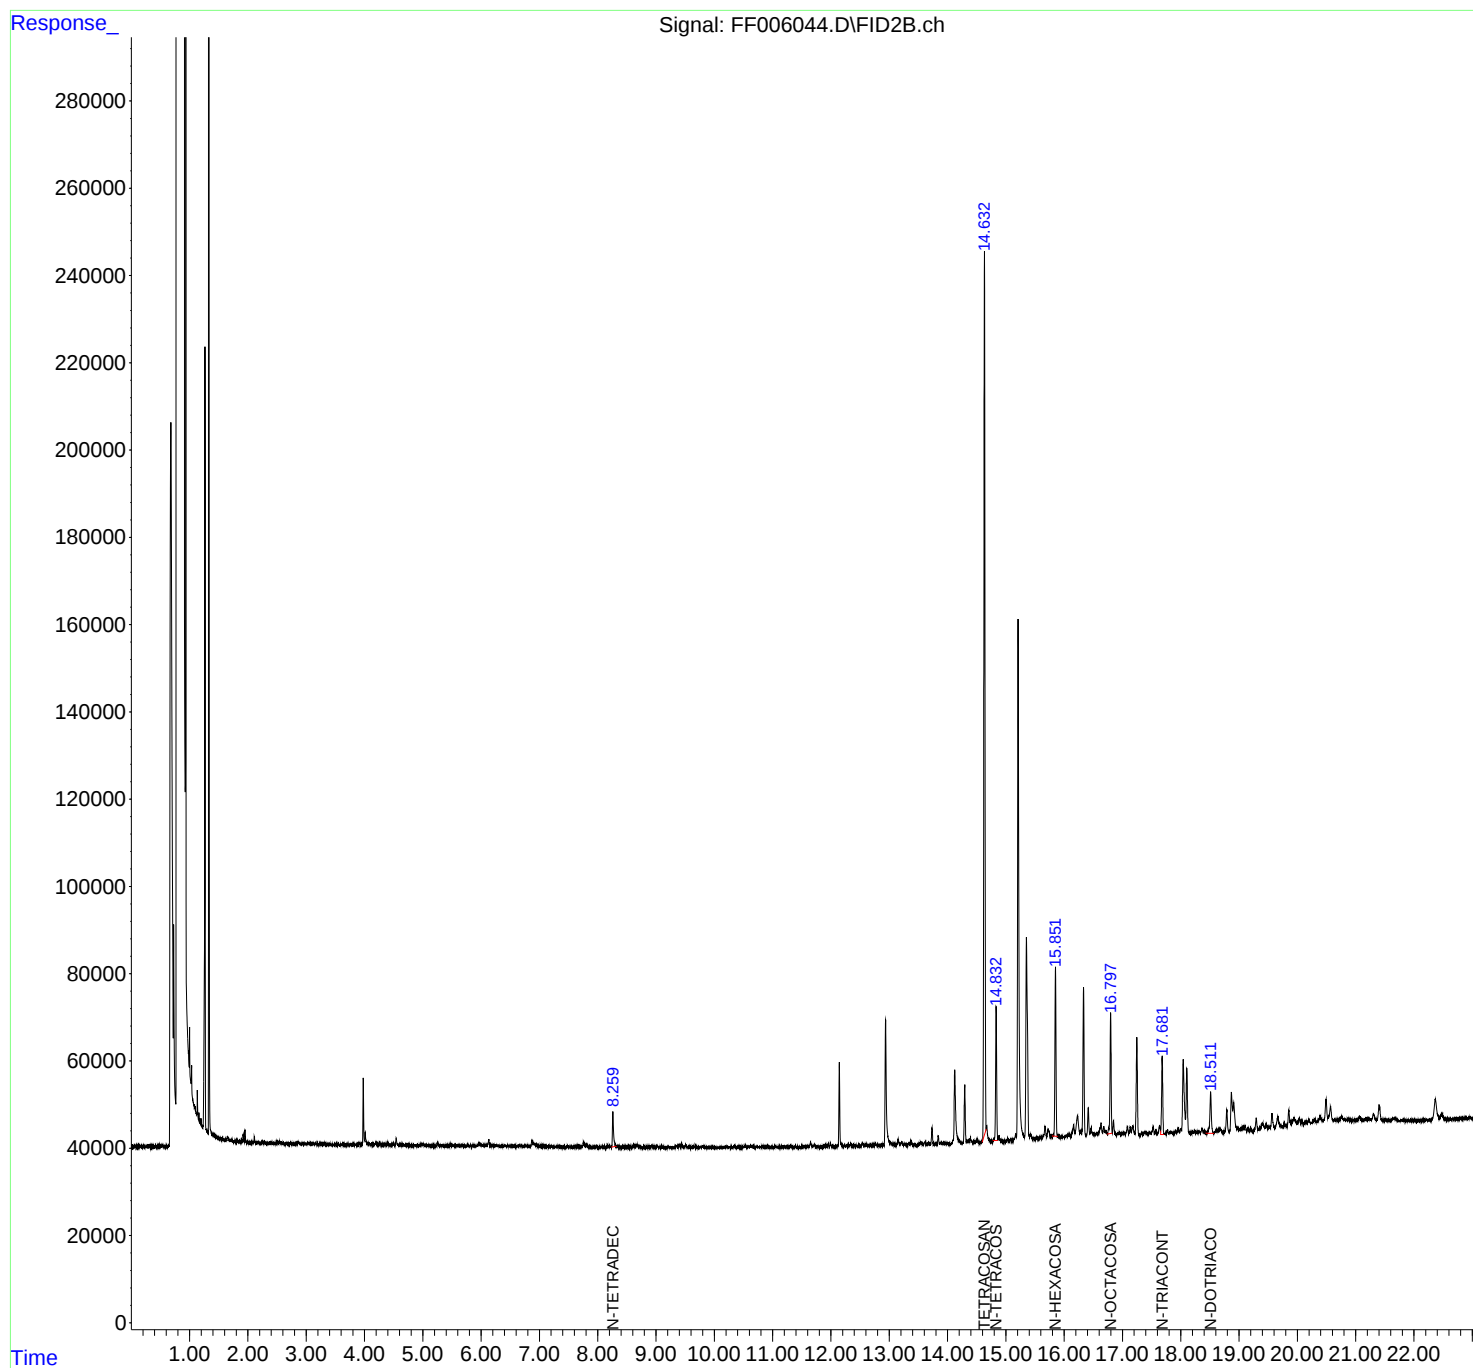


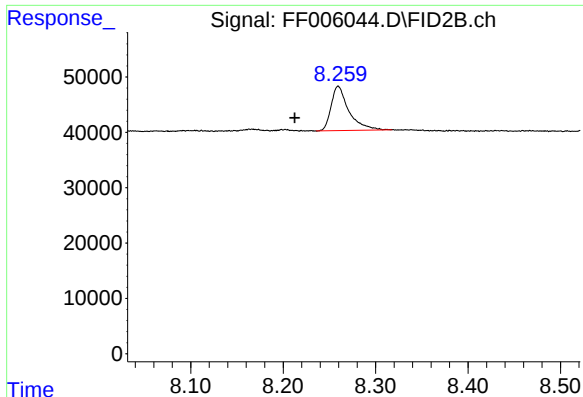

#4 N-TETRADECANE


R.T.: 8.260 min
Delta R.T.: 0.047 min
Response: 106191
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :

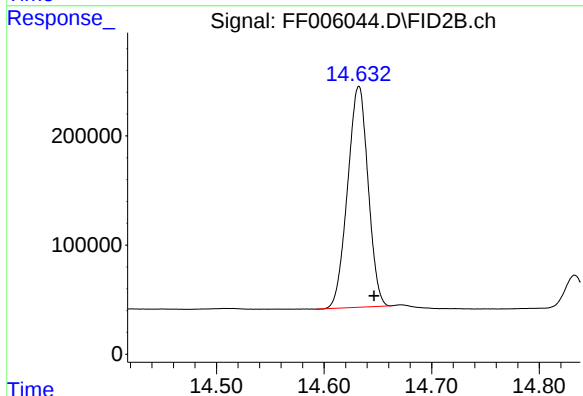


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.632 min
Delta R.T.: -0.014 min
Response: 2681916
Conc: 18.46 ug/ml

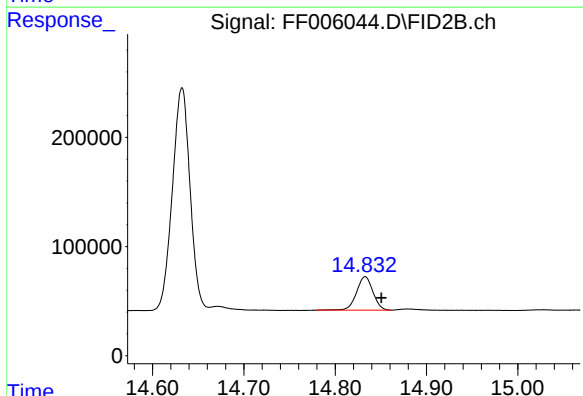


#10 N-TETRACOSANE

R.T.: 14.833 min
Delta R.T.: -0.018 min
Response: 381228
Conc: 2.28 ug/ml

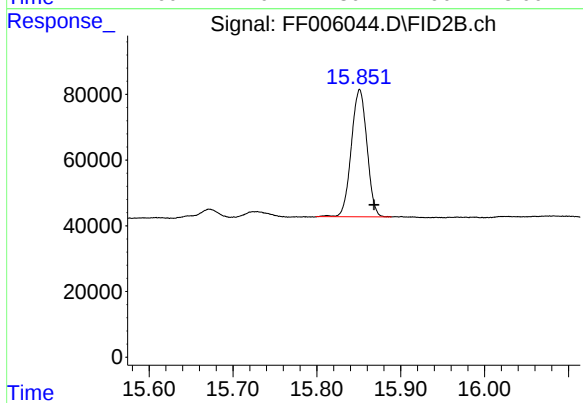

#11 N-HEXACOSANE


R.T.: 15.851 min
Delta R.T.: -0.017 min
Response: 500004
Conc: 3.10 ug/ml

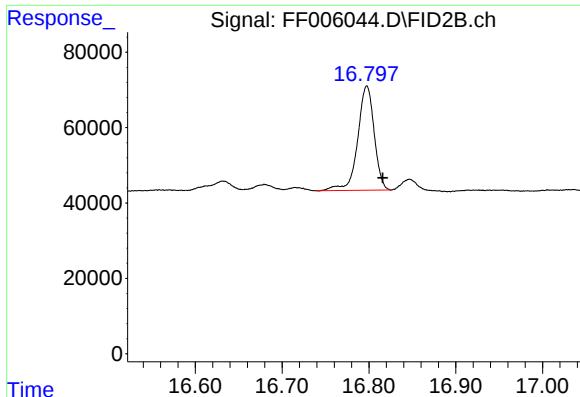

#12 N-OCTACOSANE


R.T.: 16.798 min
Delta R.T.: -0.018 min
Response: 365171
Conc: 2.38 ug/ml

Instrument :
FID_F
ClientSampleId :

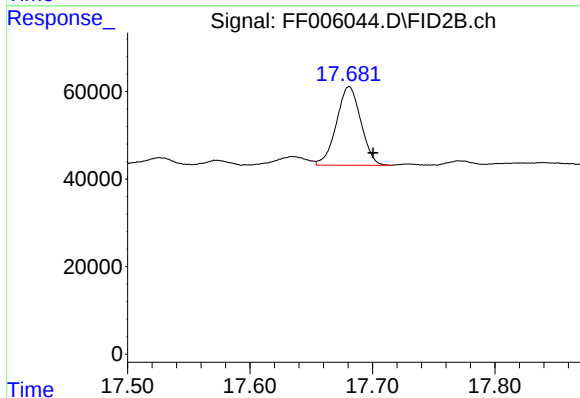

#13 N-TRIACONTANE

R.T.: 17.681 min
Delta R.T.: -0.020 min
Response: 248750
Conc: 1.71 ug/ml

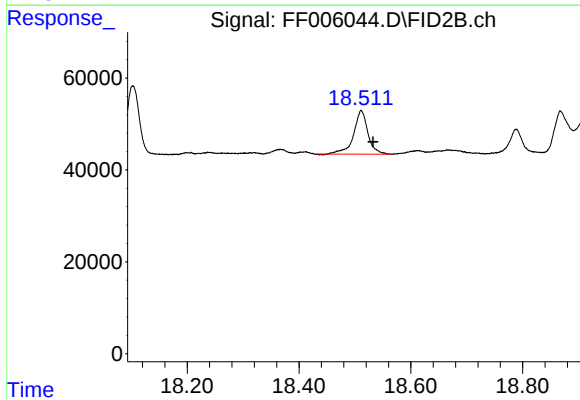

#14 N-DOTRIACONTANE

R.T.: 18.511 min
Delta R.T.: -0.021 min
Response: 169451
Conc: 1.22 ug/ml