

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121819\
 Data File : FF006047.D
 Signal(s) : FID2B.ch
 Acq On : 18 Dec 2019 16:52
 Operator : DD\AJ
 Sample : K6300-04
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 19 00:29:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	2997547	20.633 ug/ml
Target Compounds			
4) N-TETRADECANE	8.259	220294	1.299 ug/ml
10) N-TETRACOSANE	14.833	626713	3.755 ug/ml
11) N-HEXACOSANE	15.851	690869	4.290 ug/ml
12) N-OCTACOSANE	16.798	447471	2.917 ug/ml
13) N-TRIACONTANE	17.681	297601	2.051 ug/ml
14) N-DOTRIACONTANE	18.510	203701	1.467 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121819\
Data File : FF006047.D
Signal(s) : FID2B.ch
Acq On : 18 Dec 2019 16:52
Operator : DD\AJ
Sample : K6300-04
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 19 00:29:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

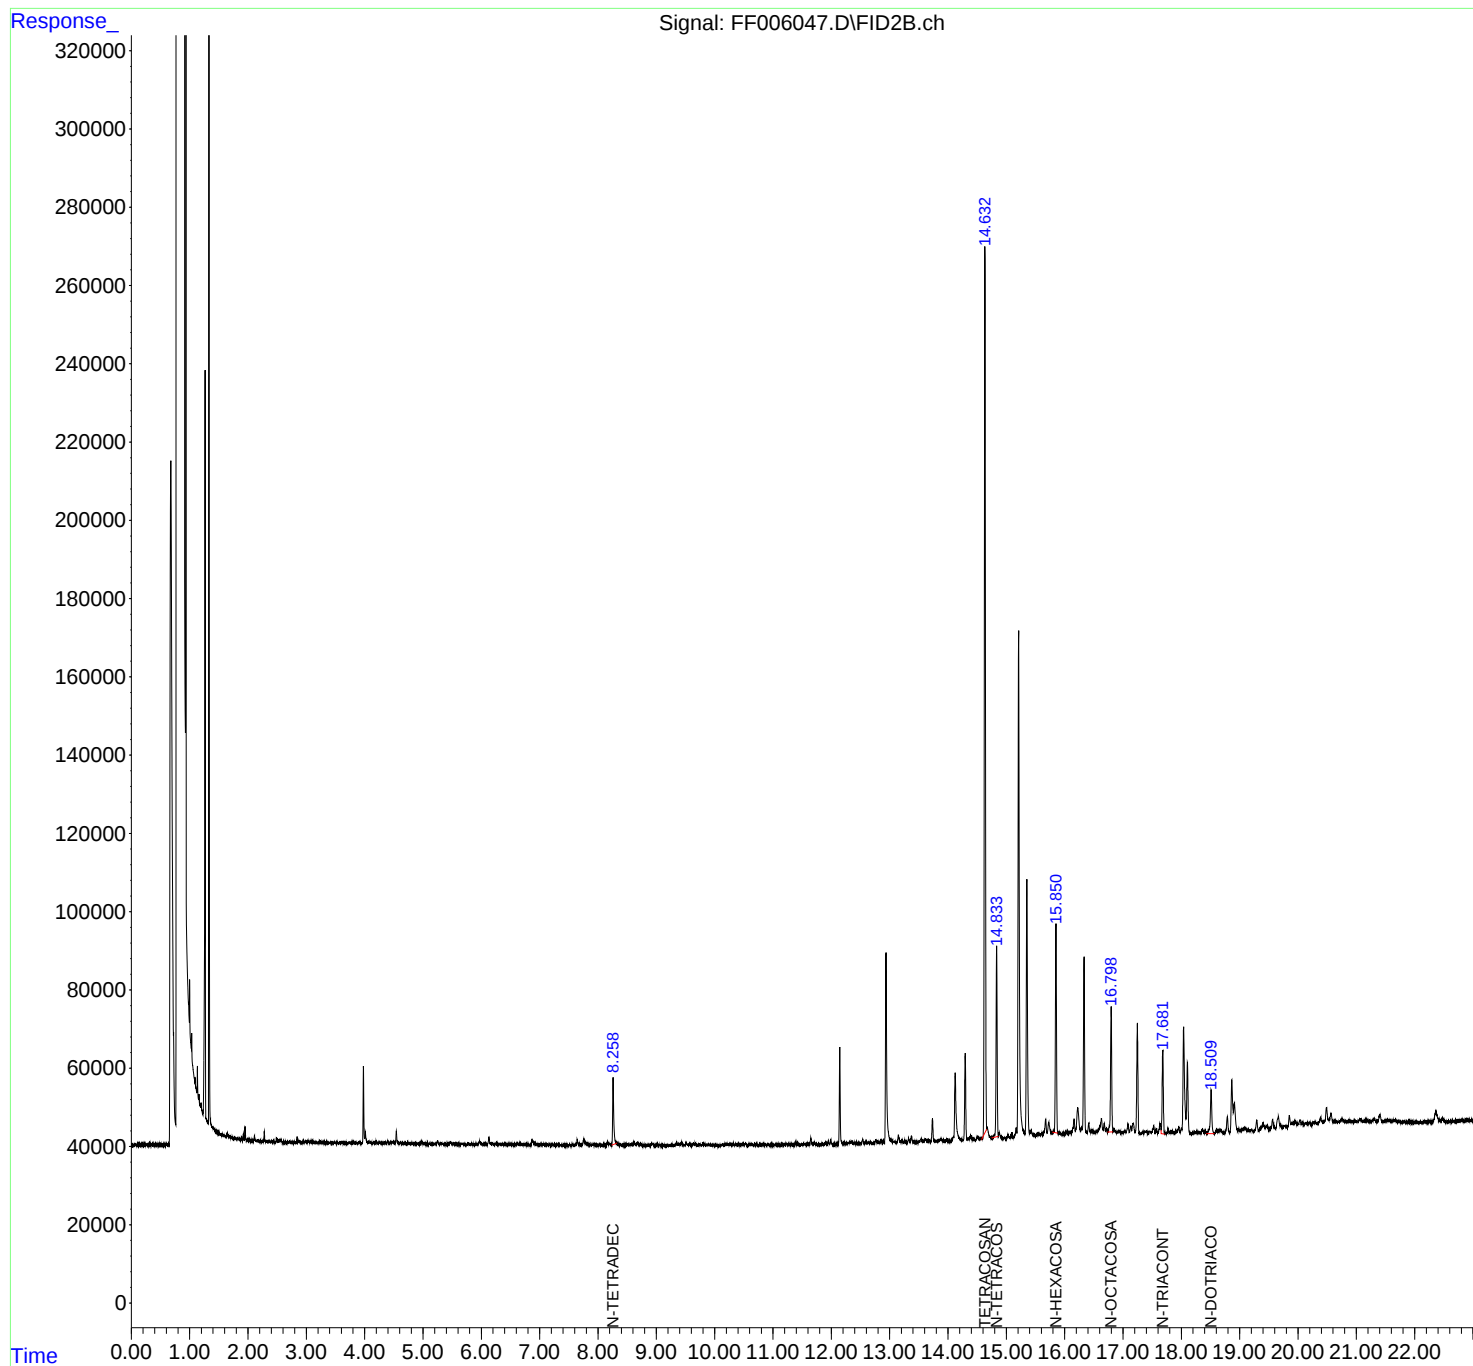


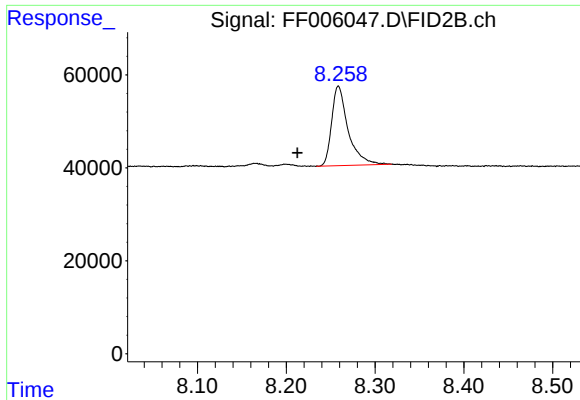

#4 N-TETRADECANE


R.T.: 8.259 min
Delta R.T.: 0.046 min
Response: 220294
Conc: 1.30 ug/ml

Instrument :
FID_F
ClientSampleId :

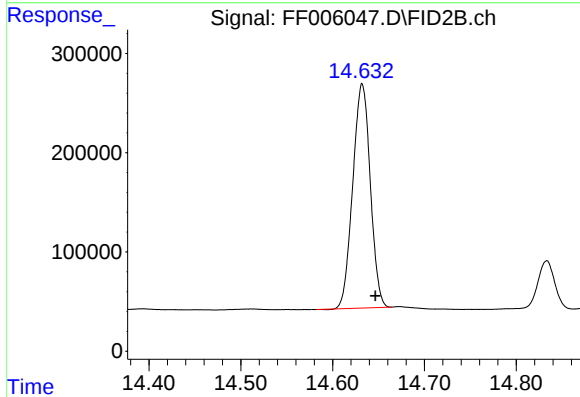


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.632 min
Delta R.T.: -0.014 min
Response: 2997547
Conc: 20.63 ug/ml

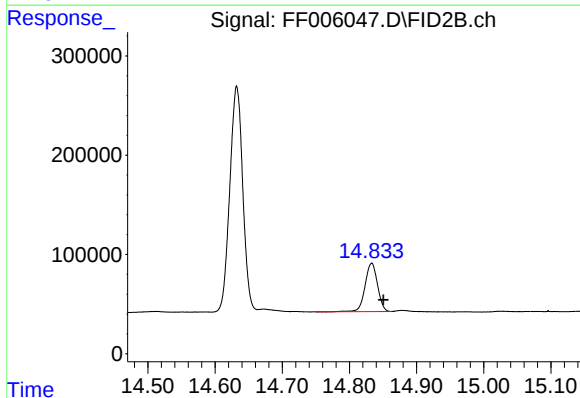


#10 N-TETRACOSANE

R.T.: 14.833 min
Delta R.T.: -0.017 min
Response: 626713
Conc: 3.76 ug/ml

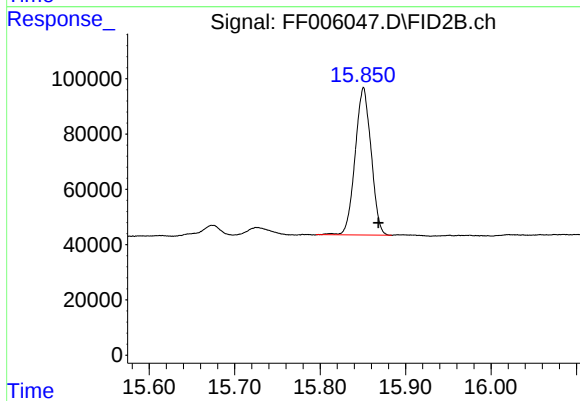

#11 N-HEXACOSANE


R.T.: 15.851 min
Delta R.T.: -0.018 min
Response: 690869
Conc: 4.29 ug/ml

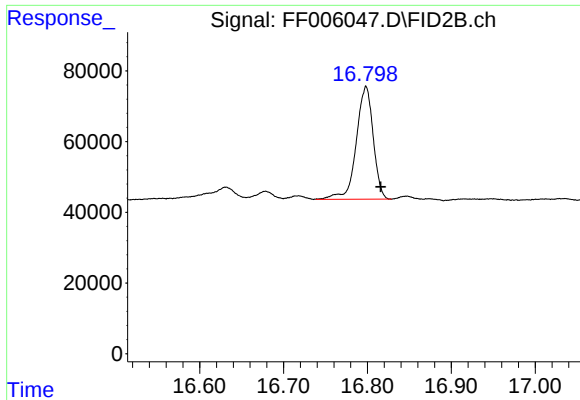

#12 N-OCTACOSANE


R.T.: 16.798 min
Delta R.T.: -0.017 min
Response: 447471
Conc: 2.92 ug/ml

Instrument :
FID_F
ClientSampleId :

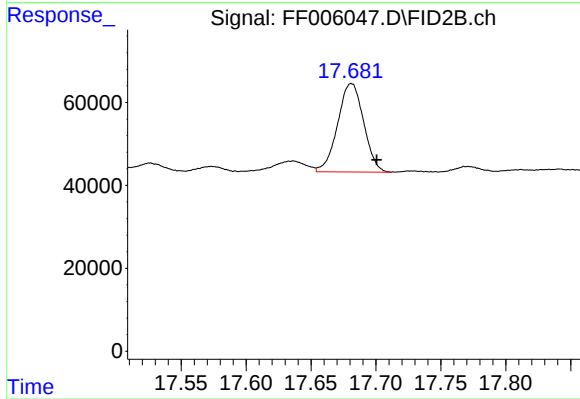

#13 N-TRIACONTANE

R.T.: 17.681 min
Delta R.T.: -0.019 min
Response: 297601
Conc: 2.05 ug/ml

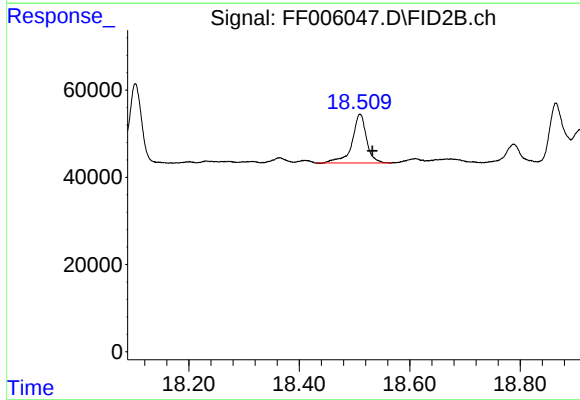

#14 N-DOTRIACONTANE

R.T.: 18.510 min
Delta R.T.: -0.022 min
Response: 203701
Conc: 1.47 ug/ml