

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121819\
 Data File : FF006050.D
 Signal(s) : FID2B.ch
 Acq On : 18 Dec 2019 18:23
 Operator : DD\AJ
 Sample : K6300-07
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 19 00:29:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	2436314	16.770 ug/ml
Target Compounds			
3) N-DODECANE	6.426	184307	1.096 ug/ml
4) N-TETRADECANE	8.258	281387	1.659 ug/ml
10) N-TETRACOSANE	14.833	570930	3.421 ug/ml
11) N-HEXACOSANE	15.851	527404	3.275 ug/ml
12) N-OCTACOSANE	16.796	354260	2.309 ug/ml
13) N-TRIACONTANE	17.680	279722	1.928 ug/ml
14) N-DOTRIACONTANE	18.508	205695	1.481 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121819\
Data File : FF006050.D
Signal(s) : FID2B.ch
Acq On : 18 Dec 2019 18:23
Operator : DD\AJ
Sample : K6300-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 19 00:29:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

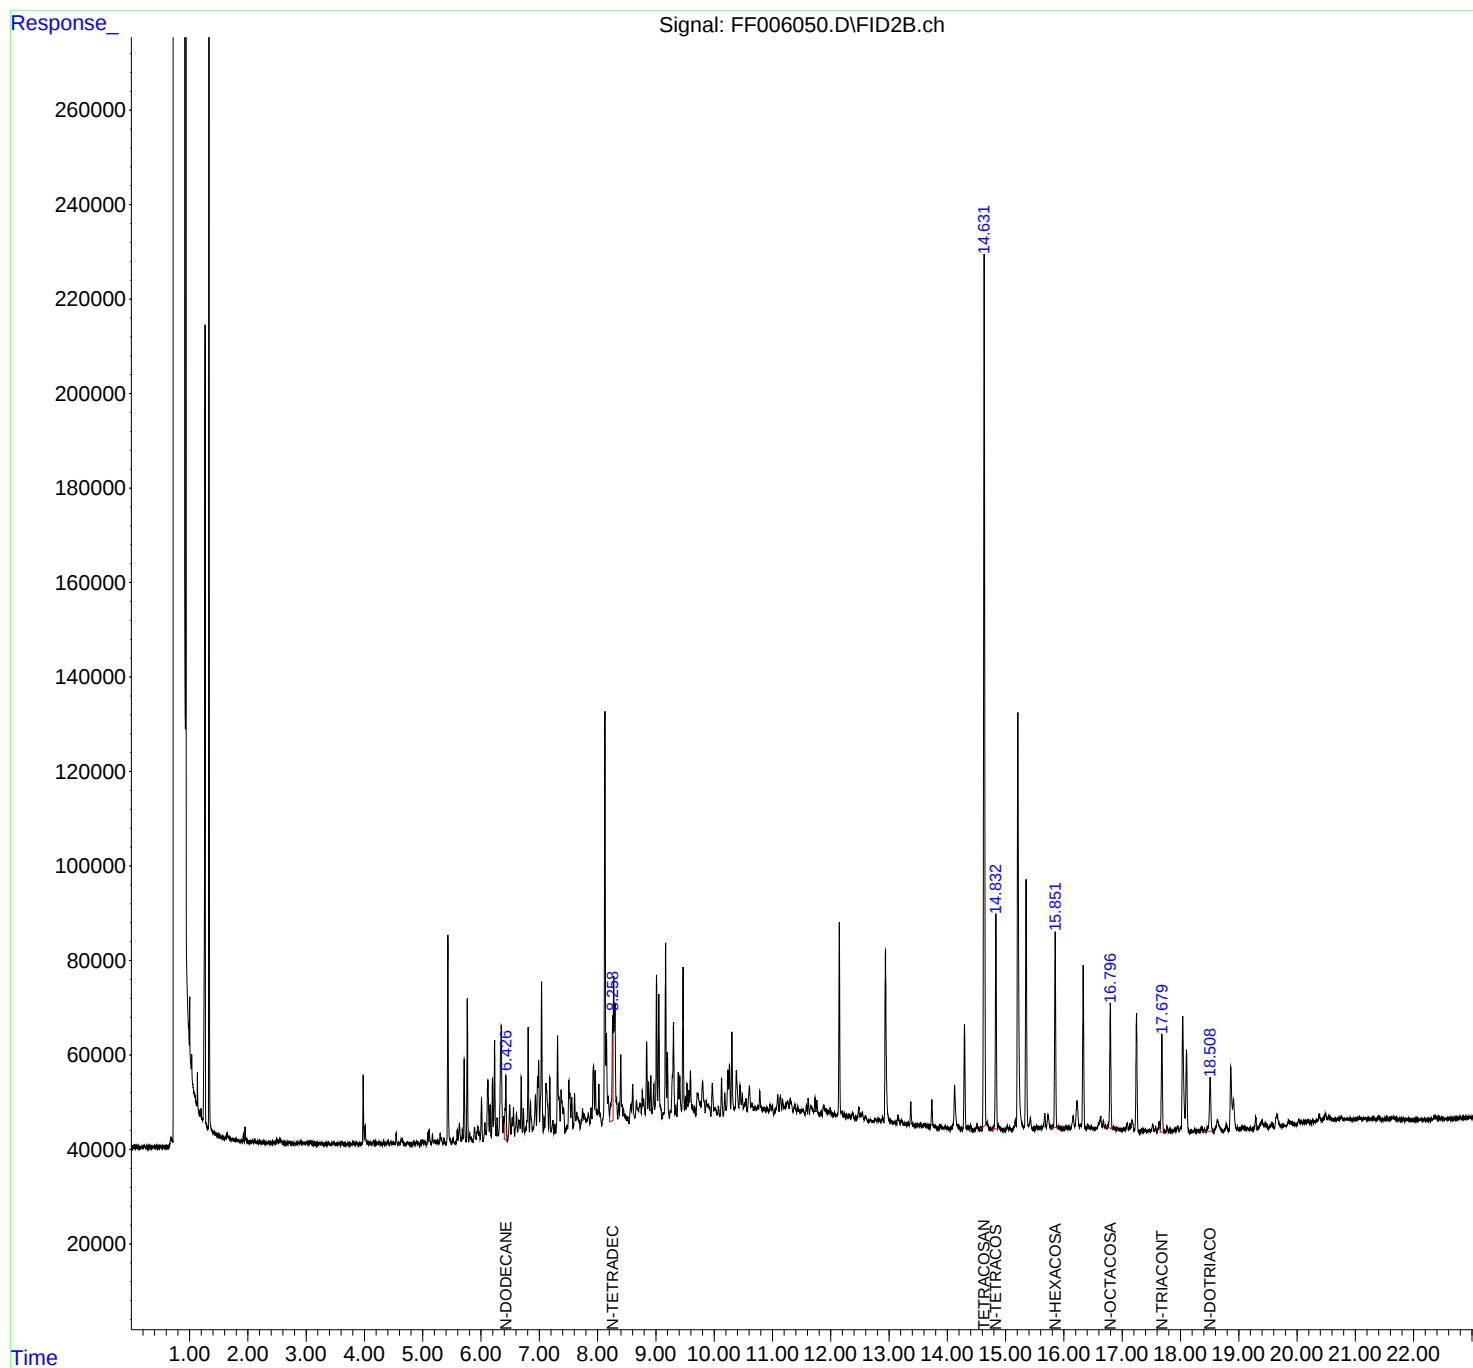


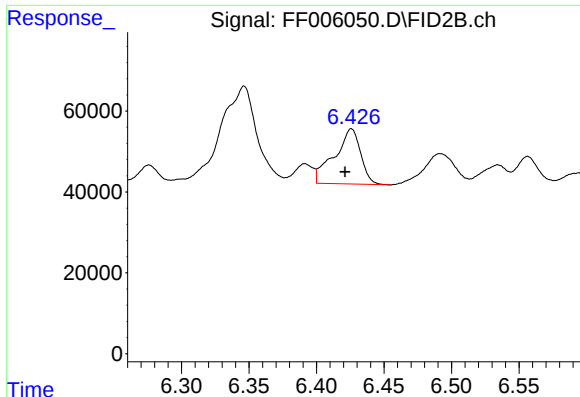

#3 N-DODECANE


R.T.: 6.426 min
Delta R.T.: 0.005 min
Response: 184307
Conc: 1.10 ug/ml

Instrument :
FID_F
ClientSampleId :

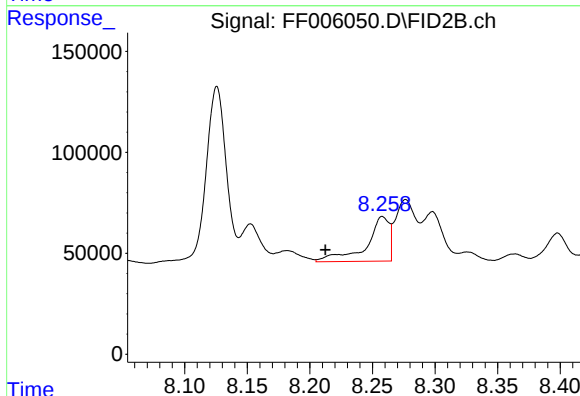


#4 N-TETRADECANE

R.T.: 8.258 min
Delta R.T.: 0.045 min
Response: 281387
Conc: 1.66 ug/ml

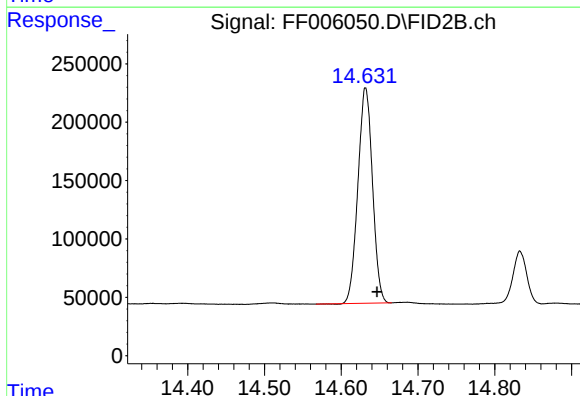


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.632 min
Delta R.T.: -0.015 min
Response: 2436314
Conc: 16.77 ug/ml

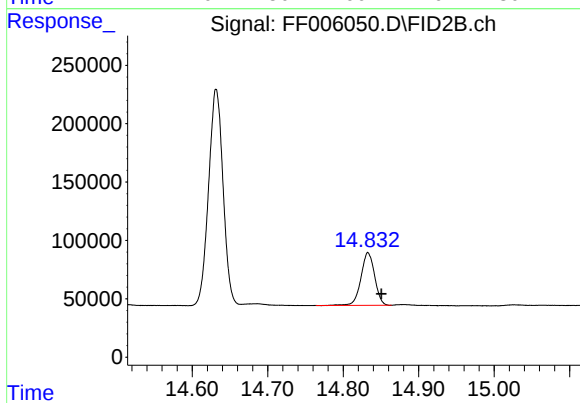

#10 N-TETRACOSANE


R.T.: 14.833 min
Delta R.T.: -0.018 min
Response: 570930
Conc: 3.42 ug/ml

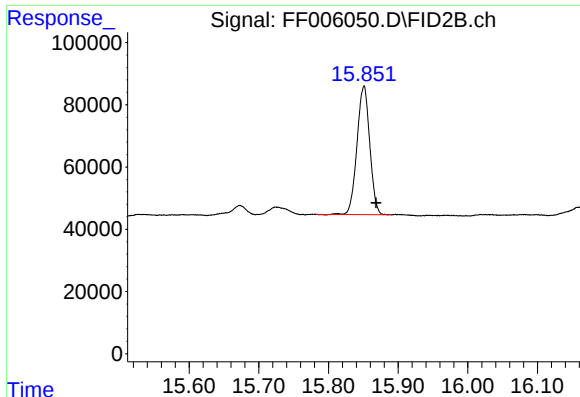

#11 N-HEXACOSANE


R.T.: 15.851 min
Delta R.T.: -0.017 min
Response: 527404
Conc: 3.27 ug/ml

Instrument :
FID_F
ClientSampleId :

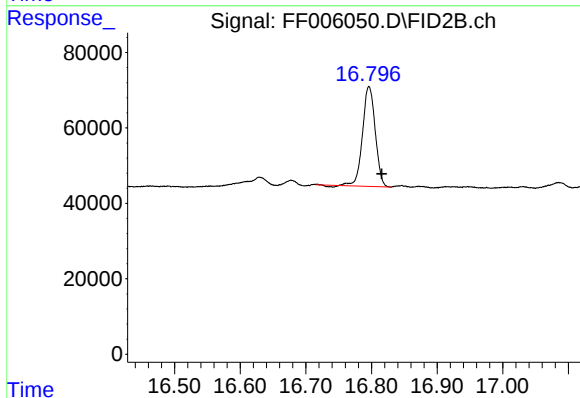


#12 N-OCTACOSANE

R.T.: 16.796 min
Delta R.T.: -0.020 min
Response: 354260
Conc: 2.31 ug/ml

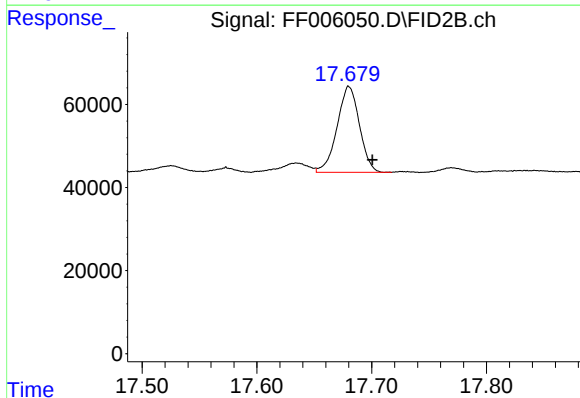

#13 N-TRIACONTANE

R.T.: 17.680 min
Delta R.T.: -0.020 min
Response: 279722
Conc: 1.93 ug/ml

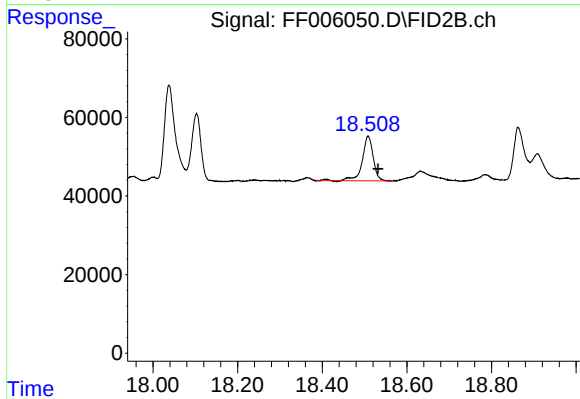

#14 N-DOTRIACONTANE

R.T.: 18.508 min
Delta R.T.: -0.024 min
Response: 205695
Conc: 1.48 ug/ml