

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121819\
 Data File : FF006045.D
 Signal(s) : FID2B.ch
 Acq On : 18 Dec 2019 15:52
 Operator : DD\AJ
 Sample : K6300-02MS
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 SSI-MW-4MS

Integration File: autoint1.e
 Quant Time: Dec 19 00:28:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	2571010	17.697 ug/ml
Target Compounds			
2) N-DECANE	4.396	2595260	15.806 ug/ml
3) N-DODECANE	6.411	2741029	16.307 ug/ml
4) N-TETRADECANE	8.201	2843819	16.771 ug/ml
5) N-HEXADECANE	9.797	2939159	17.058 ug/ml
6) N-OCTADECANE	11.235	2935555	17.122 ug/ml
7) N-EICOSANE	12.540	2911418	16.857 ug/ml
8) N-DOCOSANE	13.735	2864675	16.829 ug/ml
10) N-TETRACOSANE	14.835	2823576	16.918 ug/ml
11) N-HEXACOSANE	15.852	2731414	16.961 ug/ml
12) N-OCTACOSANE	16.799	2650835	17.281 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121819\
Data File : FF006045.D
Signal(s) : FID2B.ch
Acq On : 18 Dec 2019 15:52
Operator : DD\AJ
Sample : K6300-02MS
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
SSI-MW-4MS

Integration File: autoint1.e
Quant Time: Dec 19 00:28:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

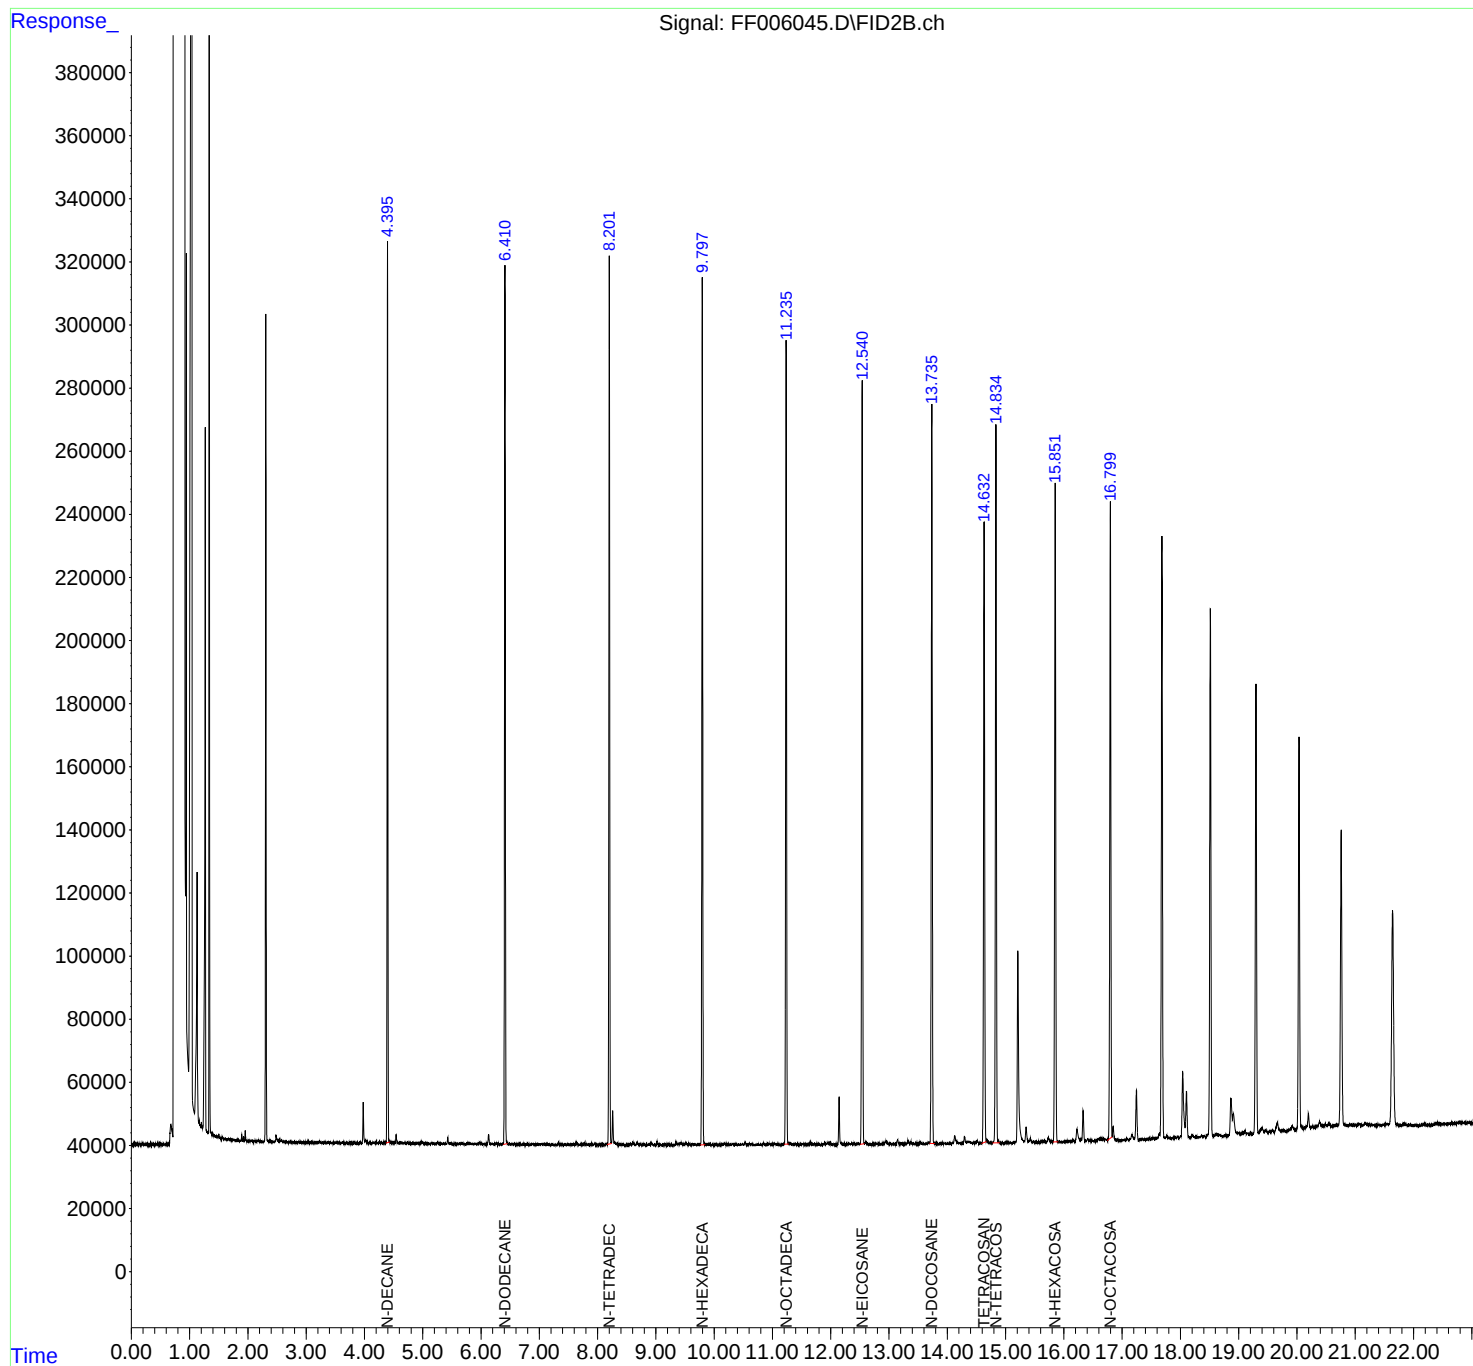


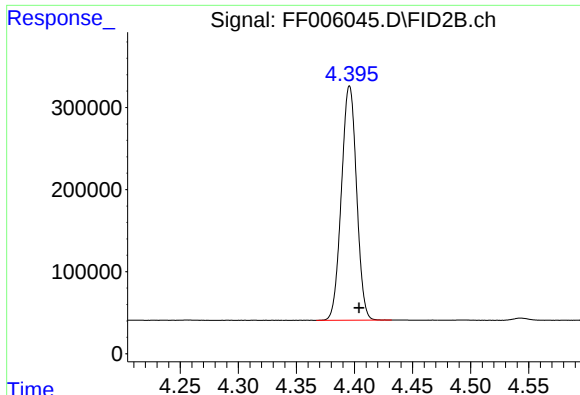

#2 N-DECANE


R.T.: 4.396 min
Delta R.T.: -0.008 min
Response: 2595260
Conc: 15.81 ug/ml

Instrument :
FID_F
ClientSampleId :
SSI-MW-4MS

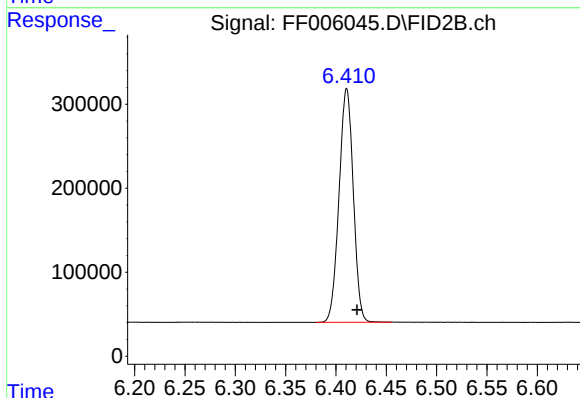


#3 N-DODECANE

R.T.: 6.411 min
Delta R.T.: -0.010 min
Response: 2741029
Conc: 16.31 ug/ml

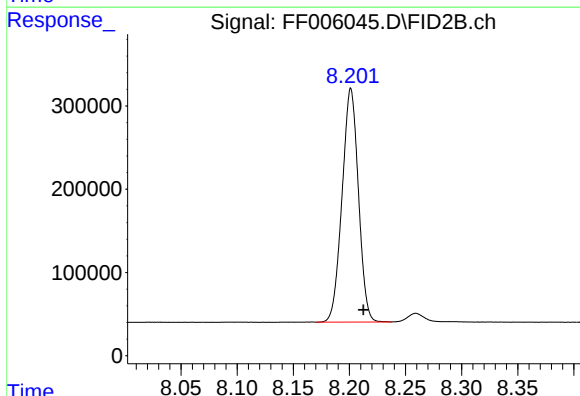


#4 N-TETRADECANE

R.T.: 8.201 min
Delta R.T.: -0.011 min
Response: 2843819
Conc: 16.77 ug/ml

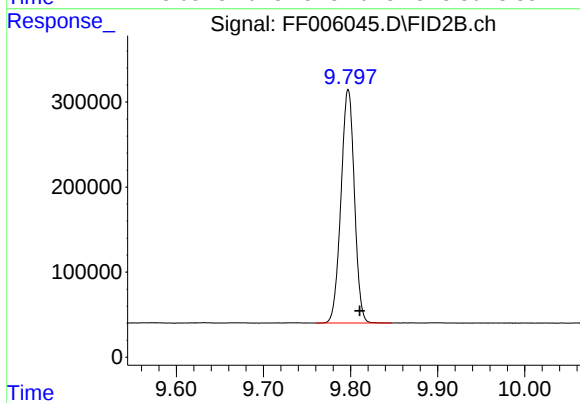

#5 N-HEXADECANE


R.T.: 9.797 min
Delta R.T.: -0.013 min
Response: 2939159
Conc: 17.06 ug/ml

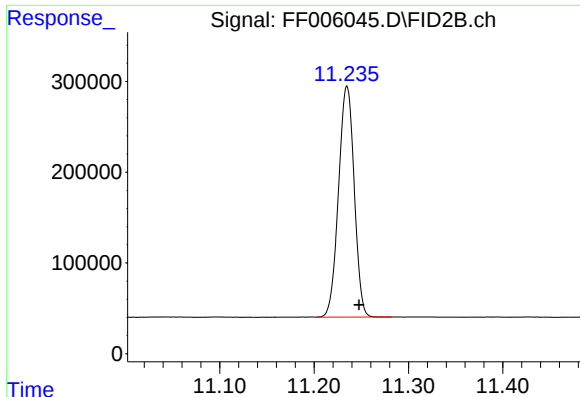

#6 N-OCTADECANE


R.T.: 11.235 min
Delta R.T.: -0.013 min
Response: 2935555
Conc: 17.12 ug/ml

Instrument :
FID_F
ClientSampleId :
SSI-MW-4MS

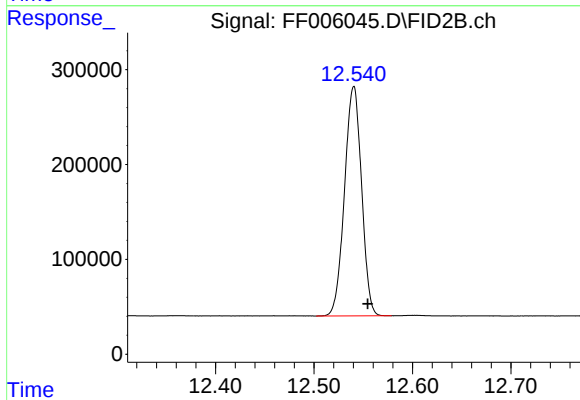


#7 N-EICOSANE

R.T.: 12.540 min
Delta R.T.: -0.014 min
Response: 2911418
Conc: 16.86 ug/ml

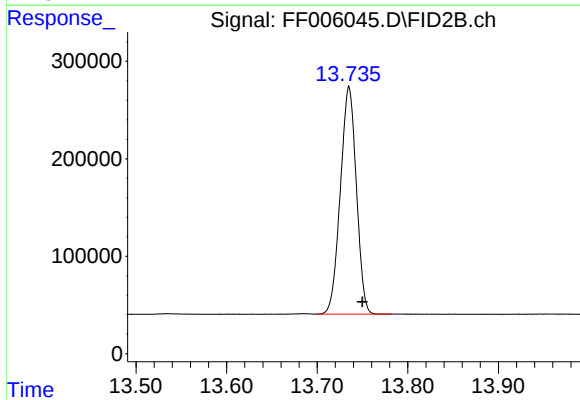


#8 N-DOCOSANE

R.T.: 13.735 min
Delta R.T.: -0.015 min
Response: 2864675
Conc: 16.83 ug/ml

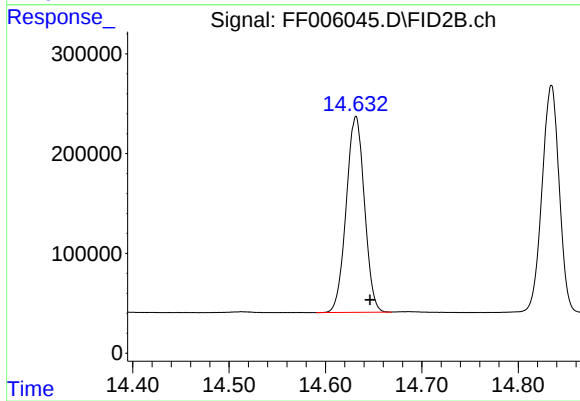

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.632 min
Delta R.T.: -0.015 min
Response: 2571010
Conc: 17.70 ug/ml

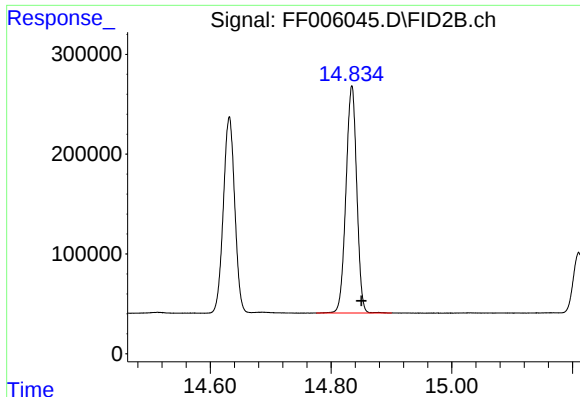

#10 N-TETRACOSANE


R.T.: 14.835 min
Delta R.T.: -0.016 min
Response: 2823576
Conc: 16.92 ug/ml

Instrument :
FID_F
ClientSampleId :
SSI-MW-4MS

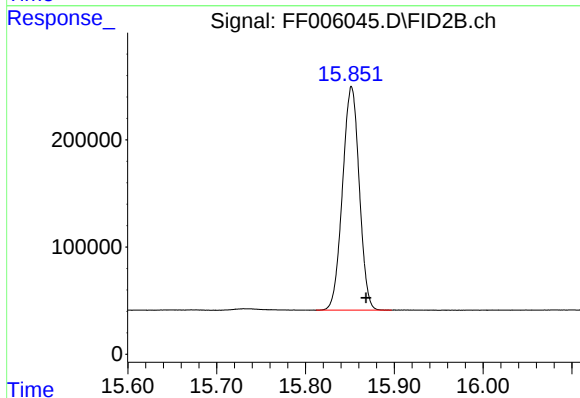

#11 N-HEXACOSANE

R.T.: 15.852 min
Delta R.T.: -0.016 min
Response: 2731414
Conc: 16.96 ug/ml

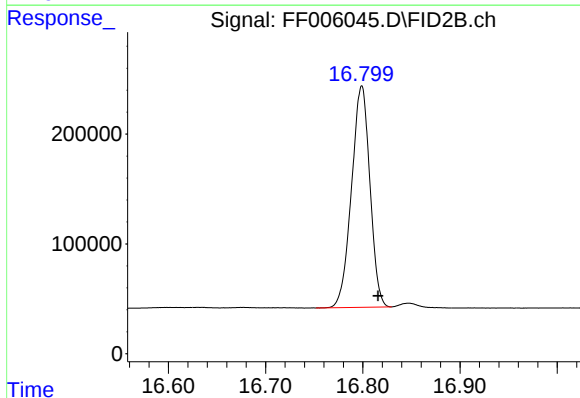

#12 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: -0.017 min
Response: 2650835
Conc: 17.28 ug/ml