

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121823\
Data File : FF013888.D
Signal(s) : FID2B.ch
Acq On : 18 Dec 2023 08:41
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 18 23:19:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
15) N-TETRATRIACONTANE	19.624	41920	0.428 ug/ml
18) N-TETRACONTANE	22.034	146141	1.871 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121823\
Data File : FF013888.D
Signal(s) : FID2B.ch
Acq On : 18 Dec 2023 08:41
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 18 23:19:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

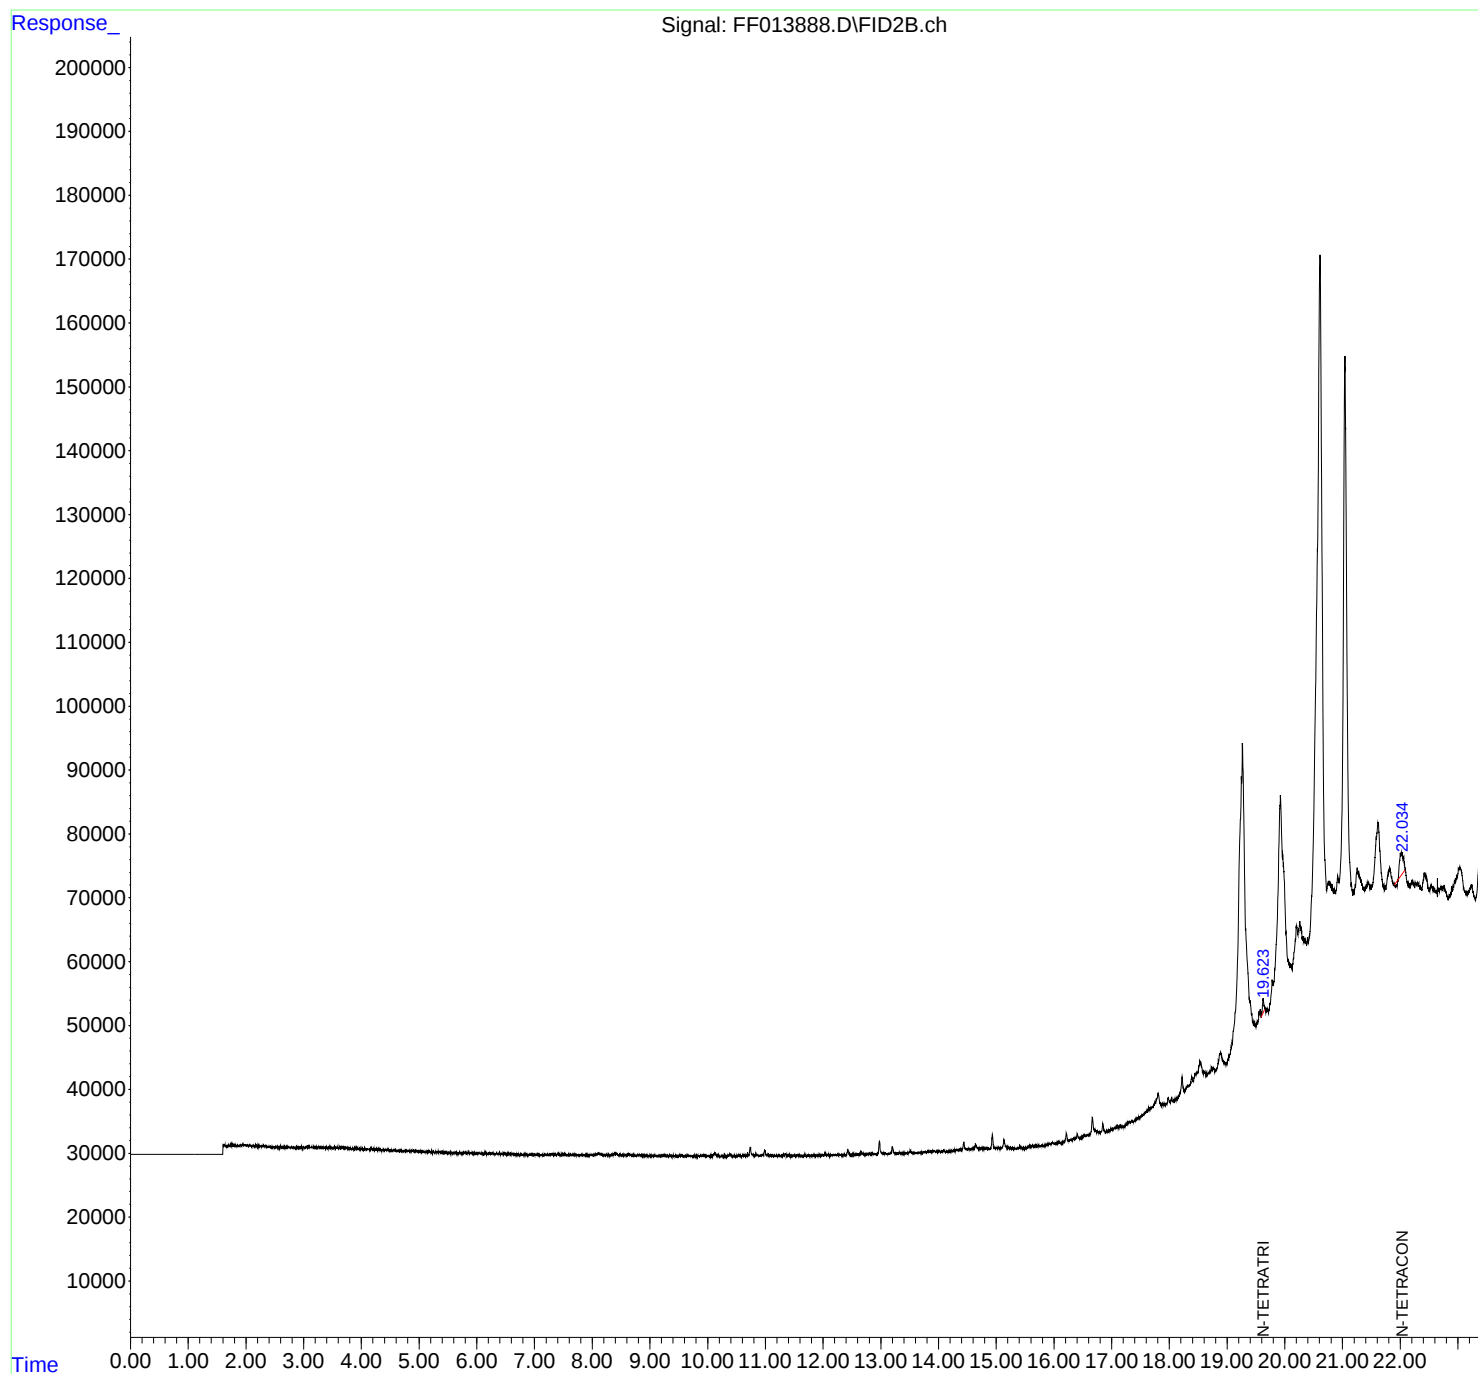


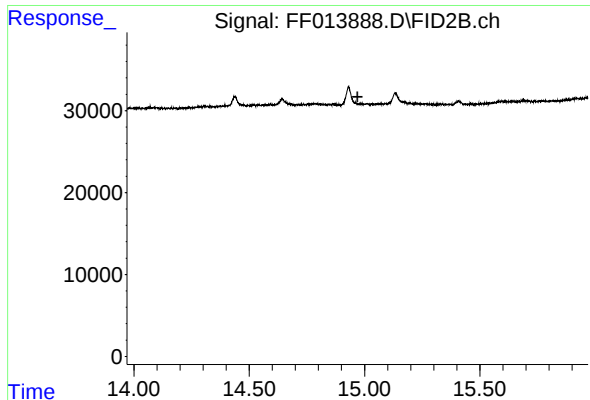

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.969 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

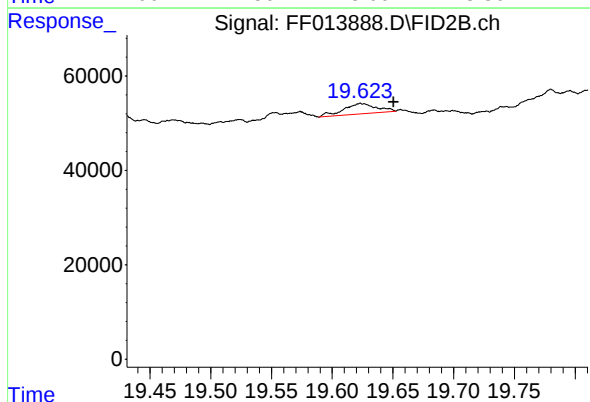

#15 N-TETRATRIACONTANE

R.T.: 19.624 min
Delta R.T.: -0.027 min
Response: 41920
Conc: 0.43 ug/ml

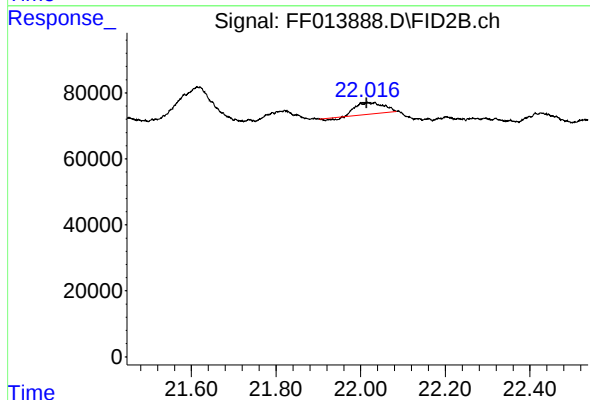

#18 N-TETRACONTANE

R.T.: 22.034 min
Delta R.T.: 0.019 min
Response: 146141
Conc: 1.87 ug/ml