

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121823\
 Data File : FF013897.D
 Signal(s) : FID2B.ch
 Acq On : 18 Dec 2023 13:41
 Operator : YP\AJ
 Sample : PB1587845BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 18 23:20:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
 Quant Title :
 QLast Update : Tue Dec 05 11:16:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.969	2491735	21.086 ug/ml
Target Compounds			
12) N-OCTACOSANE	17.145	68496	0.577 ug/ml
13) N-TRIACONTANE	18.035	132966	1.133 ug/ml
14) N-DOTRIACONTANE	18.867	152566	1.345 ug/ml
15) N-TETRATRIACONTANE	19.651	141760	1.446 ug/ml
16) N-HEXATRIACONTANE	20.393	101145	1.257 ug/ml
18) N-TETRACONTANE	22.017	53238	0.682 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121823\
Data File : FF013897.D
Signal(s) : FID2B.ch
Acq On : 18 Dec 2023 13:41
Operator : YP\AJ
Sample : PB1587845BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 18 23:20:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120523.M
Quant Title :
QLast Update : Tue Dec 05 11:16:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

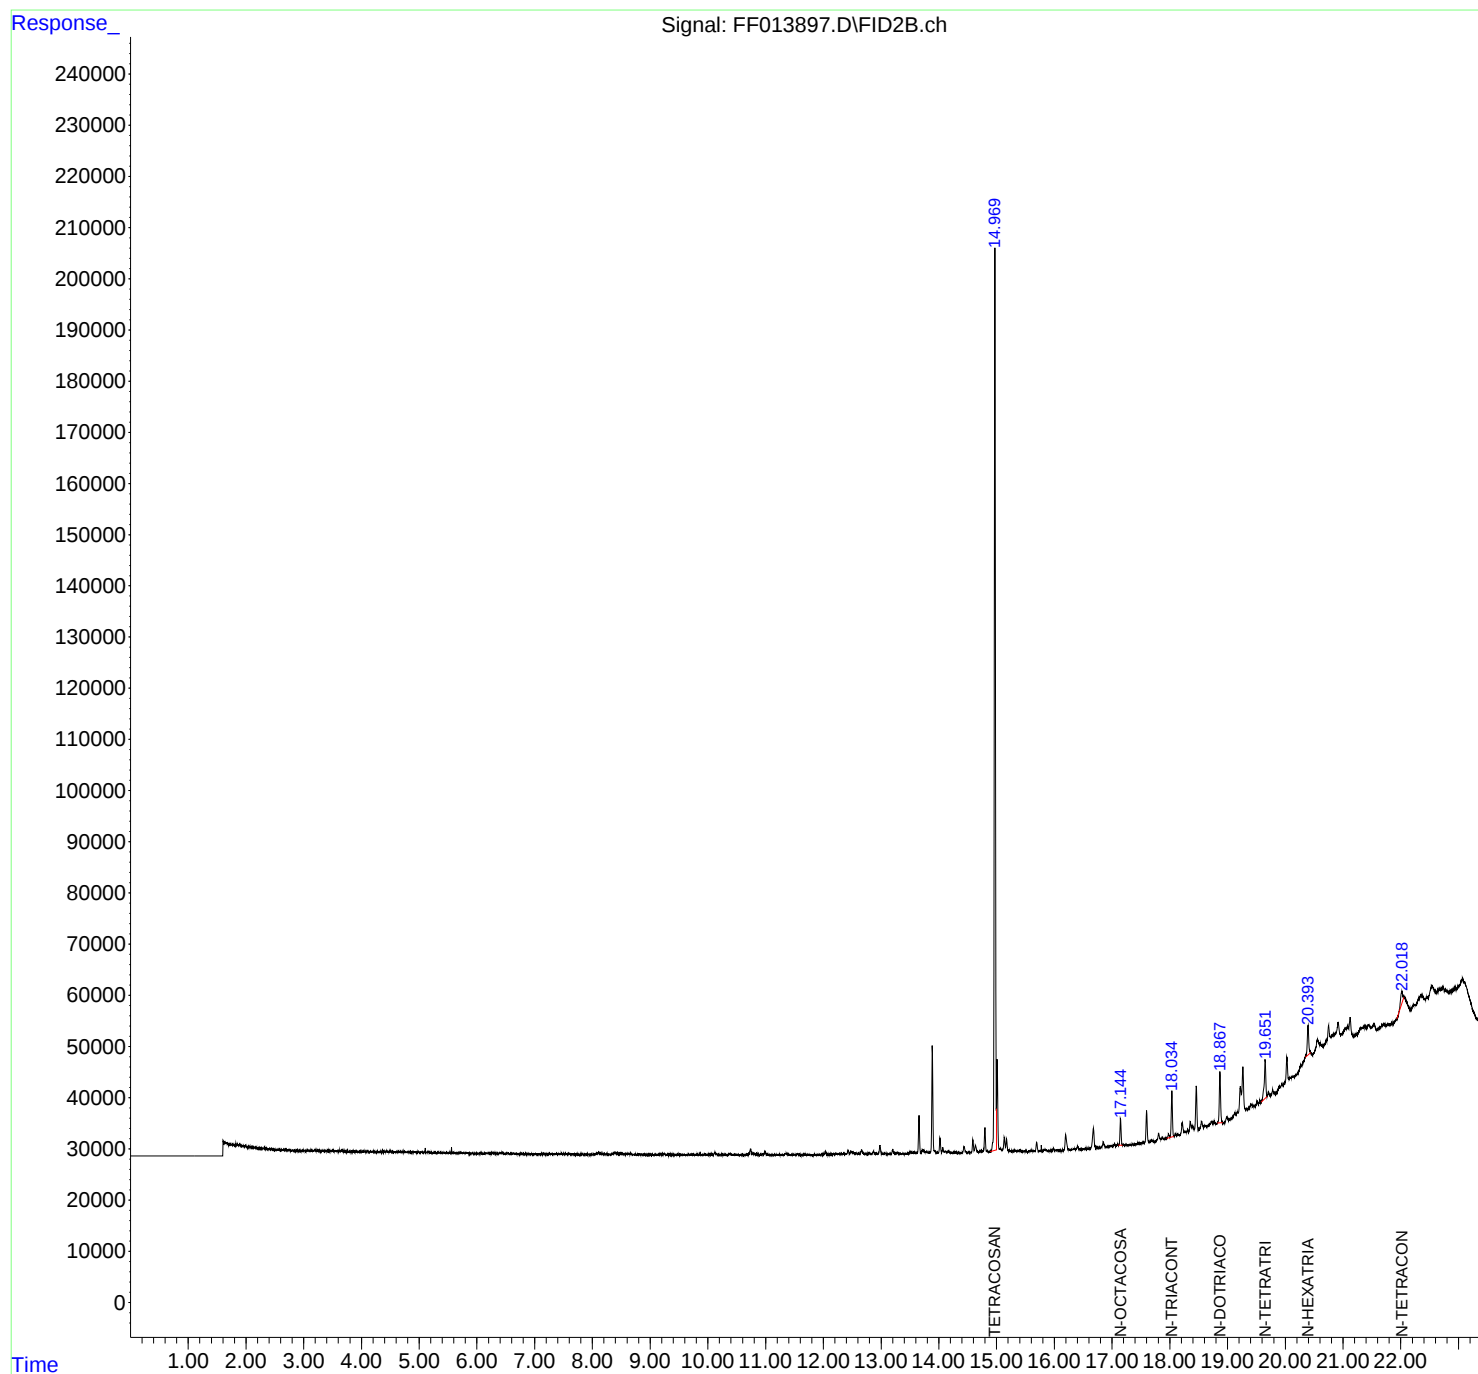


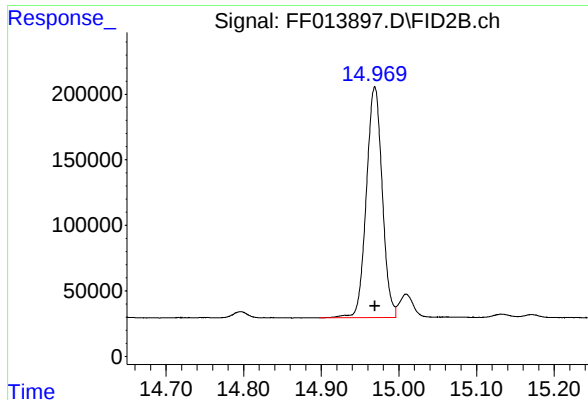

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.969 min
Delta R.T.: 0.000 min
Response: 2491735
Conc: 21.09 ug/ml

Instrument : FID_F
ClientSampleId :

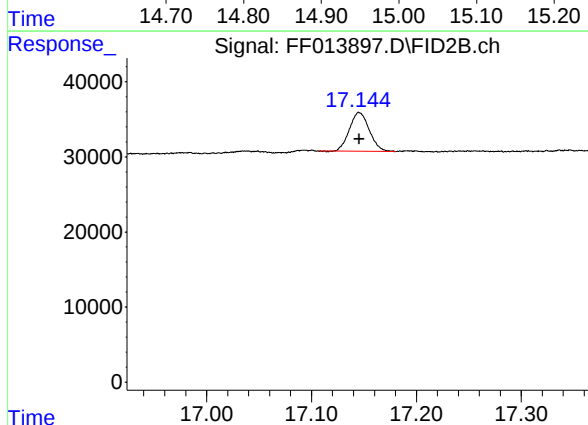


#12 N-OCTACOSANE

R.T.: 17.145 min
Delta R.T.: 0.000 min
Response: 68496
Conc: 0.58 ug/ml

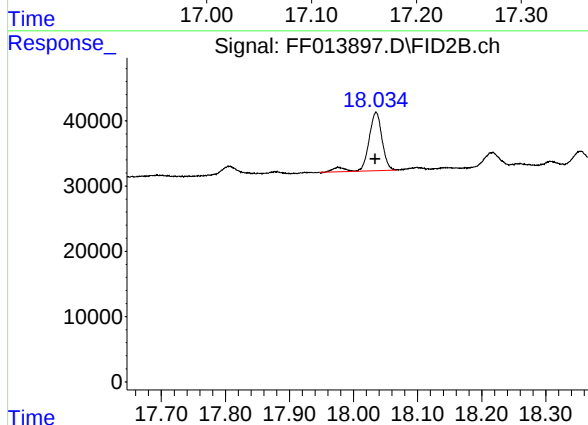


#13 N-TRIACONTANE

R.T.: 18.035 min
Delta R.T.: 0.001 min
Response: 132966
Conc: 1.13 ug/ml

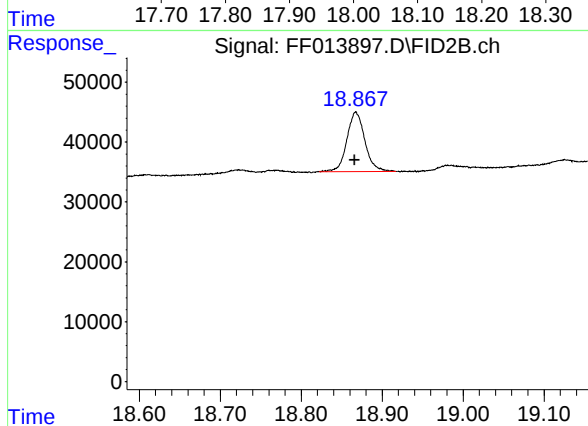

#14 N-DOTRIACONTANE


R.T.: 18.867 min
Delta R.T.: 0.001 min
Response: 152566
Conc: 1.35 ug/ml

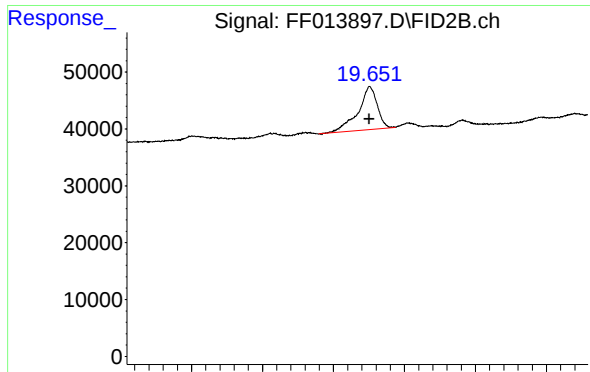

#15 N-TETRATRIACONTANE


R.T.: 19.651 min
Delta R.T.: 0.000 min
Response: 141760
Conc: 1.45 ug/ml

Instrument :
FID_F
ClientSampleId :

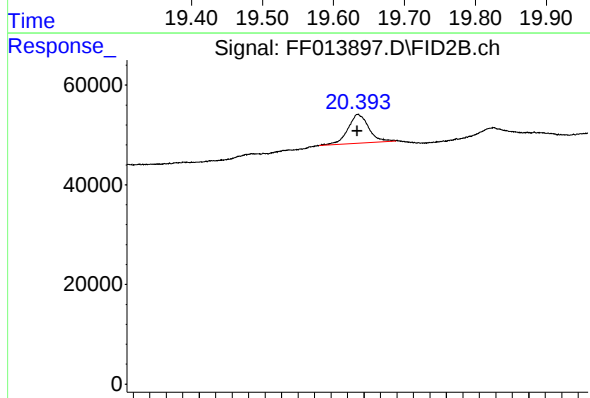

#16 N-HEXATRIACONTANE

R.T.: 20.393 min
Delta R.T.: 0.000 min
Response: 101145
Conc: 1.26 ug/ml

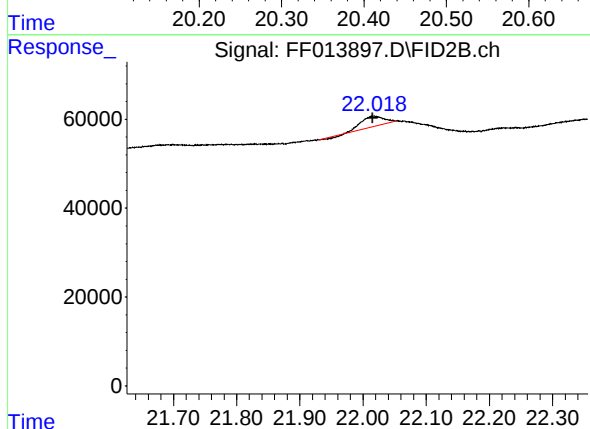

#18 N-TETRACONTANE

R.T.: 22.017 min
Delta R.T.: 0.002 min
Response: 53238
Conc: 0.68 ug/ml