

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121918\
 Data File : FF003045.D
 Signal(s) : FID2B.ch
 Acq On : 19 Dec 2018 16:18
 Operator : AJ\SJ
 Sample : J6199-09 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 20 00:34:48 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	175663	1.353 ug/ml
Target Compounds			
3) N-DODECANE	6.383	88297	0.556 ug/ml
4) N-TETRADECANE	8.176	133136	0.831 ug/ml
5) N-HEXADECANE	9.776	146676	0.916 ug/ml
6) N-OCTADECANE	11.219	107353	0.678 ug/ml
7) N-EICOSANE	12.531	96687	0.627 ug/ml
8) N-DOCOSANE	13.733	60457	0.404 ug/ml
10) N-TETRACOSANE	14.810	104558	0.724 ug/ml
11) N-HEXACOSANE	15.861	115194	0.825 ug/ml
12) N-OCTACOSANE	16.814	154877	1.156 ug/ml
13) N-TRIACONTANE	17.703	250673	1.956 ug/ml
14) N-DOTRIACONTANE	18.541	261032	2.186 ug/ml
15) N-TETRATRIACONTANE	19.326	94531	0.834 ug/ml
16) N-HEXATRIACONTANE	20.069	39581	0.367 ug/ml
18) N-TETRACONTANE	21.742	758171	7.213 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF121918\
Data File : FF003045.D
Signal(s) : FID2B.ch
Acq On : 19 Dec 2018 16:18
Operator : AJ\SJ
Sample : J6199-09 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 20 00:34:48 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

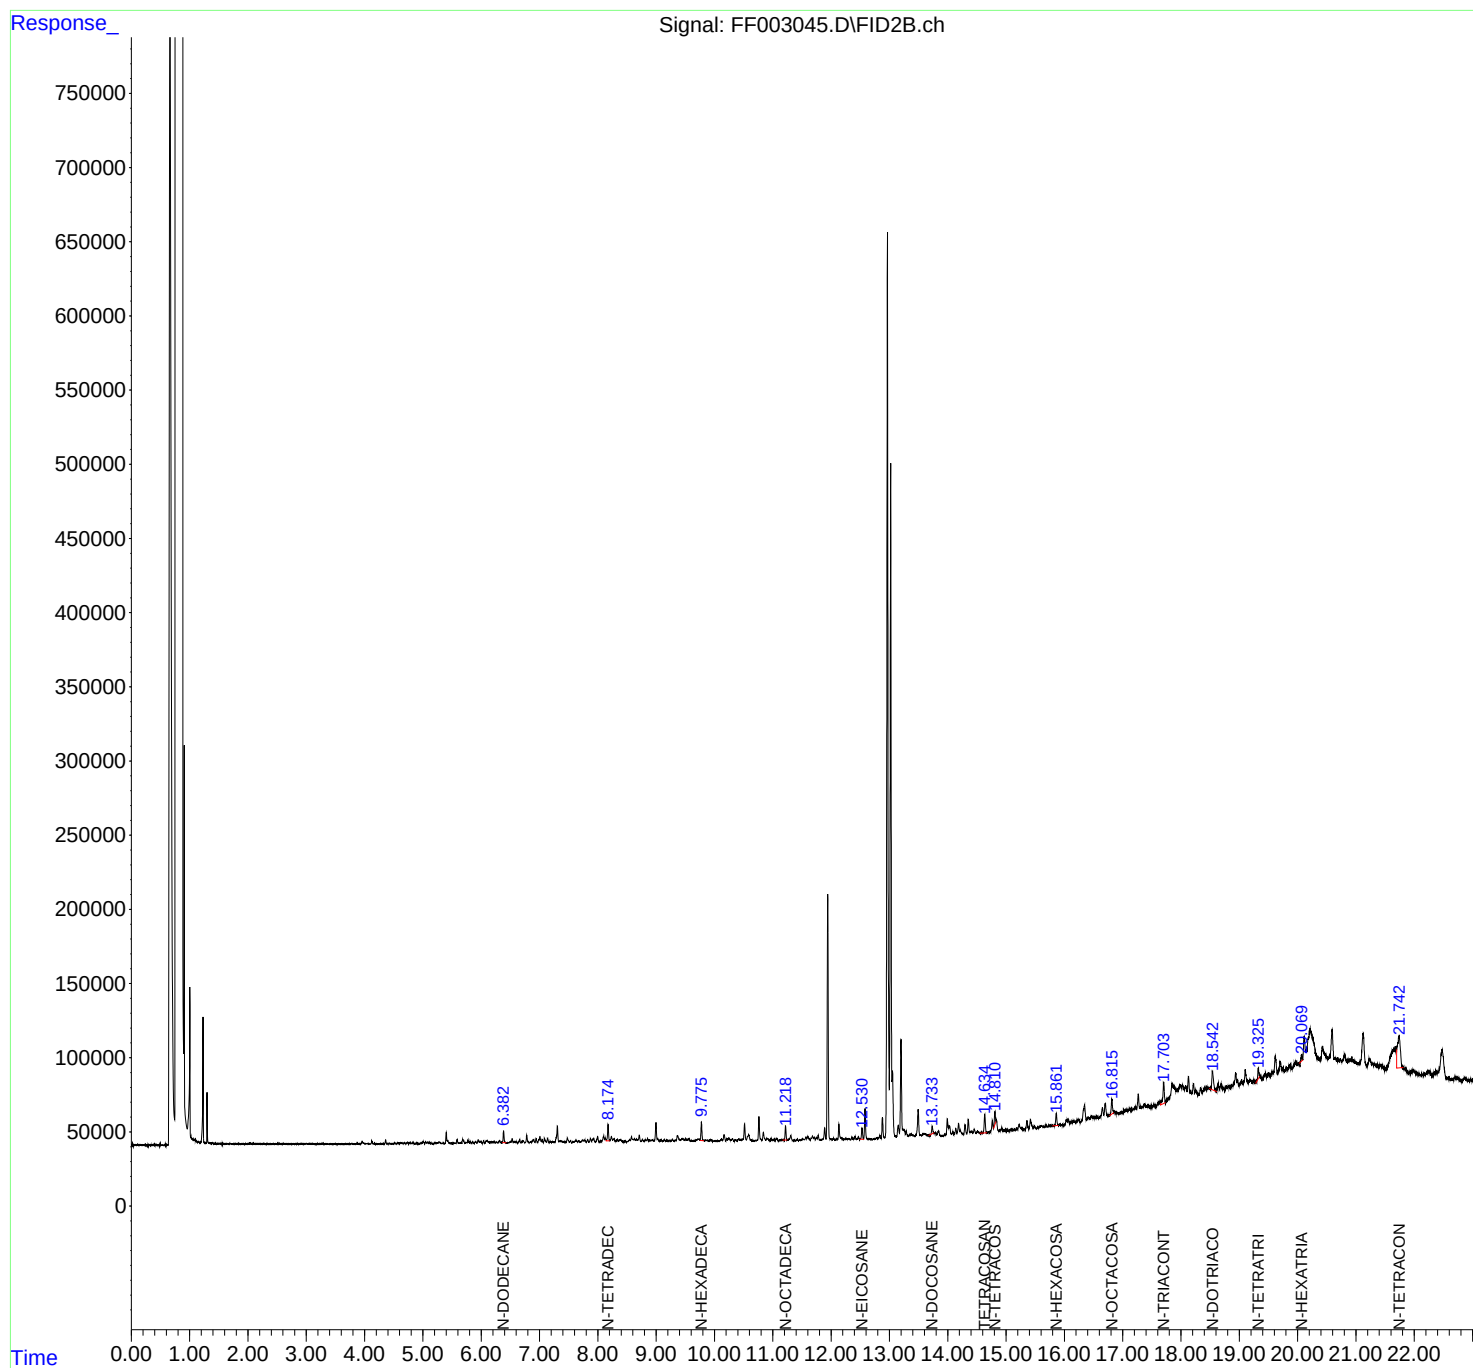

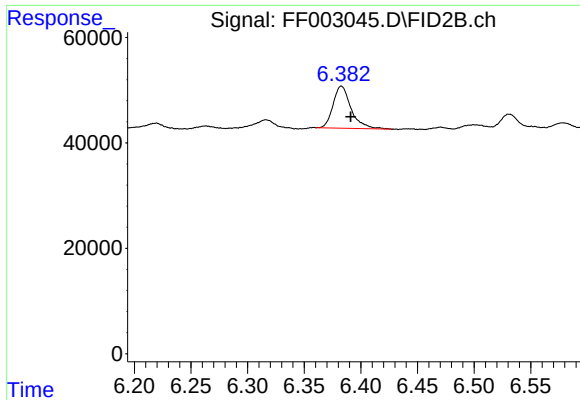


#3 N-DODECANE

R.T.: 6.383 min
Delta R.T.: -0.008 min
Response: 88297
Conc: 0.56 ug/ml

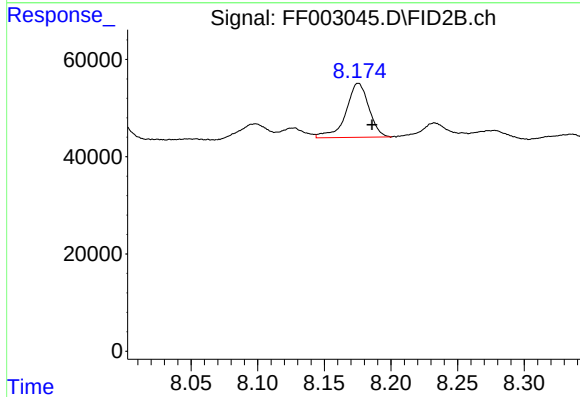


#4 N-TETRADECANE

R.T.: 8.176 min
Delta R.T.: -0.010 min
Response: 133136
Conc: 0.83 ug/ml

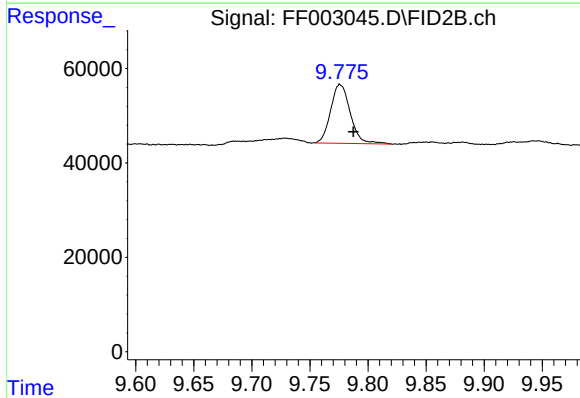


#5 N-HEXADECANE

R.T.: 9.776 min
Delta R.T.: -0.012 min
Response: 146676
Conc: 0.92 ug/ml

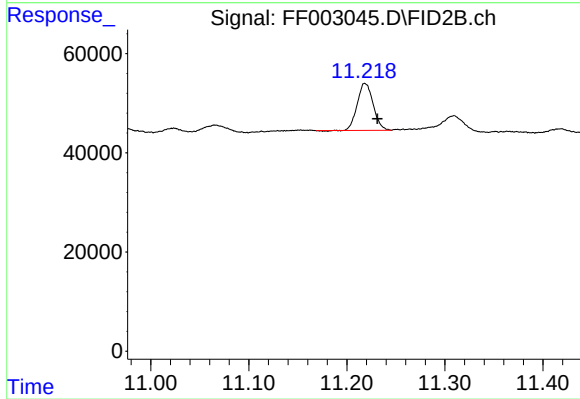


#6 N-OCTADECANE

R.T.: 11.219 min
Delta R.T.: -0.013 min
Response: 107353
Conc: 0.68 ug/ml

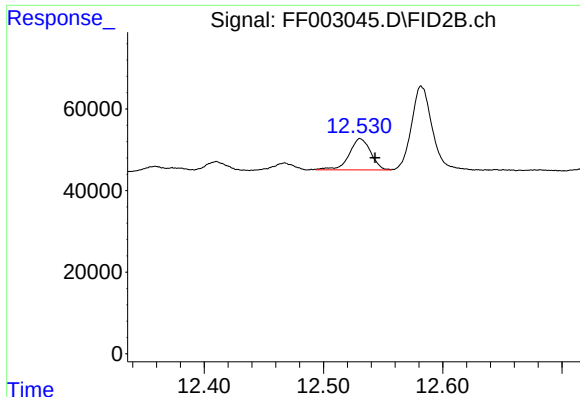


#7 N-EICOSANE

R.T.: 12.531 min
Delta R.T.: -0.012 min
Response: 96687
Conc: 0.63 ug/ml

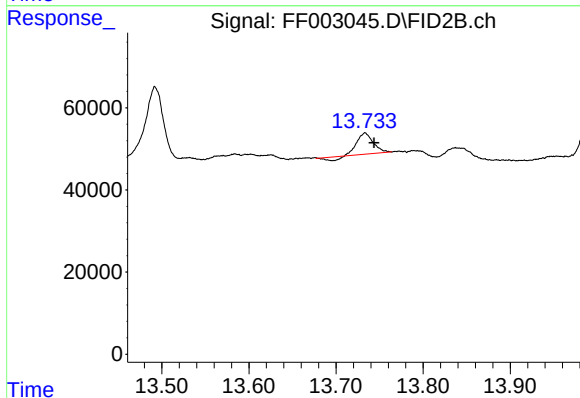


#8 N-DOCOSANE

R.T.: 13.733 min
Delta R.T.: -0.010 min
Response: 60457
Conc: 0.40 ug/ml

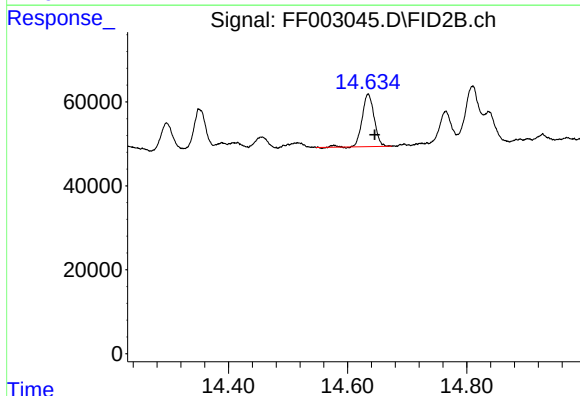


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.635 min
Delta R.T.: -0.011 min
Response: 175663
Conc: 1.35 ug/ml

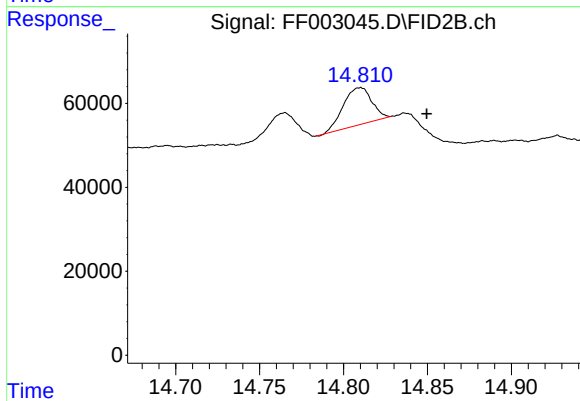


#10 N-TETRACOSANE

R.T.: 14.810 min
Delta R.T.: -0.040 min
Response: 104558
Conc: 0.72 ug/ml

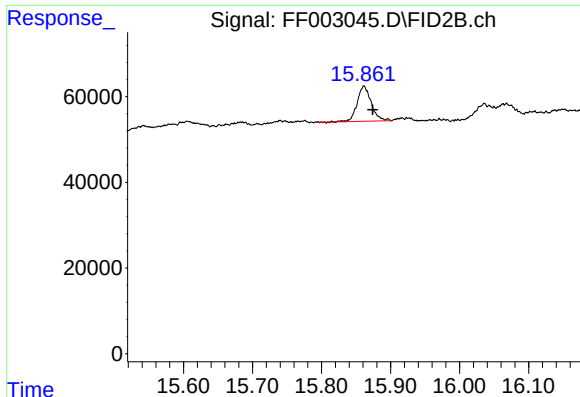


#11 N-HEXACOSANE

R.T.: 15.861 min
Delta R.T.: -0.013 min
Response: 115194
Conc: 0.83 ug/ml

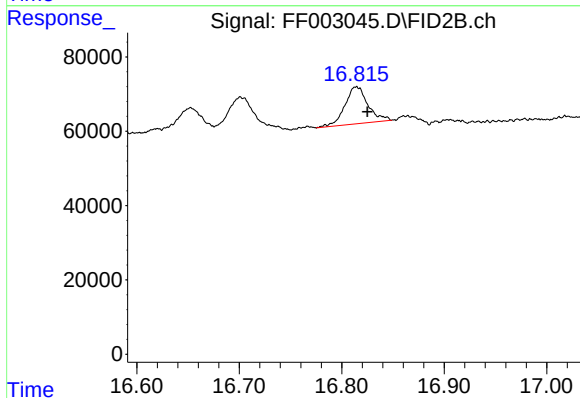


#12 N-OCTACOSANE

R.T.: 16.814 min
Delta R.T.: -0.011 min
Response: 154877
Conc: 1.16 ug/ml

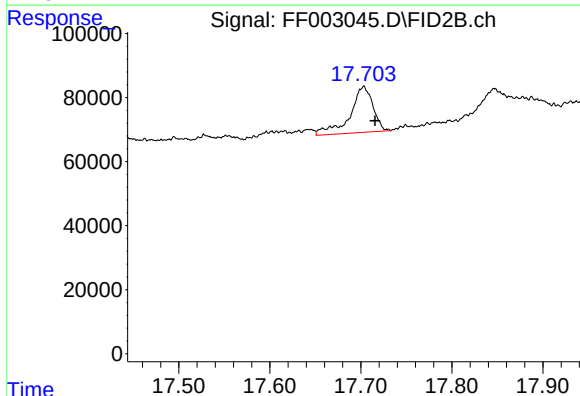


#13 N-TRIACONTANE

R.T.: 17.703 min
Delta R.T.: -0.012 min
Response: 250673
Conc: 1.96 ug/ml

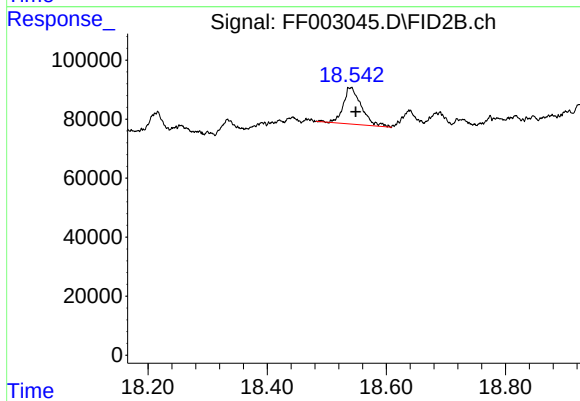


#14 N-DOTRIACONTANE

R.T.: 18.541 min
Delta R.T.: -0.007 min
Response: 261032
Conc: 2.19 ug/ml

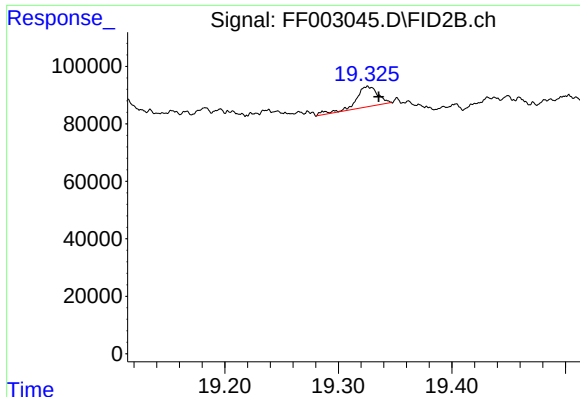


#15 N-TETRATRIACONTANE

R.T.: 19.326 min
Delta R.T.: -0.010 min
Response: 94531
Conc: 0.83 ug/ml

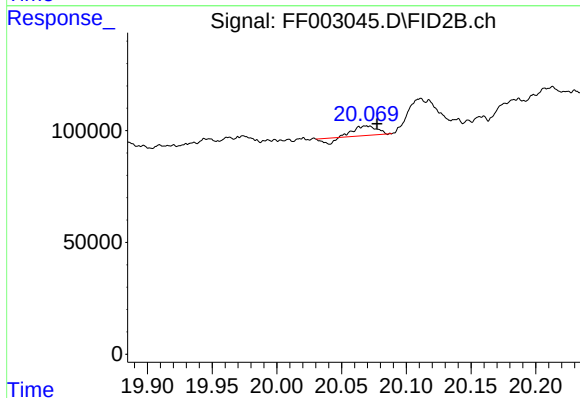

#16 N-HEXATRIACONTANE

R.T.: 20.069 min
Delta R.T.: -0.008 min
Response: 39581
Conc: 0.37 ug/ml

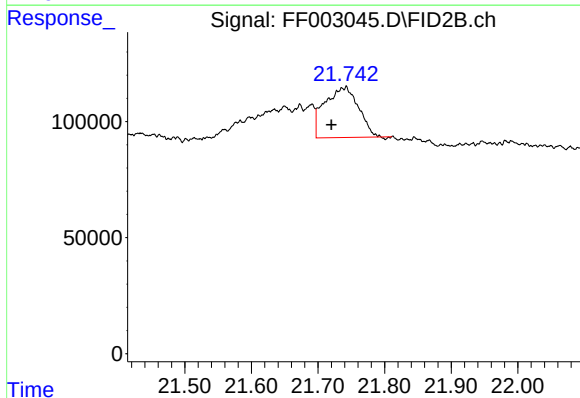

#18 N-TETRACONTANE

R.T.: 21.742 min
Delta R.T.: 0.022 min
Response: 758171
Conc: 7.21 ug/ml