

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF122018\
 Data File : FF003054.D
 Signal(s) : FID2B.ch
 Acq On : 20 Dec 2018 12:03
 Operator : AJ\SJ
 Sample : J6196-11 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 20 15:11:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.634	327250	2.521 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.176	78208	0.488 ug/ml
5)	N-HEXADECANE	9.777	90786	0.567 ug/ml
6)	N-OCTADECANE	11.220	85481	0.540 ug/ml
7)	N-EICOSANE	12.531	99650	0.646 ug/ml
10)	N-TETRACOSANE	14.807	345999	2.394 ug/ml
11)	N-HEXACOSANE	15.863	118957	0.852 ug/ml
12)	N-OCTACOSANE	16.813	257695	1.923 ug/ml
13)	N-TRIACONTANE	17.706	431885	3.371 ug/ml
14)	N-DOTRIACONTANE	18.541	233818	1.958 ug/ml
15)	N-TETRATRIACONTANE	19.328	77166	0.681 ug/ml
16)	N-HEXATRIACONTANE	20.075	138658	1.285 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : \\TERASTORAGE\Terastorage\pestpcbsrv\HPCHEM1\FID_F\Data\FF122018\
Data File : FF003054.D
Signal(s) : FID2B.ch
Acq On : 20 Dec 2018 12:03
Operator : AJ\SJ
Sample : J6196-11 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 20 15:11:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

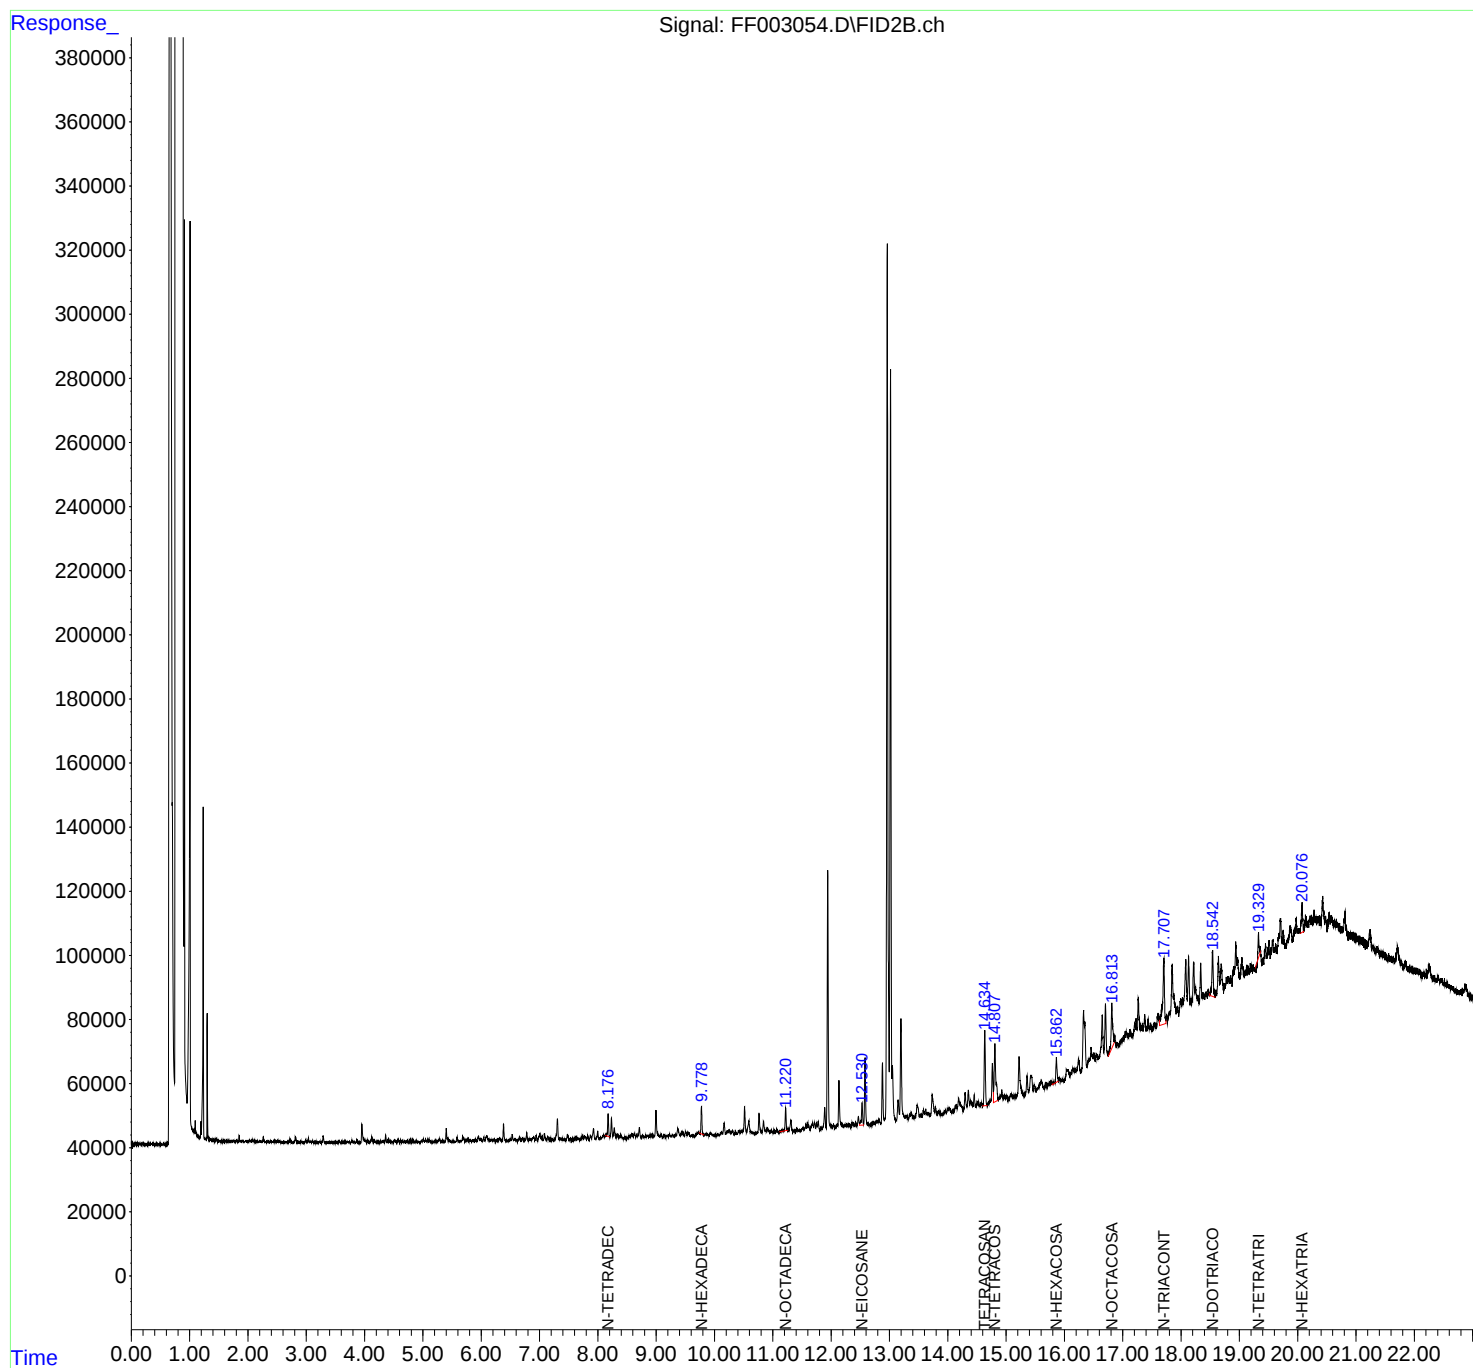

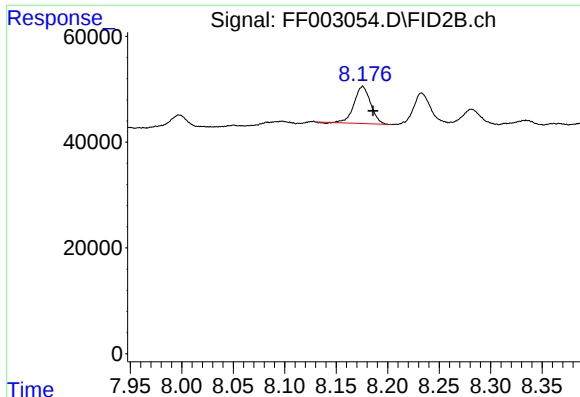


#4 N-TETRADECANE

R.T.: 8.176 min
Delta R.T.: -0.010 min
Response: 78208
Conc: 0.49 ug/ml

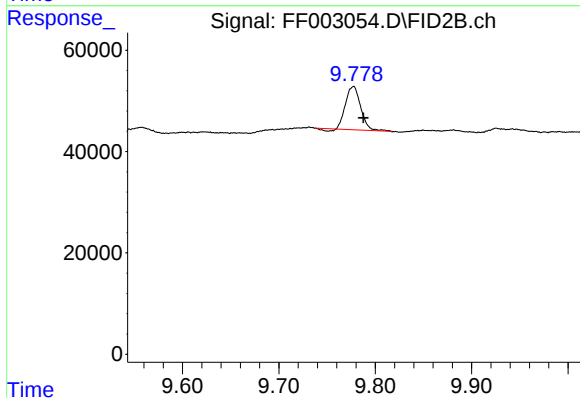


#5 N-HEXADECANE

R.T.: 9.777 min
Delta R.T.: -0.010 min
Response: 90786
Conc: 0.57 ug/ml

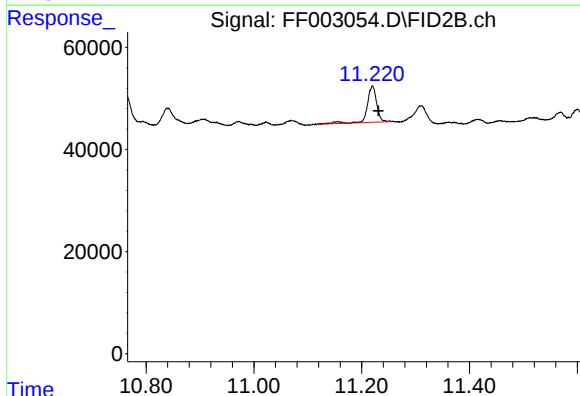


#6 N-OCTADECANE

R.T.: 11.220 min
Delta R.T.: -0.011 min
Response: 85481
Conc: 0.54 ug/ml

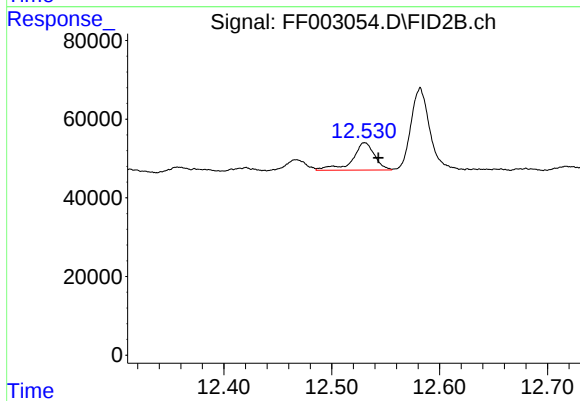


#7 N-EICOSANE

R.T.: 12.531 min
Delta R.T.: -0.013 min
Response: 99650
Conc: 0.65 ug/ml

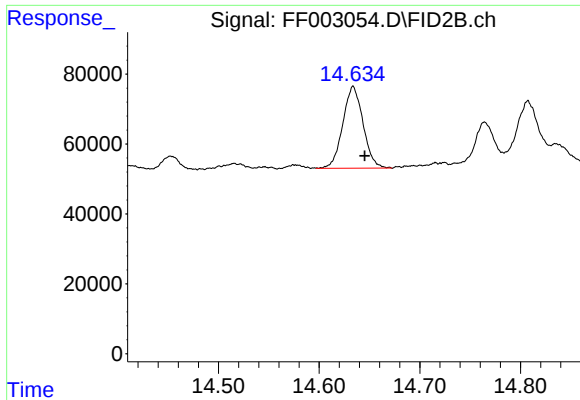


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.634 min
Delta R.T.: -0.012 min
Response: 327250
Conc: 2.52 ug/ml

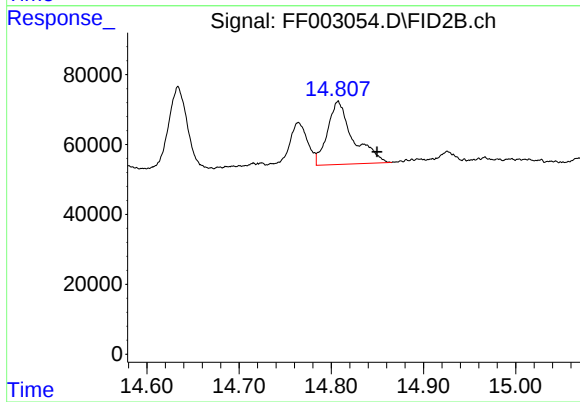


#10 N-TETRACOSANE

R.T.: 14.807 min
Delta R.T.: -0.042 min
Response: 345999
Conc: 2.39 ug/ml

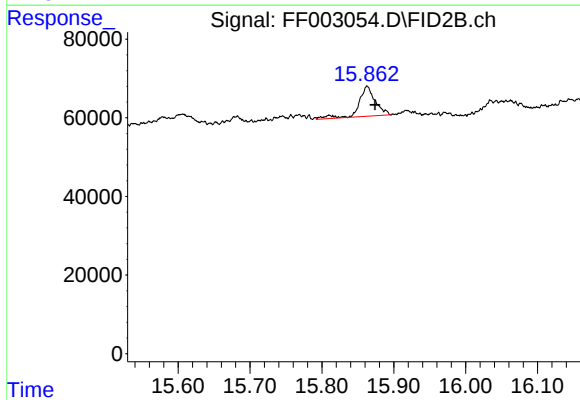


#11 N-HEXACOSANE

R.T.: 15.863 min
Delta R.T.: -0.011 min
Response: 118957
Conc: 0.85 ug/ml

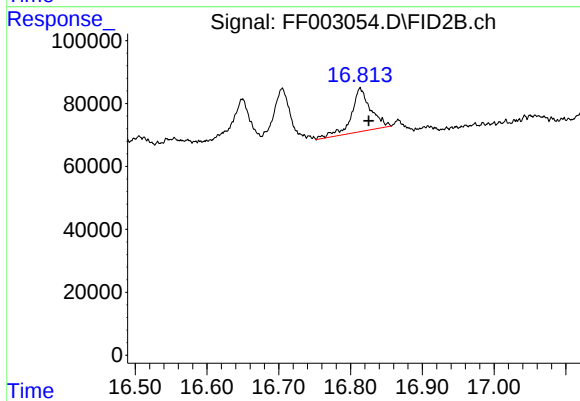


#12 N-OCTACOSANE

R.T.: 16.813 min
Delta R.T.: -0.012 min
Response: 257695
Conc: 1.92 ug/ml

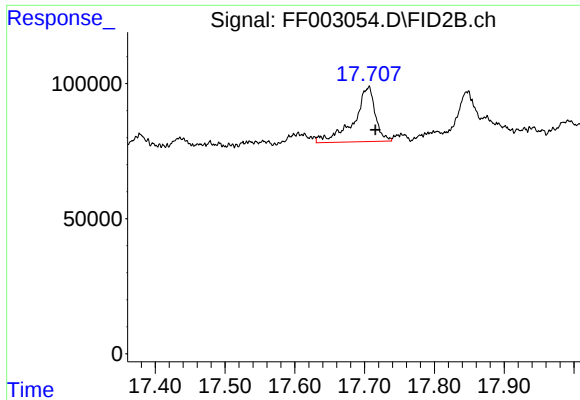


#13 N-TRIACONTANE

R.T.: 17.706 min
Delta R.T.: -0.009 min
Response: 431885
Conc: 3.37 ug/ml

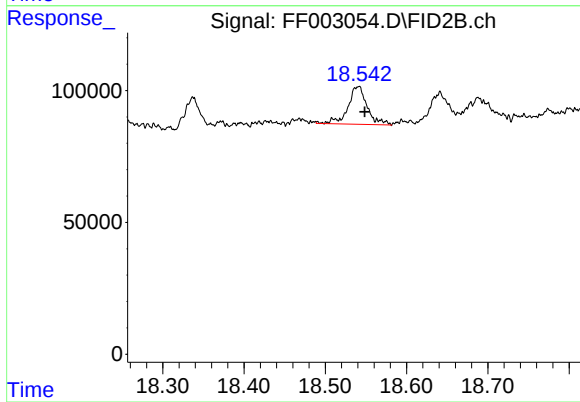


#14 N-DOTRIACONTANE

R.T.: 18.541 min
Delta R.T.: -0.007 min
Response: 233818
Conc: 1.96 ug/ml

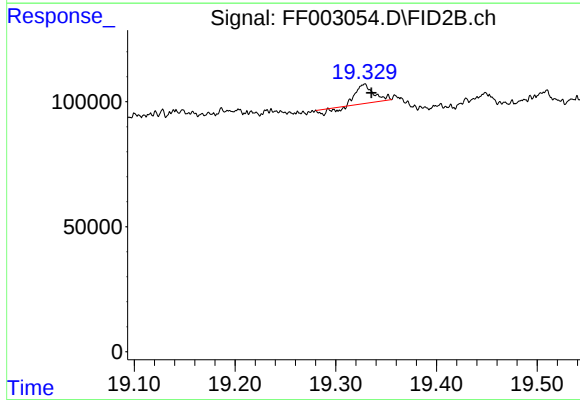

#15 N-TETRATRIACONTANE

R.T.: 19.328 min
Delta R.T.: -0.007 min
Response: 77166
Conc: 0.68 ug/ml

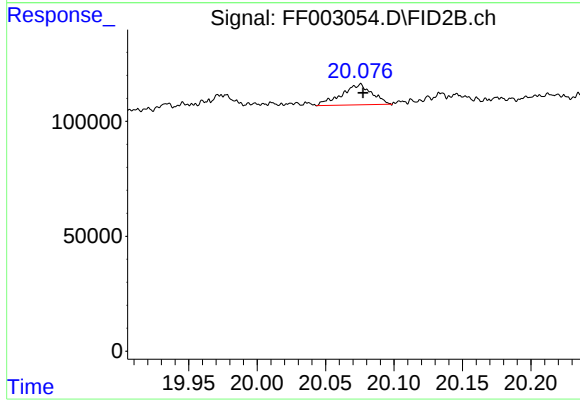

#16 N-HEXATRIACONTANE

R.T.: 20.075 min
Delta R.T.: -0.002 min
Response: 138658
Conc: 1.29 ug/ml