

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122021\
 Data File : FF009480.D
 Signal(s) : FID2B.ch
 Acq On : 20 Dec 2021 14:00
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 21 00:02:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.266	2674245	18.492 ug/ml
12) N-OCTACOSANE	16.643	2219036	18.635 ug/ml
13) N-TRIACONTANE	17.526	166121	1.450 ug/ml
14) N-DOTRIACONTANE	18.354	205927	1.884 ug/ml
15) N-TETRATRIACONTANE	19.135	172260	1.626 ug/ml
16) N-HEXATRIACONTANE	19.873	116253	1.161 ug/ml
17) N-OCTATRIACONTANE	20.579	66024	0.672 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122021\
Data File : FF009480.D
Signal(s) : FID2B.ch
Acq On : 20 Dec 2021 14:00
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 21 00:02:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

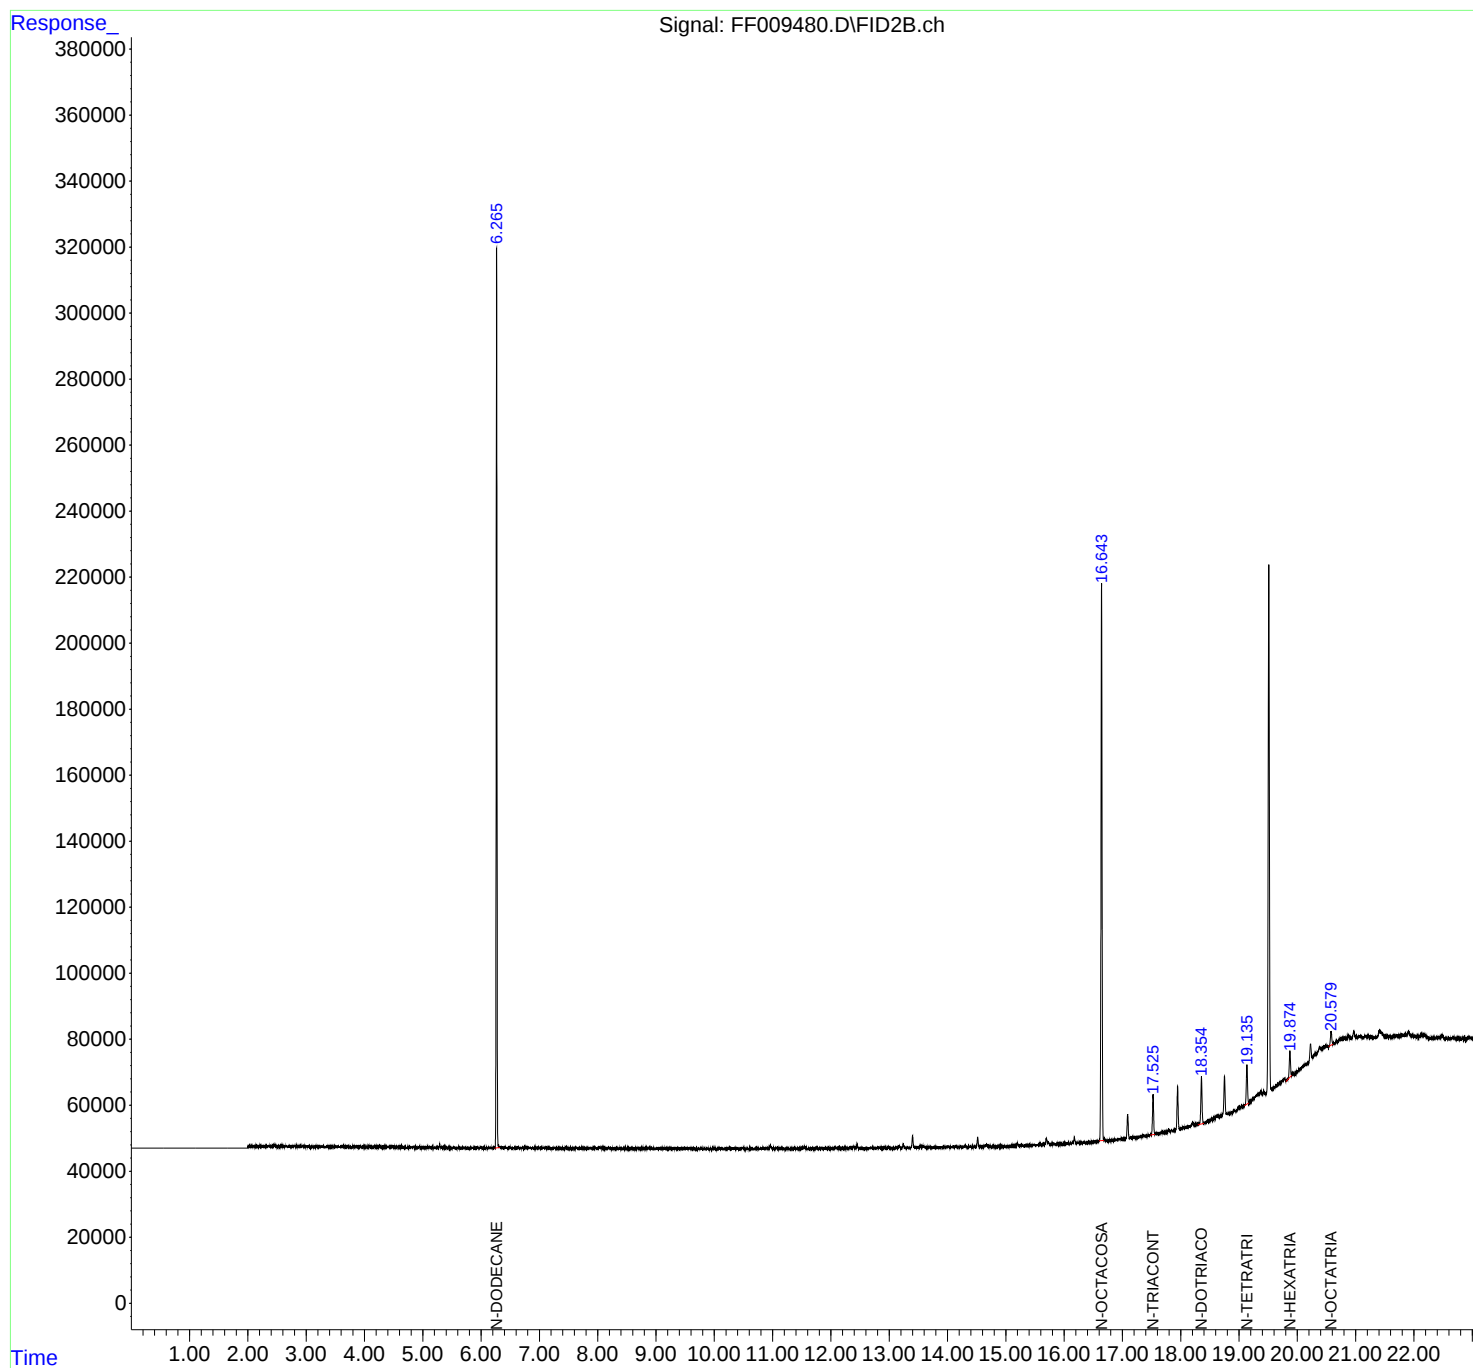


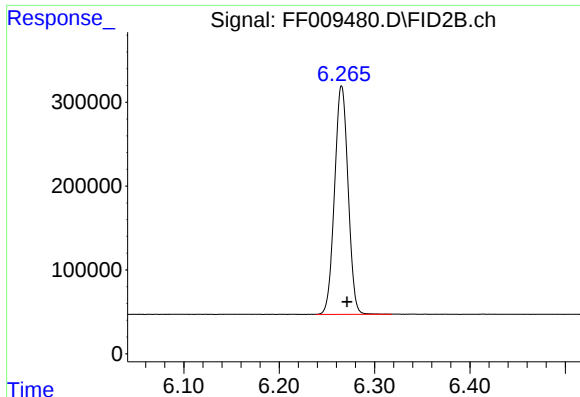

#3 N-DODECANE


R.T.: 6.266 min
Delta R.T.: -0.006 min
Response: 2674245
Conc: 18.49 ug/ml

Instrument :
FID_F
ClientSampleId :

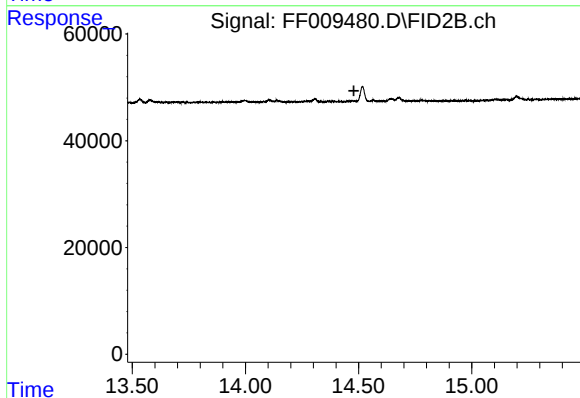


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

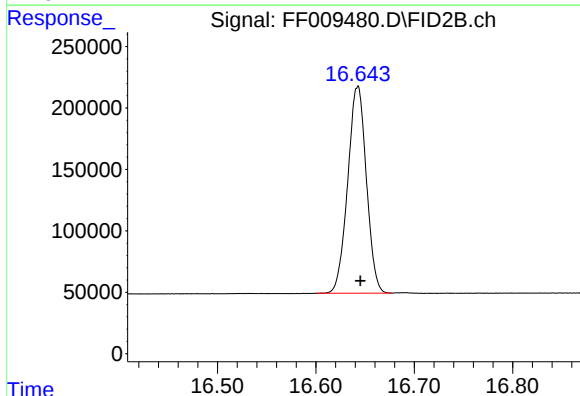


#12 N-OCTACOSANE

R.T.: 16.643 min
Delta R.T.: -0.002 min
Response: 2219036
Conc: 18.64 ug/ml

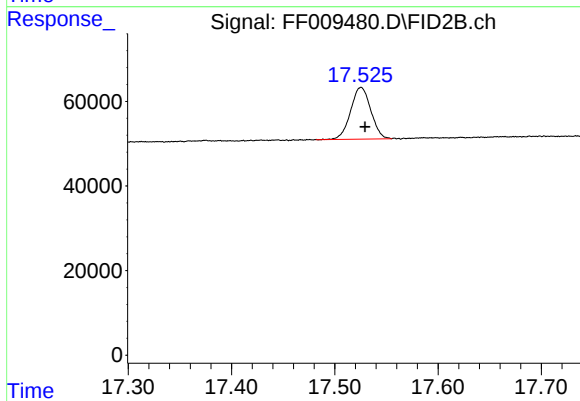

#13 N-TRIACONTANE


R.T.: 17.526 min
Delta R.T.: -0.003 min
Response: 166121
Conc: 1.45 ug/ml

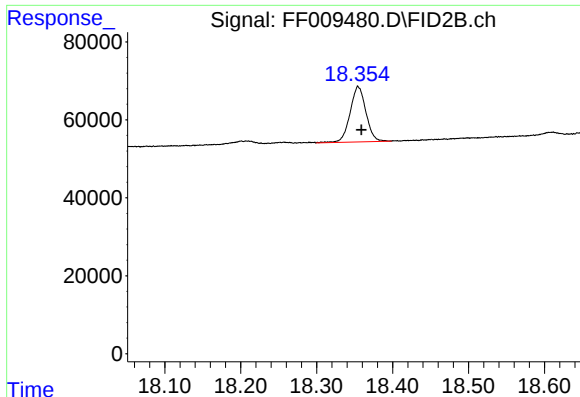

#14 N-DOTRIACONTANE


R.T.: 18.354 min
Delta R.T.: -0.005 min
Response: 205927
Conc: 1.88 ug/ml

Instrument :
FID_F
ClientSampleId :

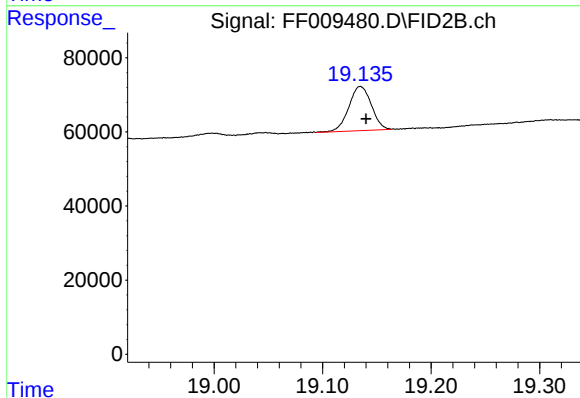


#15 N-TETRATRIACONTANE

R.T.: 19.135 min
Delta R.T.: -0.005 min
Response: 172260
Conc: 1.63 ug/ml

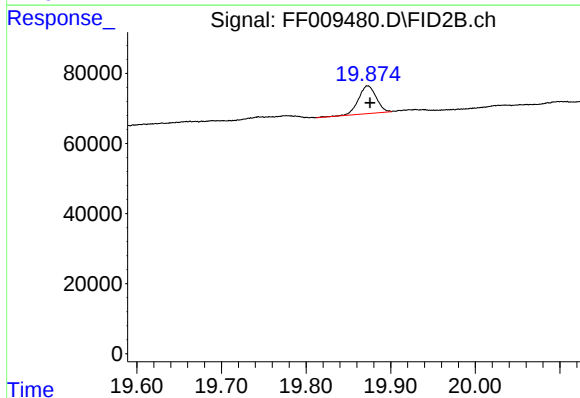

#16 N-HEXATRIACONTANE

R.T.: 19.873 min
Delta R.T.: -0.002 min
Response: 116253
Conc: 1.16 ug/ml

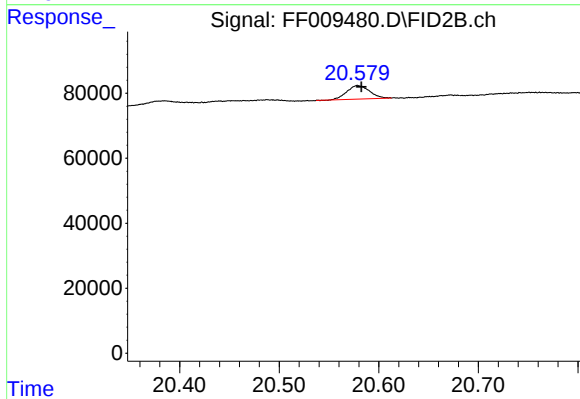

#17 N-OCTATRIACONTANE

R.T.: 20.579 min
Delta R.T.: -0.004 min
Response: 66024
Conc: 0.67 ug/ml