

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
 Data File : FF003066.D
 Signal(s) : FID2B.ch
 Acq On : 21 Dec 2018 17:47
 Operator : AJ\SJ
 Sample : J6492-02
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 21 22:11:42 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	1989667	15.326 ug/ml
Target Compounds			
3) N-DODECANE	6.399	423817	2.669 ug/ml
4) N-TETRADECANE	8.150	374520	2.337 ug/ml
5) N-HEXADECANE	9.800	601210	3.754 ug/ml
6) N-OCTADECANE	11.274	185154	1.169 ug/ml
7) N-EICOSANE	12.581	126468	0.820 ug/ml
10) N-TETRACOSANE	14.813	200366	1.386 ug/ml
12) N-OCTACOSANE	16.815	254145	1.897 ug/ml
13) N-TRIACONTANE	17.706	363709	2.839 ug/ml
14) N-DOTRIACONTANE	18.543	220600	1.847 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
Data File : FF003066.D
Signal(s) : FID2B.ch
Acq On : 21 Dec 2018 17:47
Operator : AJ\SJ
Sample : J6492-02
Misc :
ALS Vial : 59 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 21 22:11:42 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

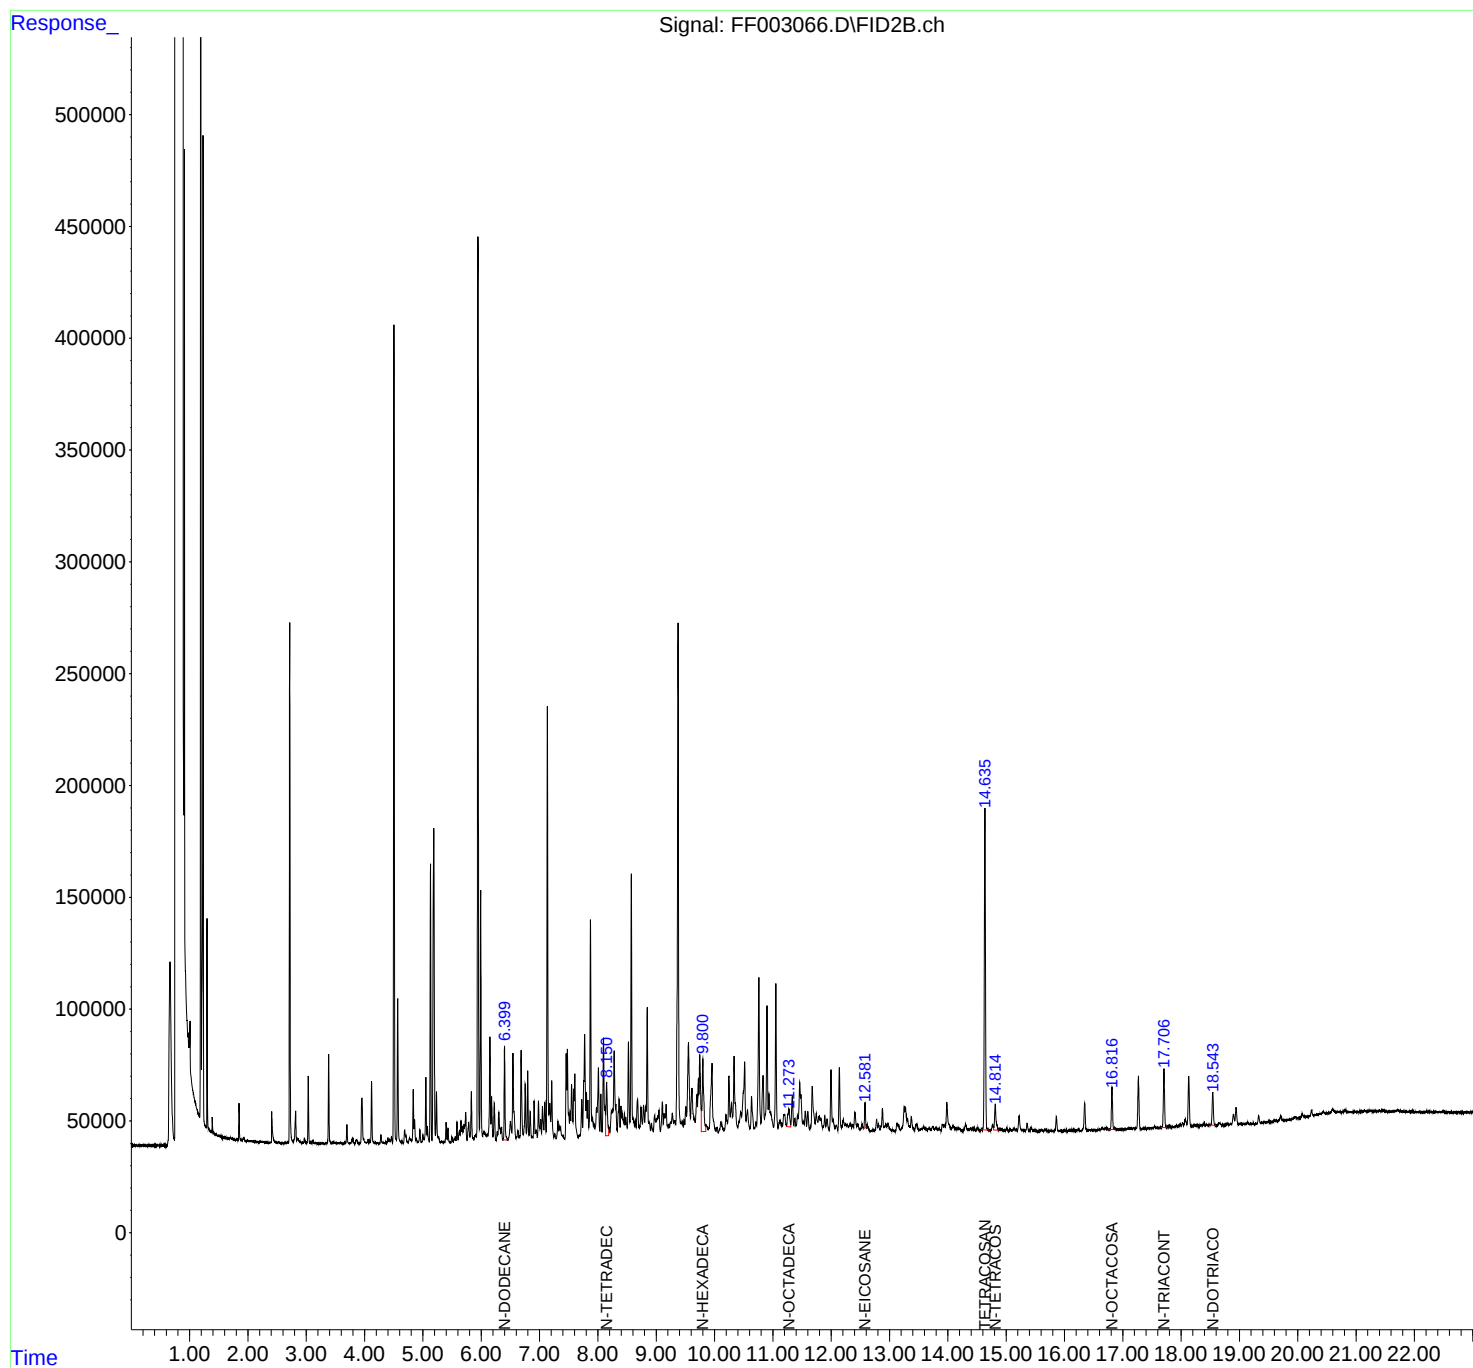

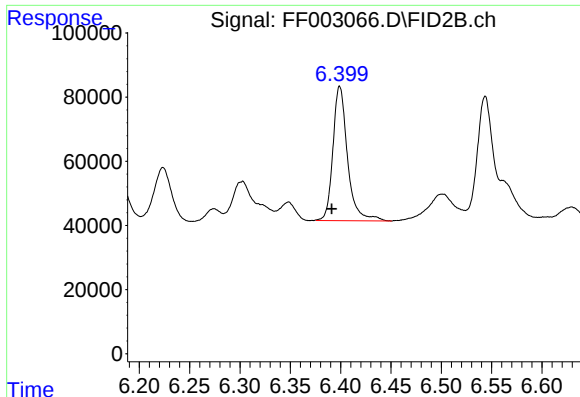


#3 N-DODECANE

R.T.: 6.399 min
Delta R.T.: 0.008 min
Response: 423817
Conc: 2.67 ug/ml

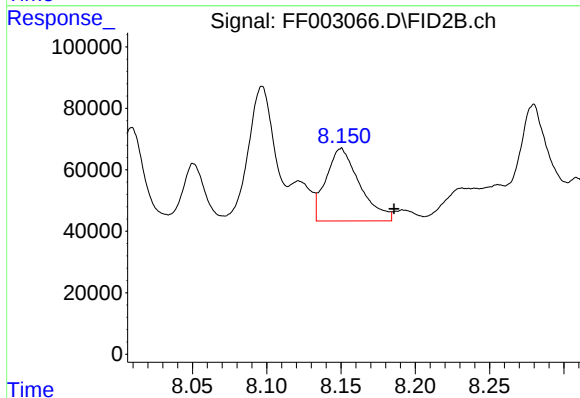


#4 N-TETRADECANE

R.T.: 8.150 min
Delta R.T.: -0.036 min
Response: 374520
Conc: 2.34 ug/ml

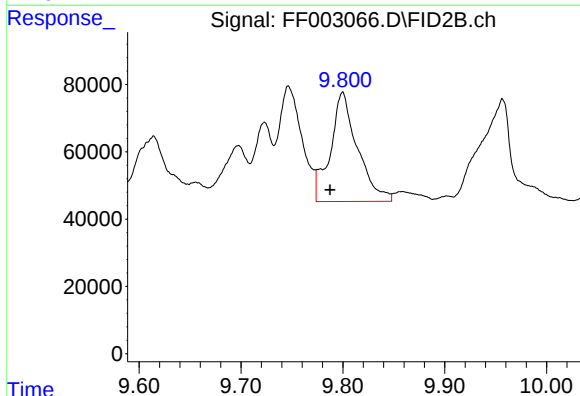


#5 N-HEXADECANE

R.T.: 9.800 min
Delta R.T.: 0.012 min
Response: 601210
Conc: 3.75 ug/ml

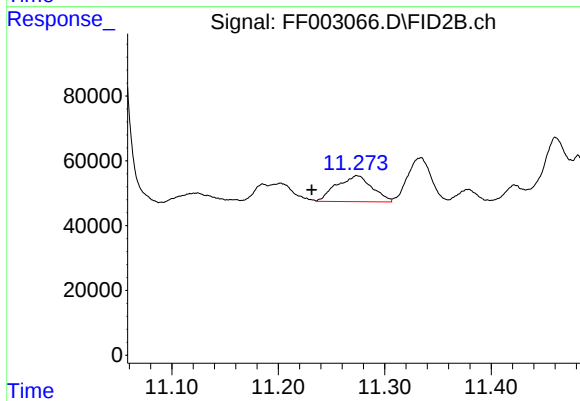


#6 N-OCTADECANE

R.T.: 11.274 min
Delta R.T.: 0.043 min
Response: 185154
Conc: 1.17 ug/ml

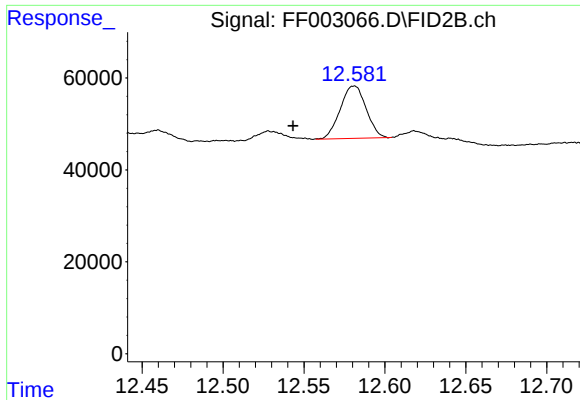


#7 N-EICOSANE

R.T.: 12.581 min
Delta R.T.: 0.038 min
Response: 126468
Conc: 0.82 ug/ml

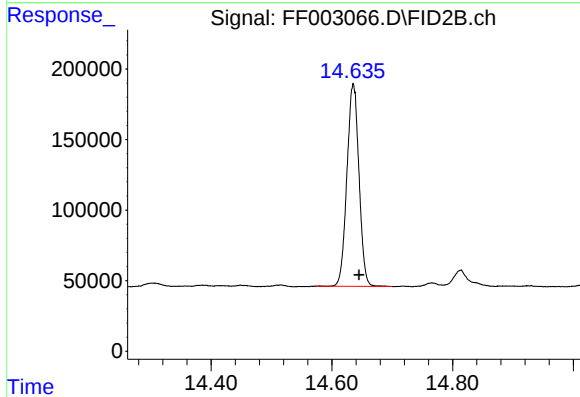


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: -0.010 min
Response: 1989667
Conc: 15.33 ug/ml

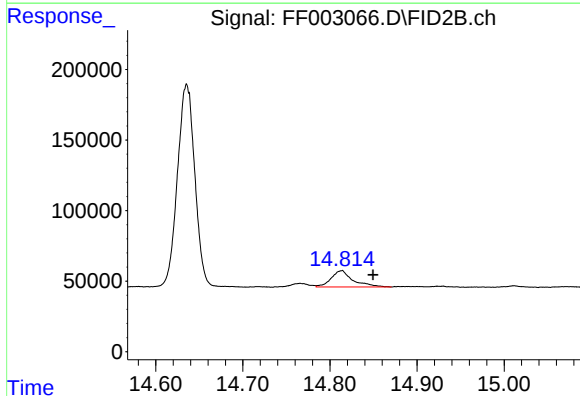


#10 N-TETRACOSANE

R.T.: 14.813 min
Delta R.T.: -0.036 min
Response: 200366
Conc: 1.39 ug/ml

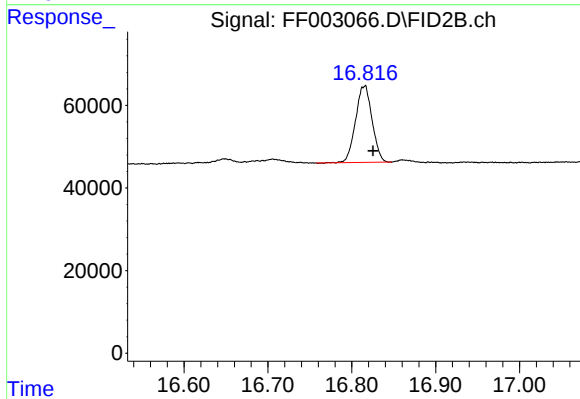


#12 N-OCTACOSANE

R.T.: 16.815 min
Delta R.T.: -0.010 min
Response: 254145
Conc: 1.90 ug/ml

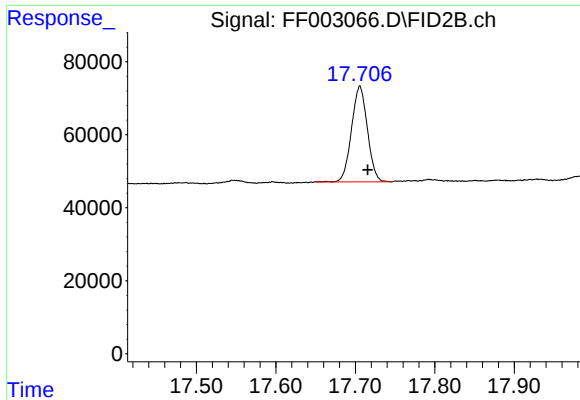

#13 N-TRIACONTANE

R.T.: 17.706 min
Delta R.T.: -0.010 min
Response: 363709
Conc: 2.84 ug/ml

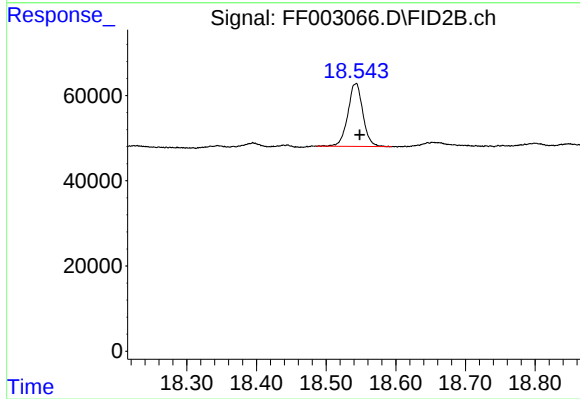

#14 N-DOTRIACONTANE

R.T.: 18.543 min
Delta R.T.: -0.006 min
Response: 220600
Conc: 1.85 ug/ml