

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
 Data File : FF003070.D
 Signal(s) : FID2B.ch
 Acq On : 21 Dec 2018 19:48
 Operator : AJ\SJ
 Sample : J6192-03 5X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 21 22:12:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.634	344520	2.654 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.232	79113	0.494 ug/ml
7)	N-EICOSANE	12.580	157913	1.024 ug/ml
10)	N-TETRACOSANE	14.810	115654	0.800 ug/ml
11)	N-HEXACOSANE	15.864	75638	0.542 ug/ml
12)	N-OCTACOSANE	16.816	386753	2.887 ug/ml
13)	N-TRIACONTANE	17.704	476026	3.715 ug/ml
14)	N-DOTRIACONTANE	18.543	354120	2.965 ug/ml
15)	N-TETRATRIACONTANE	19.332	360164	3.178 ug/ml
16)	N-HEXATRIACONTANE	20.075	165865	1.537 ug/ml
17)	N-OCTATRIACONTANE	20.815	262268	2.584 ug/ml
18)	N-TETRACONTANE	21.720	218172	2.076 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
Data File : FF003070.D
Signal(s) : FID2B.ch
Acq On : 21 Dec 2018 19:48
Operator : AJ\SJ
Sample : J6192-03 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 21 22:12:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

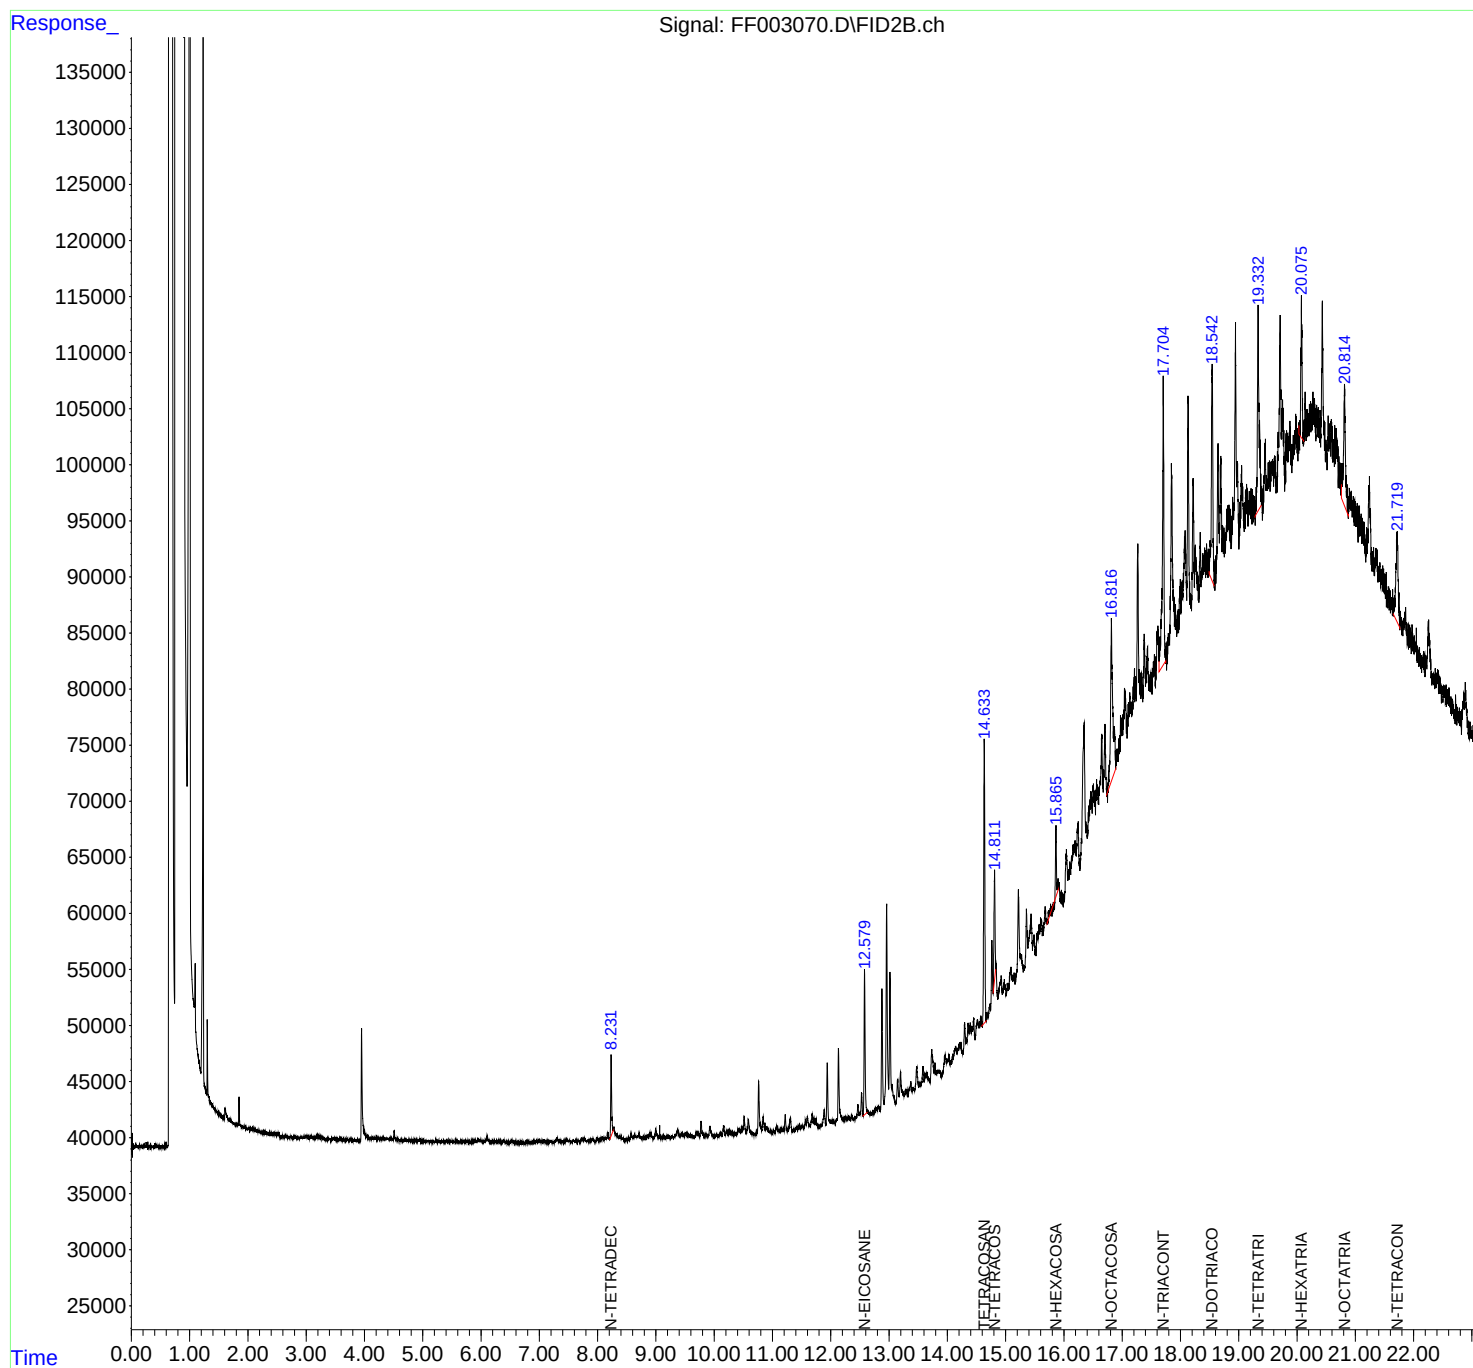

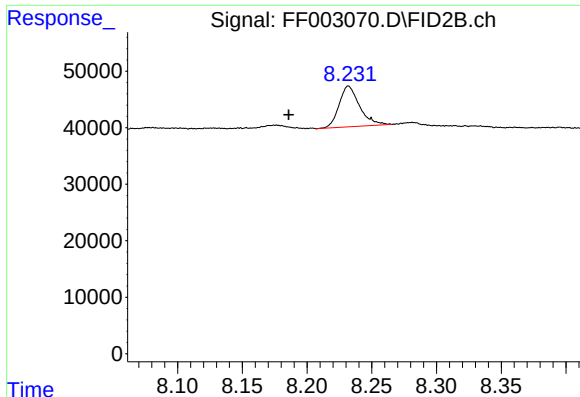


#4 N-TETRADECANE

R.T.: 8.232 min
Delta R.T.: 0.046 min
Response: 79113
Conc: 0.49 ug/ml

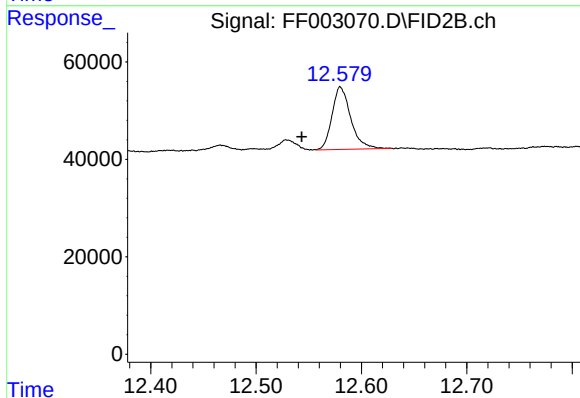


#7 N-EICOSANE

R.T.: 12.580 min
Delta R.T.: 0.037 min
Response: 157913
Conc: 1.02 ug/ml

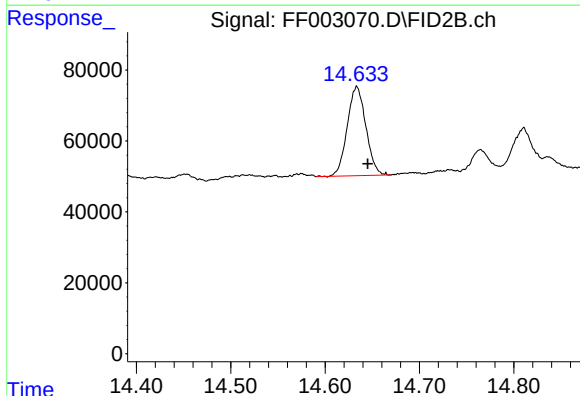


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.634 min
Delta R.T.: -0.012 min
Response: 344520
Conc: 2.65 ug/ml

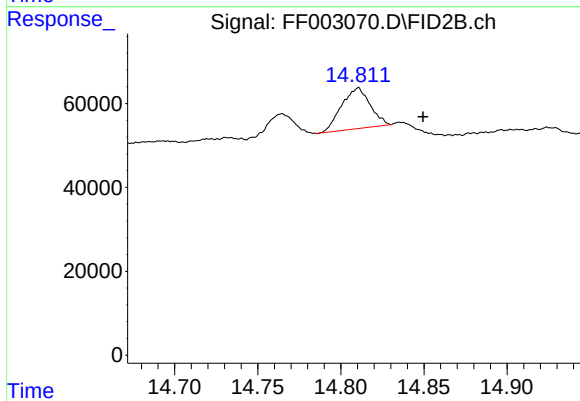


#10 N-TETRACOSANE

R.T.: 14.810 min
Delta R.T.: -0.039 min
Response: 115654
Conc: 0.80 ug/ml

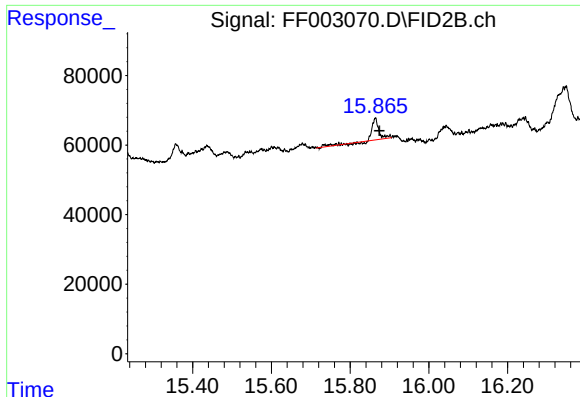


#11 N-HEXACOSANE

R.T.: 15.864 min
Delta R.T.: -0.010 min
Response: 75638
Conc: 0.54 ug/ml

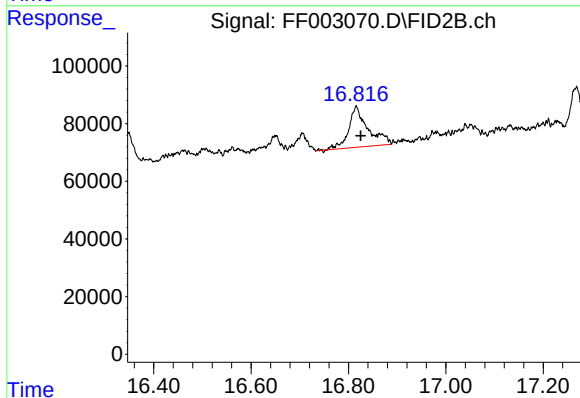


#12 N-OCTACOSANE

R.T.: 16.816 min
Delta R.T.: -0.009 min
Response: 386753
Conc: 2.89 ug/ml

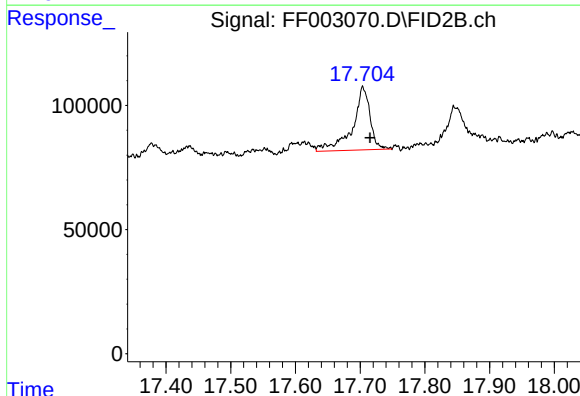


#13 N-TRIACONTANE

R.T.: 17.704 min
Delta R.T.: -0.011 min
Response: 476026
Conc: 3.72 ug/ml

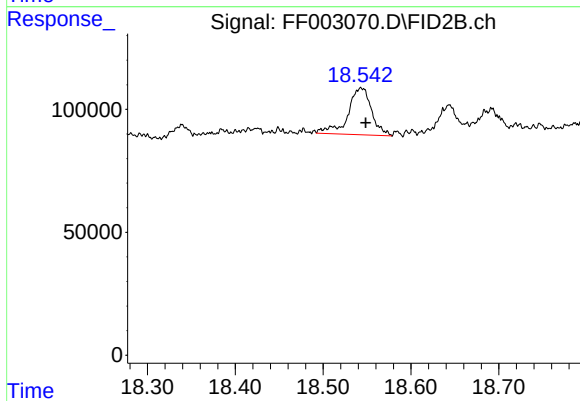


#14 N-DOTRIACONTANE

R.T.: 18.543 min
Delta R.T.: -0.005 min
Response: 354120
Conc: 2.97 ug/ml

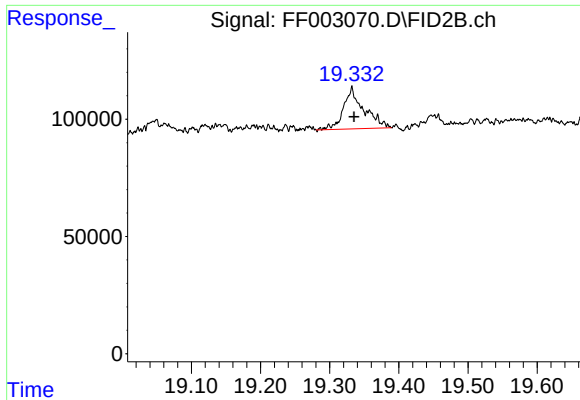


#15 N-TETRATRIACONTANE

R.T.: 19.332 min
Delta R.T.: -0.003 min
Response: 360164
Conc: 3.18 ug/ml

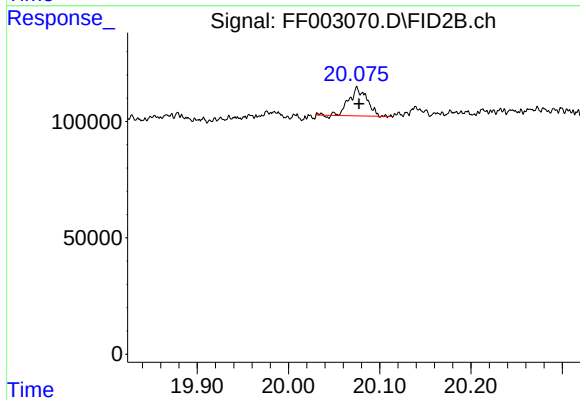


#16 N-HEXATRIACONTANE

R.T.: 20.075 min
Delta R.T.: -0.002 min
Response: 165865
Conc: 1.54 ug/ml

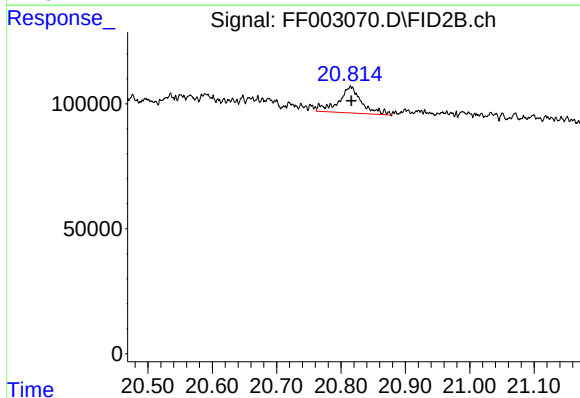

#17 N-OCTATRIACONTANE

R.T.: 20.815 min
Delta R.T.: -0.001 min
Response: 262268
Conc: 2.58 ug/ml

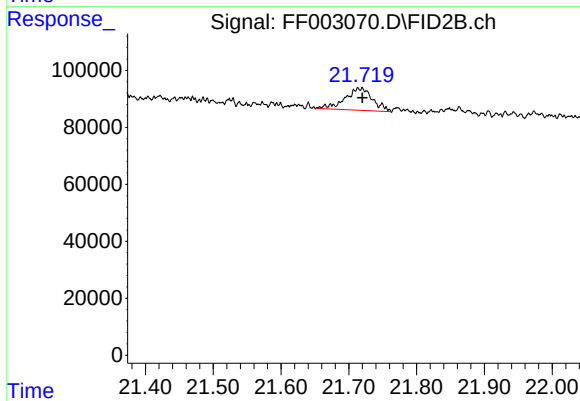

#18 N-TETRACONTANE

R.T.: 21.720 min
Delta R.T.: 0.000 min
Response: 218172
Conc: 2.08 ug/ml