

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
 Data File : FF003071.D
 Signal(s) : FID2B.ch
 Acq On : 21 Dec 2018 20:19
 Operator : AJ\SJ
 Sample : J6200-01 5X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 21 22:12:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	217763	1.677 ug/ml
Target Compounds			
4) N-TETRADECANE	8.231	82033	0.512 ug/ml
7) N-EICOSANE	12.584	236587	1.534 ug/ml
10) N-TETRACOSANE	14.815	350167	2.423 ug/ml
12) N-OCTACOSANE	16.817	118134	0.882 ug/ml
13) N-TRIACONTANE	17.706	210774	1.645 ug/ml
14) N-DOTRIACONTANE	18.541	289996	2.428 ug/ml
15) N-TETRATRIACONTANE	19.332	175152	1.545 ug/ml
16) N-HEXATRIACONTANE	20.071	182779	1.694 ug/ml
17) N-OCTATRIACONTANE	20.812	120031	1.183 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
Data File : FF003071.D
Signal(s) : FID2B.ch
Acq On : 21 Dec 2018 20:19
Operator : AJ\SJ
Sample : J6200-01 5X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 21 22:12:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

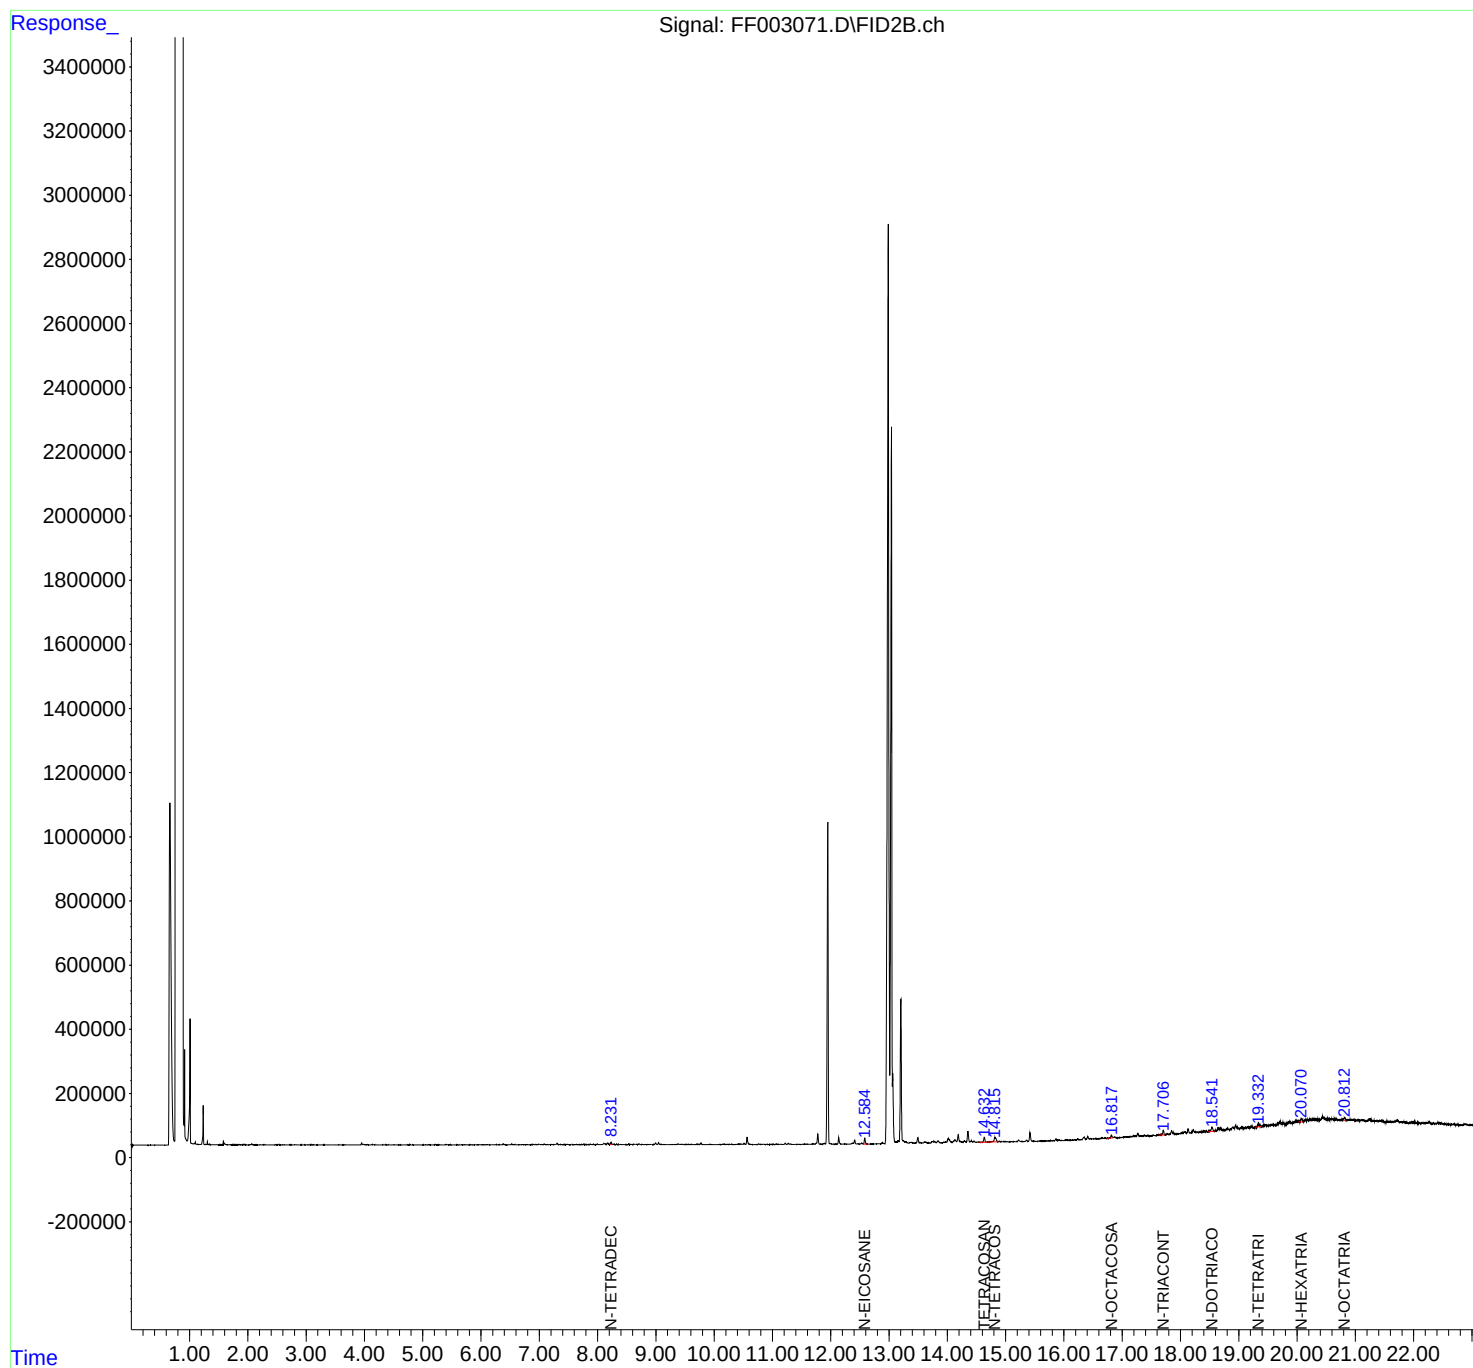

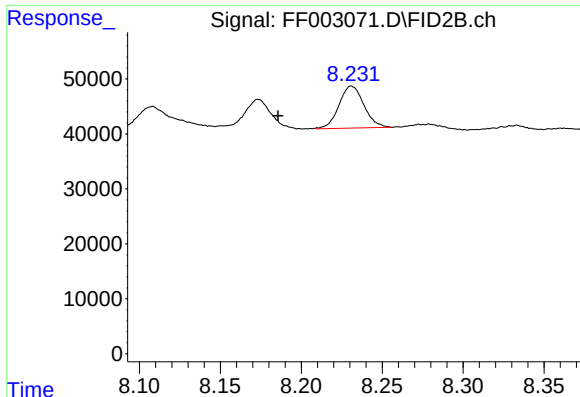


#4 N-TETRADECANE

R.T.: 8.231 min
Delta R.T.: 0.045 min
Response: 82033
Conc: 0.51 ug/ml

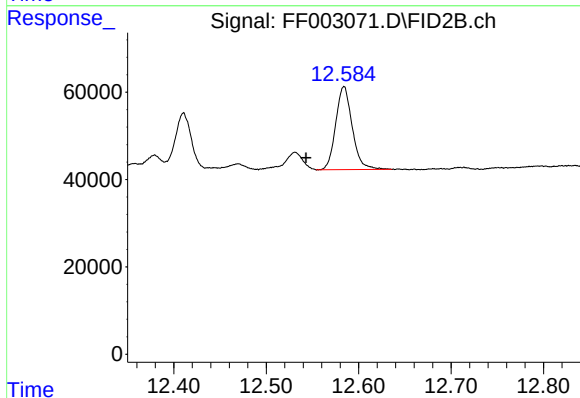


#7 N-EICOSANE

R.T.: 12.584 min
Delta R.T.: 0.041 min
Response: 236587
Conc: 1.53 ug/ml

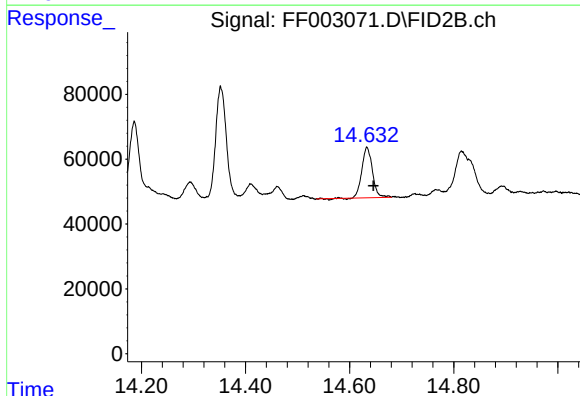


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.633 min
Delta R.T.: -0.012 min
Response: 217763
Conc: 1.68 ug/ml

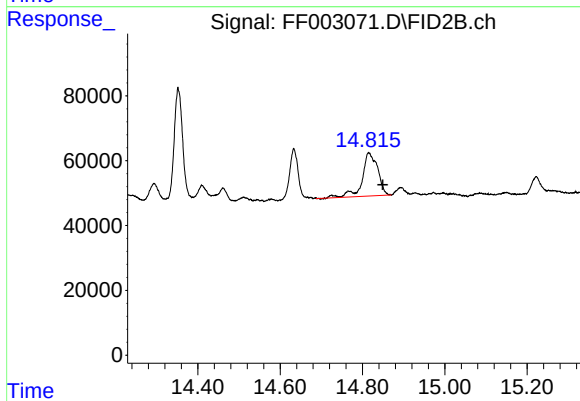


#10 N-TETRACOSANE

R.T.: 14.815 min
Delta R.T.: -0.034 min
Response: 350167
Conc: 2.42 ug/ml

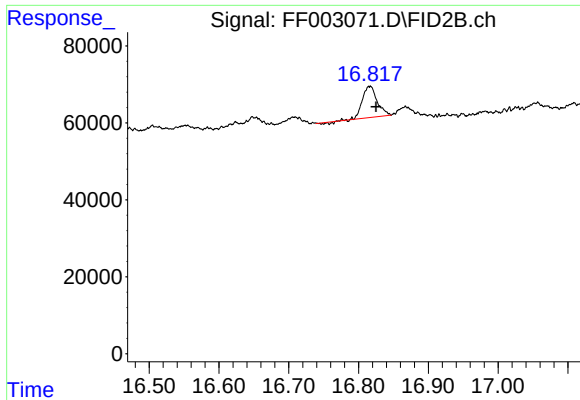


#12 N-OCTACOSANE

R.T.: 16.817 min
Delta R.T.: -0.008 min
Response: 118134
Conc: 0.88 ug/ml

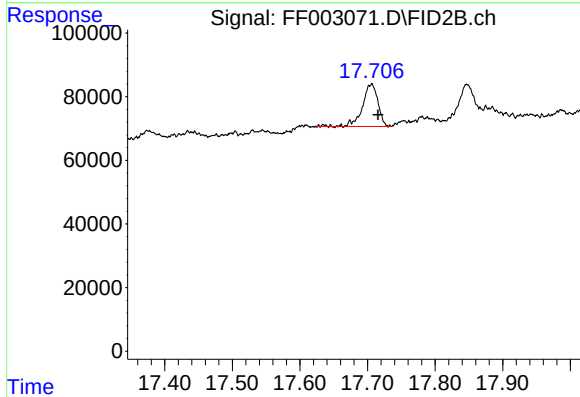


#13 N-TRIACONTANE

R.T.: 17.706 min
Delta R.T.: -0.009 min
Response: 210774
Conc: 1.64 ug/ml

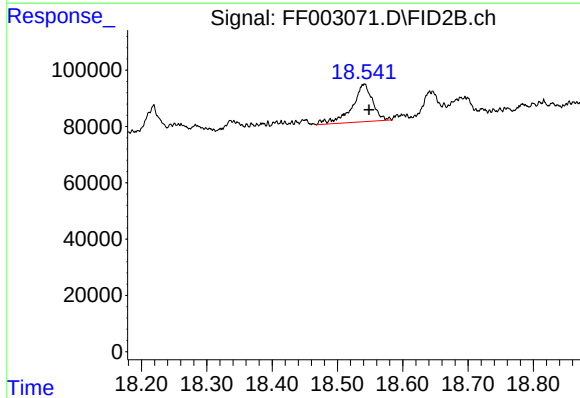


#14 N-DOTRIACONTANE

R.T.: 18.541 min
Delta R.T.: -0.007 min
Response: 289996
Conc: 2.43 ug/ml

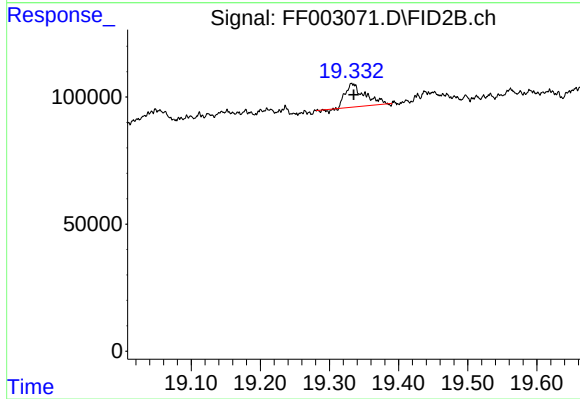


#15 N-TETRATRIACONTANE

R.T.: 19.332 min
Delta R.T.: -0.003 min
Response: 175152
Conc: 1.55 ug/ml

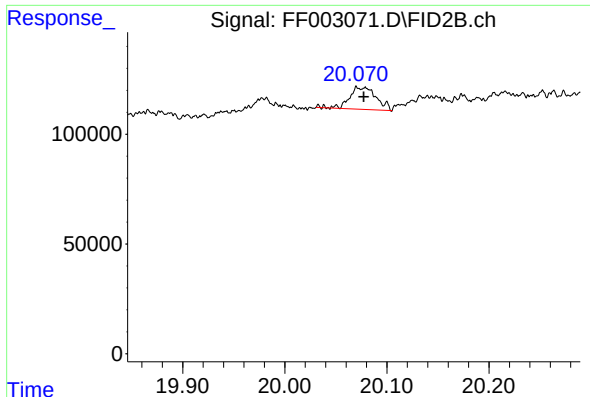

#16 N-HEXATRIACONTANE

R.T.: 20.071 min
Delta R.T.: -0.006 min
Response: 182779
Conc: 1.69 ug/ml

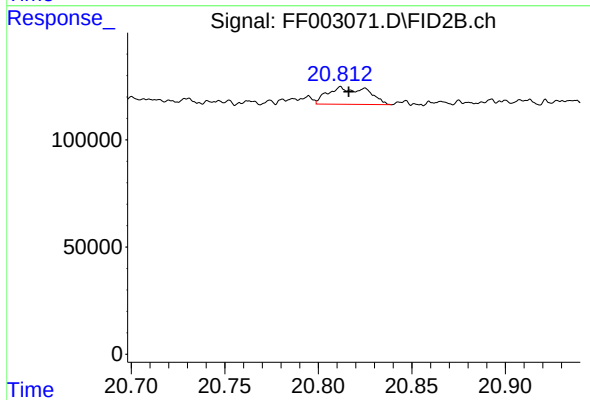

#17 N-OCTATRIACONTANE

R.T.: 20.812 min
Delta R.T.: -0.004 min
Response: 120031
Conc: 1.18 ug/ml