

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
 Data File : FF003063.D
 Signal(s) : FID2B.ch
 Acq On : 21 Dec 2018 16:08
 Operator : AJ\SJ
 Sample : PB115911BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 21 22:10:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	2345807	18.069 ug/ml
Target Compounds			
2) N-DECANE	4.358	3150895	20.112 ug/ml
3) N-DODECANE	6.380	3121972	19.660 ug/ml
4) N-TETRADECANE	8.174	3049122	19.023 ug/ml
5) N-HEXADECANE	9.775	2988146	18.659 ug/ml
6) N-OCTADECANE	11.219	2931744	18.506 ug/ml
7) N-EICOSANE	12.532	2828144	18.337 ug/ml
8) N-DOCOSANE	13.733	2734796	18.289 ug/ml
10) N-TETRACOSANE	14.841	2736179	18.933 ug/ml
11) N-HEXACOSANE	15.864	2619642	18.768 ug/ml
12) N-OCTACOSANE	16.817	2650684	19.783 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
Data File : FF003063.D
Signal(s) : FID2B.ch
Acq On : 21 Dec 2018 16:08
Operator : AJ\SJ
Sample : PB115911BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 21 22:10:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

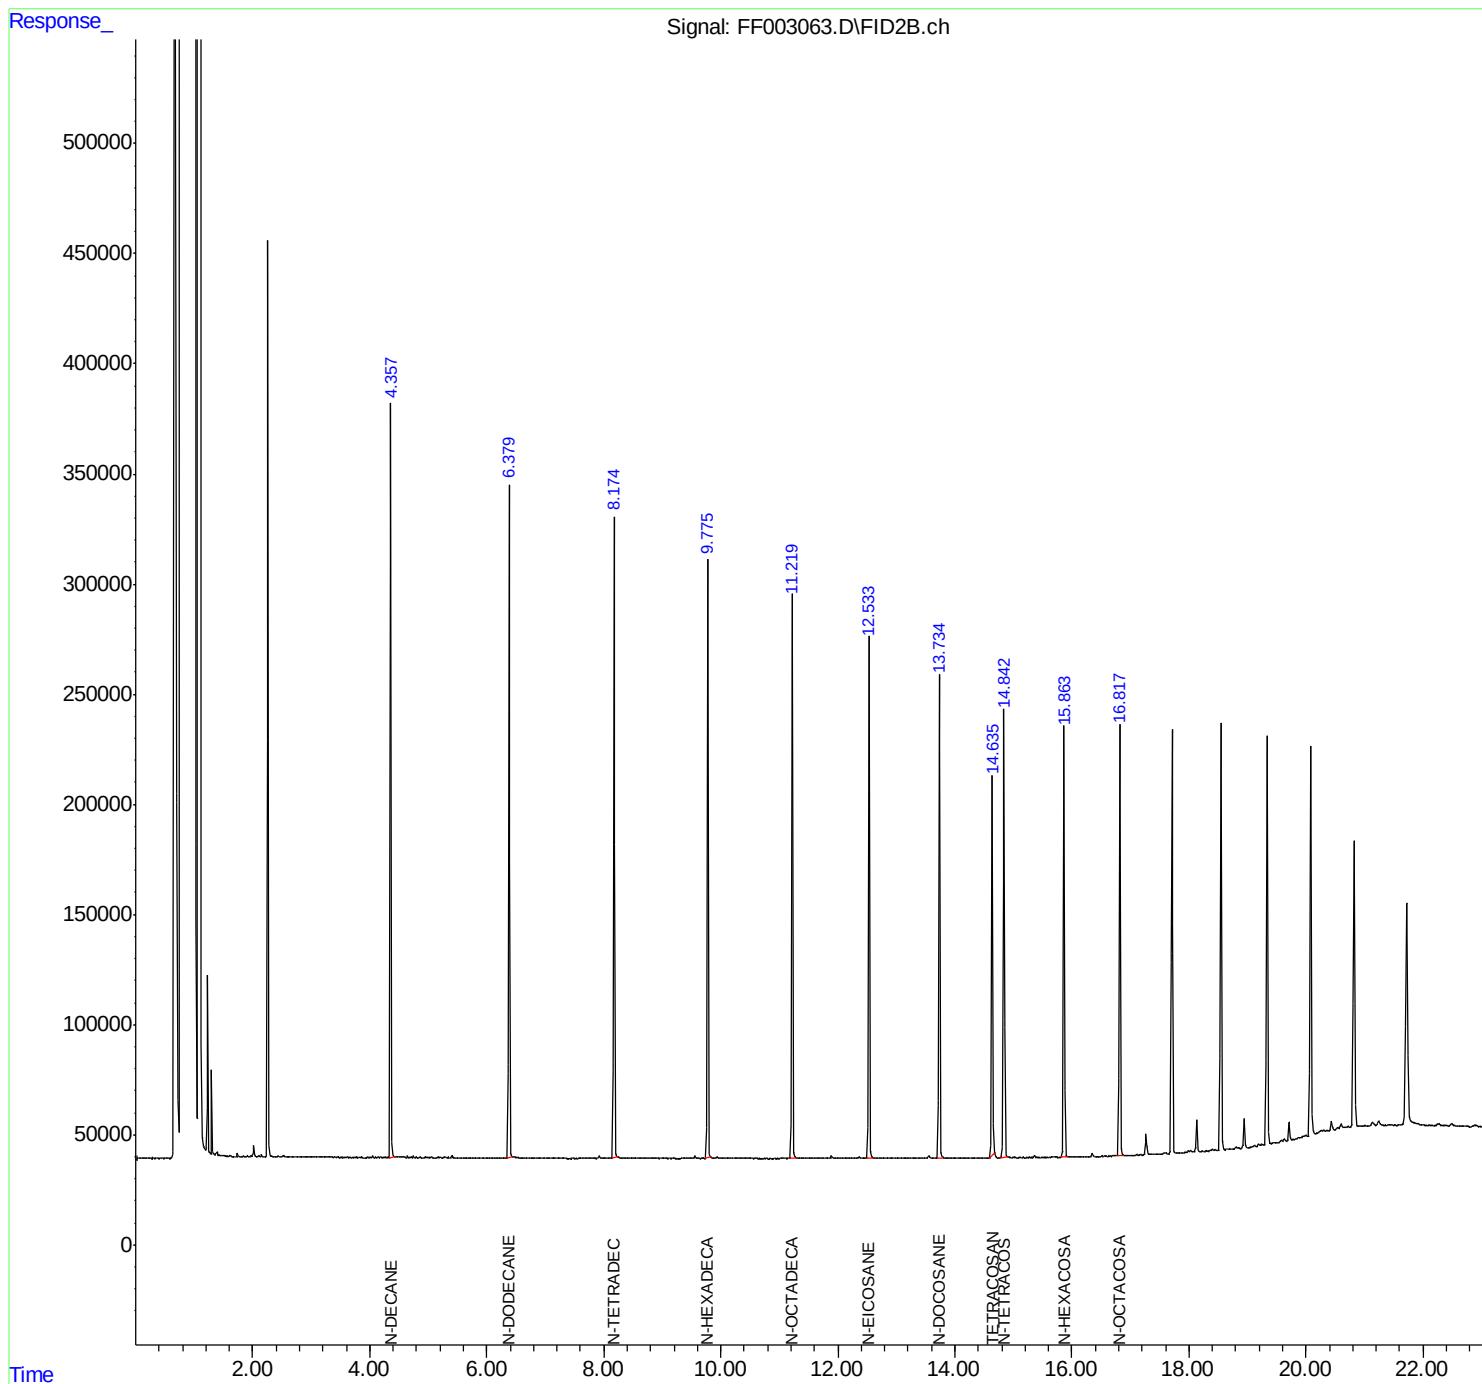

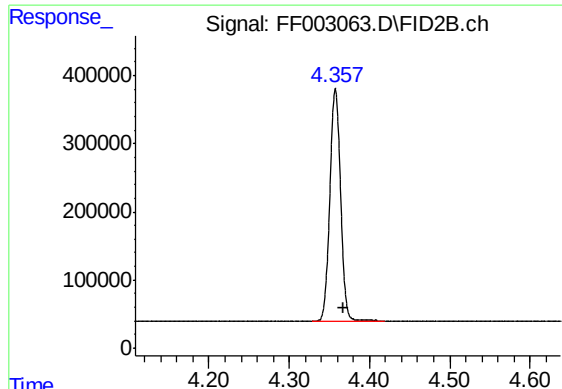


#2 N-DECANE

R.T.: 4.358 min
Delta R.T.: -0.010 min
Response: 3150895
Conc: 20.11 ug/ml

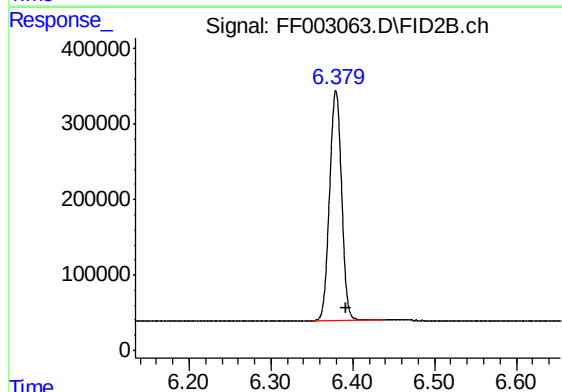


#3 N-DODECANE

R.T.: 6.380 min
Delta R.T.: -0.011 min
Response: 3121972
Conc: 19.66 ug/ml

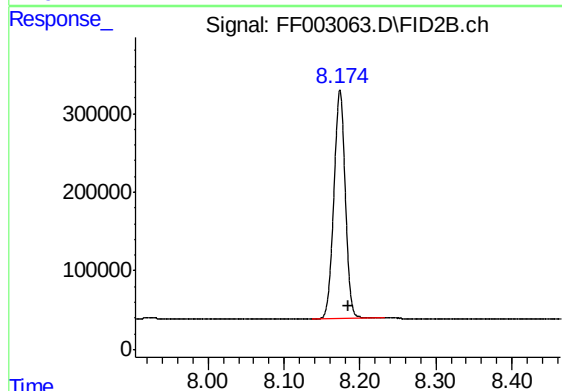


#4 N-TETRADECANE

R.T.: 8.174 min
Delta R.T.: -0.012 min
Response: 3049122
Conc: 19.02 ug/ml

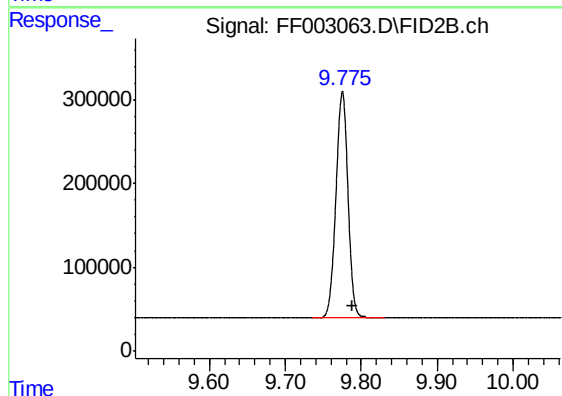


#5 N-HEXADECANE

R.T.: 9.775 min
Delta R.T.: -0.012 min
Response: 2988146
Conc: 18.66 ug/ml

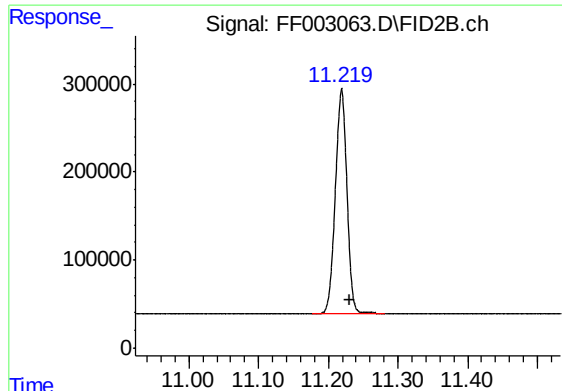


#6 N-OCTADECANE

R.T.: 11.219 min
Delta R.T.: -0.012 min
Response: 2931744
Conc: 18.51 ug/ml

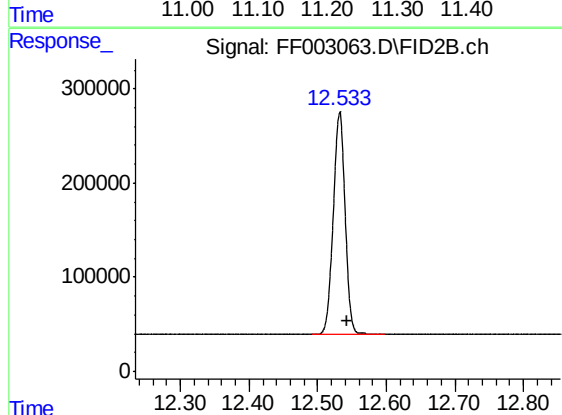


#7 N-EICOSANE

R.T.: 12.532 min
Delta R.T.: -0.011 min
Response: 2828144
Conc: 18.34 ug/ml

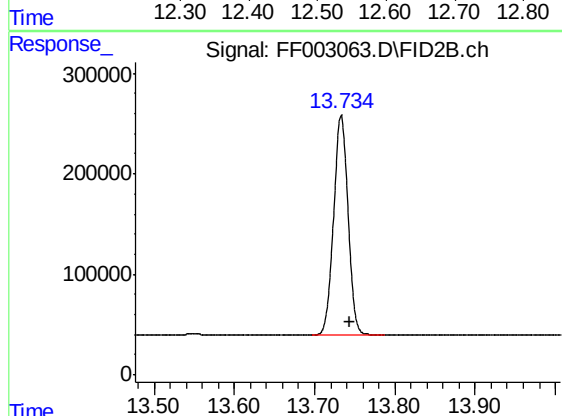


#8 N-DOCOSANE

R.T.: 13.733 min
Delta R.T.: -0.011 min
Response: 2734796
Conc: 18.29 ug/ml

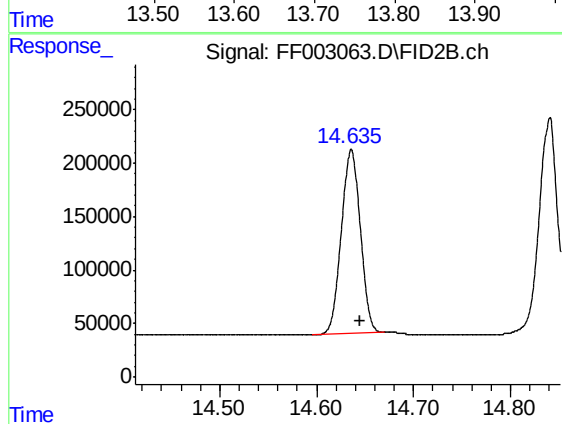


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: -0.010 min
Response: 2345807
Conc: 18.07 ug/ml

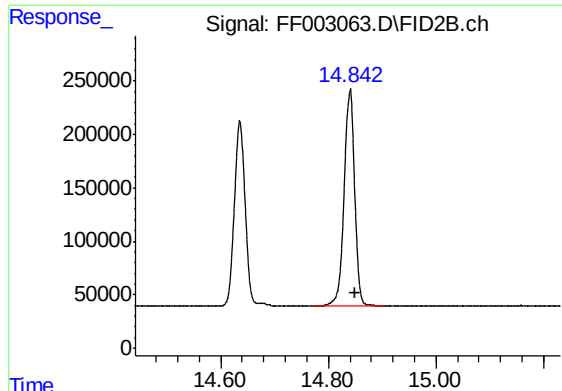


#10 N-TETRACOSANE

R.T.: 14.841 min
Delta R.T.: -0.009 min
Response: 2736179
Conc: 18.93 ug/ml

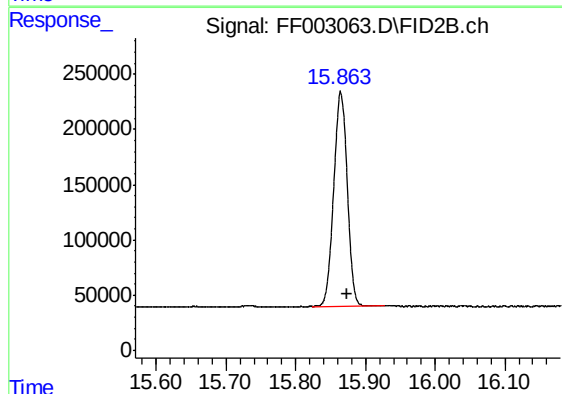

#11 N-HEXACOSANE

R.T.: 15.864 min
Delta R.T.: -0.010 min
Response: 2619642
Conc: 18.77 ug/ml

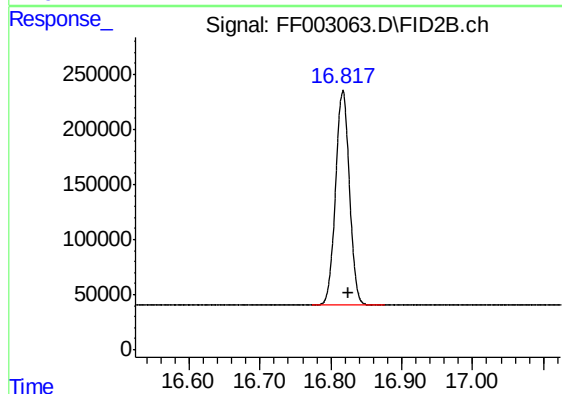

#12 N-OCTACOSANE

R.T.: 16.817 min
Delta R.T.: -0.008 min
Response: 2650684
Conc: 19.78 ug/ml