

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
 Data File : FF003064.D
 Signal(s) : FID2B.ch
 Acq On : 21 Dec 2018 16:39
 Operator : AJ\SJ
 Sample : PB115911BSD
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 21 22:11:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	2736366	21.077 ug/ml
Target Compounds			
2) N-DECANE	4.361	3724909	23.776 ug/ml
3) N-DODECANE	6.381	3688396	23.227 ug/ml
4) N-TETRADECANE	8.175	3610660	22.526 ug/ml
5) N-HEXADECANE	9.777	3530388	22.045 ug/ml
6) N-OCTADECANE	11.220	3451720	21.789 ug/ml
7) N-EICOSANE	12.532	3322524	21.543 ug/ml
8) N-DOCOSANE	13.734	3207206	21.449 ug/ml
10) N-TETRACOSANE	14.840	3186761	22.051 ug/ml
11) N-HEXACOSANE	15.865	3041980	21.794 ug/ml
12) N-OCTACOSANE	16.817	3066881	22.890 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122118\
Data File : FF003064.D
Signal(s) : FID2B.ch
Acq On : 21 Dec 2018 16:39
Operator : AJ\SJ
Sample : PB115911BSD
Misc :
ALS Vial : 57 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 21 22:11:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

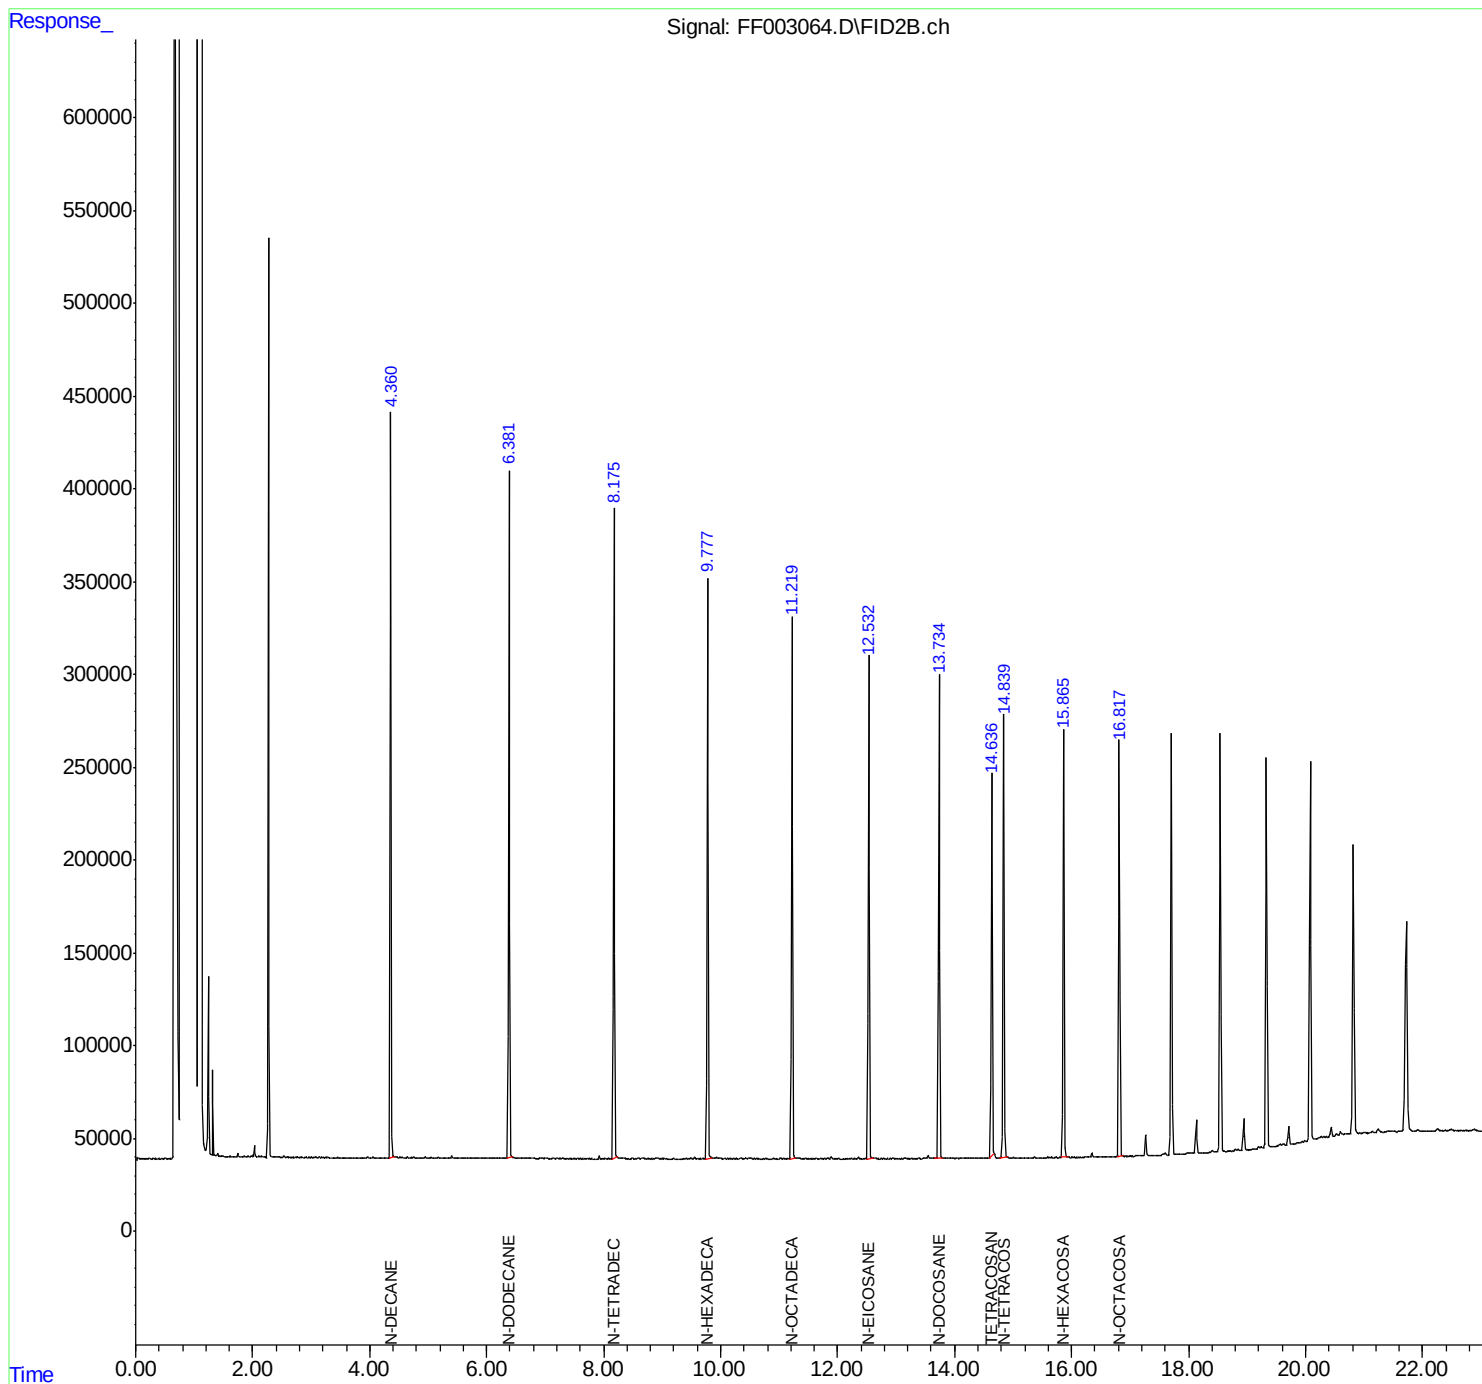

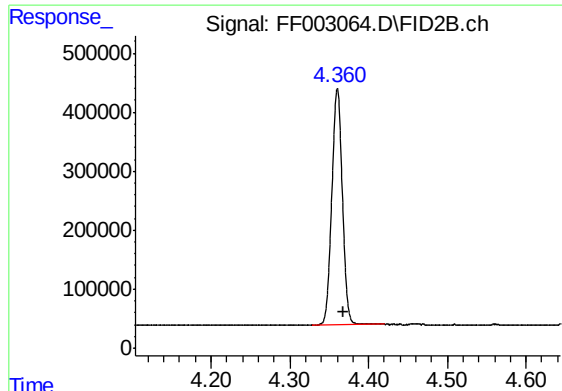


#2 N-DECANE

R.T.: 4.361 min
Delta R.T.: -0.007 min
Response: 3724909
Conc: 23.78 ug/ml

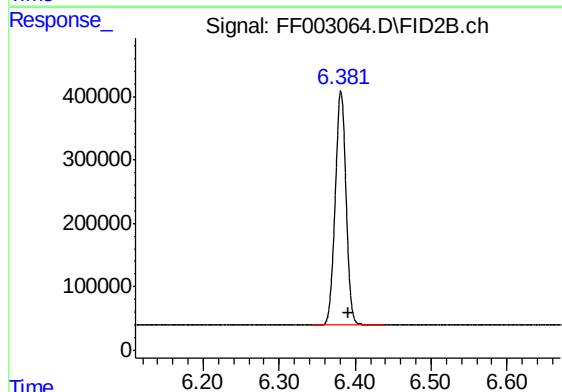


#3 N-DODECANE

R.T.: 6.381 min
Delta R.T.: -0.010 min
Response: 3688396
Conc: 23.23 ug/ml

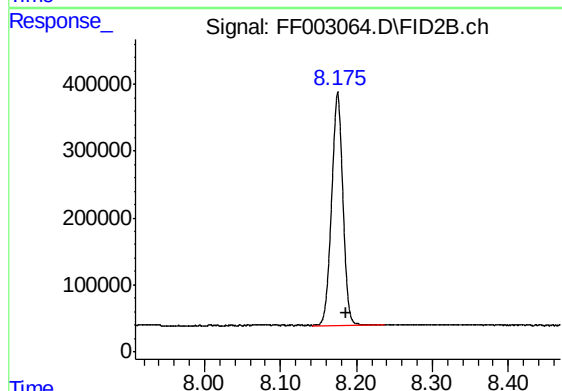


#4 N-TETRADECANE

R.T.: 8.175 min
Delta R.T.: -0.010 min
Response: 3610660
Conc: 22.53 ug/ml

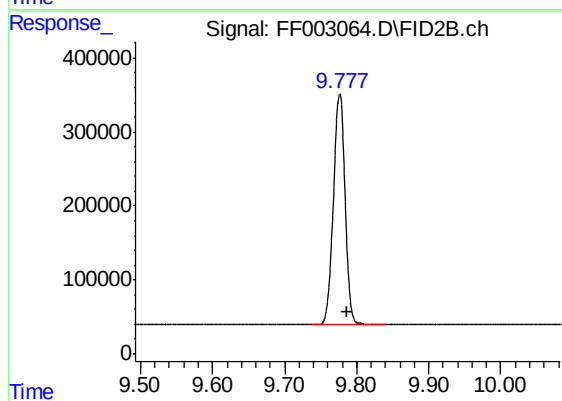


#5 N-HEXADECANE

R.T.: 9.777 min
Delta R.T.: -0.011 min
Response: 3530388
Conc: 22.04 ug/ml

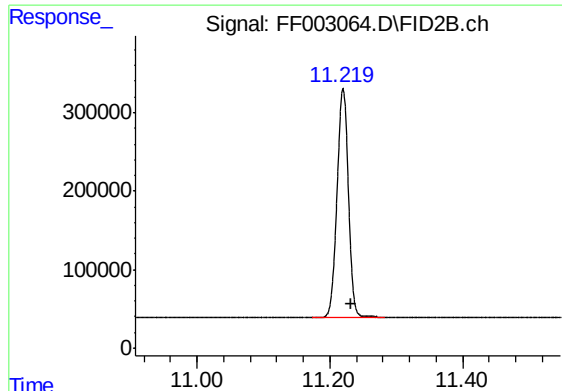


#6 N-OCTADECANE

R.T.: 11.220 min
Delta R.T.: -0.011 min
Response: 3451720
Conc: 21.79 ug/ml

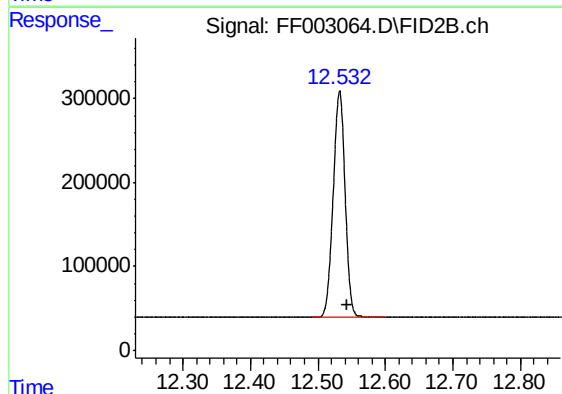


#7 N-EICOSANE

R.T.: 12.532 min
Delta R.T.: -0.011 min
Response: 3322524
Conc: 21.54 ug/ml

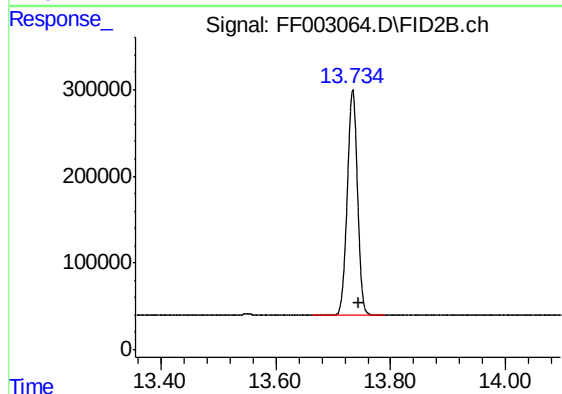


#8 N-DOCOSANE

R.T.: 13.734 min
Delta R.T.: -0.010 min
Response: 3207206
Conc: 21.45 ug/ml

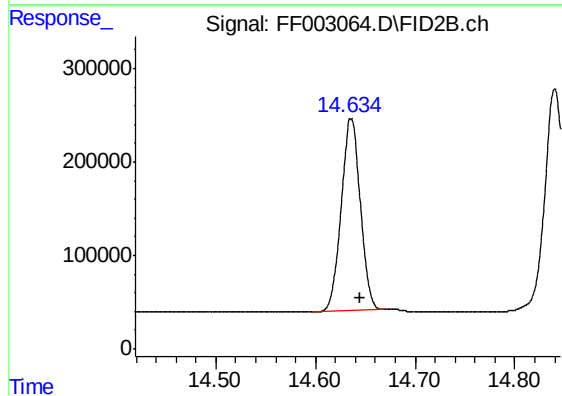


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: -0.010 min
Response: 2736366
Conc: 21.08 ug/ml

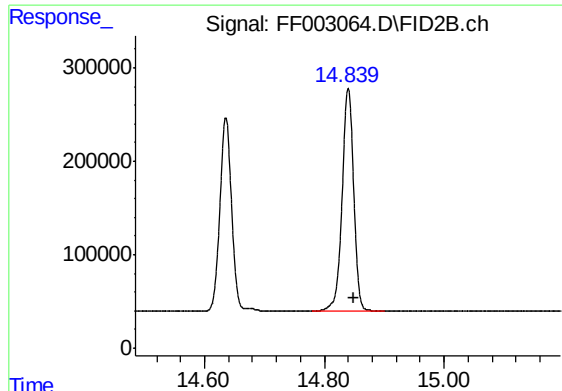


#10 N-TETRACOSANE

R.T.: 14.840 min
Delta R.T.: -0.010 min
Response: 3186761
Conc: 22.05 ug/ml

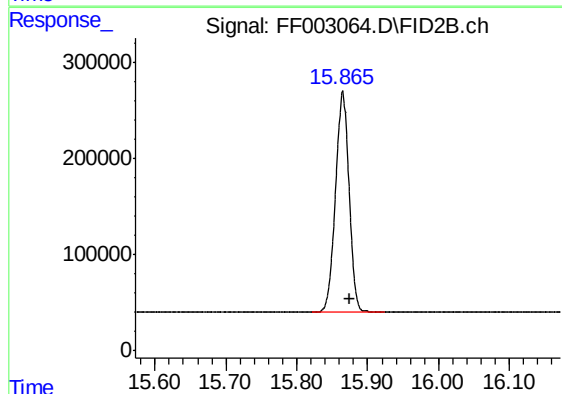

#11 N-HEXACOSANE

R.T.: 15.865 min
Delta R.T.: -0.009 min
Response: 3041980
Conc: 21.79 ug/ml

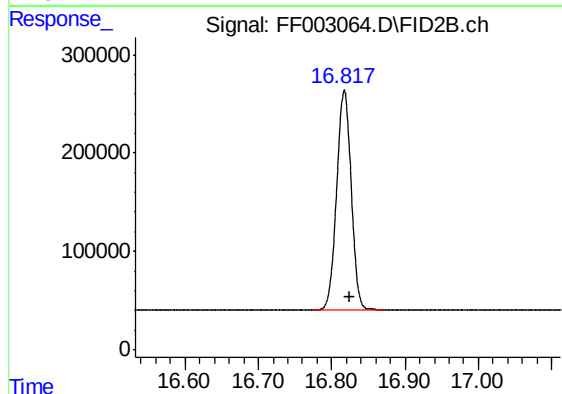

#12 N-OCTACOSANE

R.T.: 16.817 min
Delta R.T.: -0.008 min
Response: 3066881
Conc: 22.89 ug/ml