

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122121\
Data File : FF009506.D
Signal(s) : FID2B.ch
Acq On : 21 Dec 2021 22:09
Operator : AJ\MA
Sample : M5182-10
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
HB-3-(20-25)-12-17-21

Integration File: autoint1.e
Quant Time: Dec 22 00:22:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.476	2130874	18.395 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122121\
Data File : FF009506.D
Signal(s) : FID2B.ch
Acq On : 21 Dec 2021 22:09
Operator : AJ\MA
Sample : M5182-10
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
HB-3-(20-25)-12-17-21

Integration File: autoint1.e
Quant Time: Dec 22 00:22:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

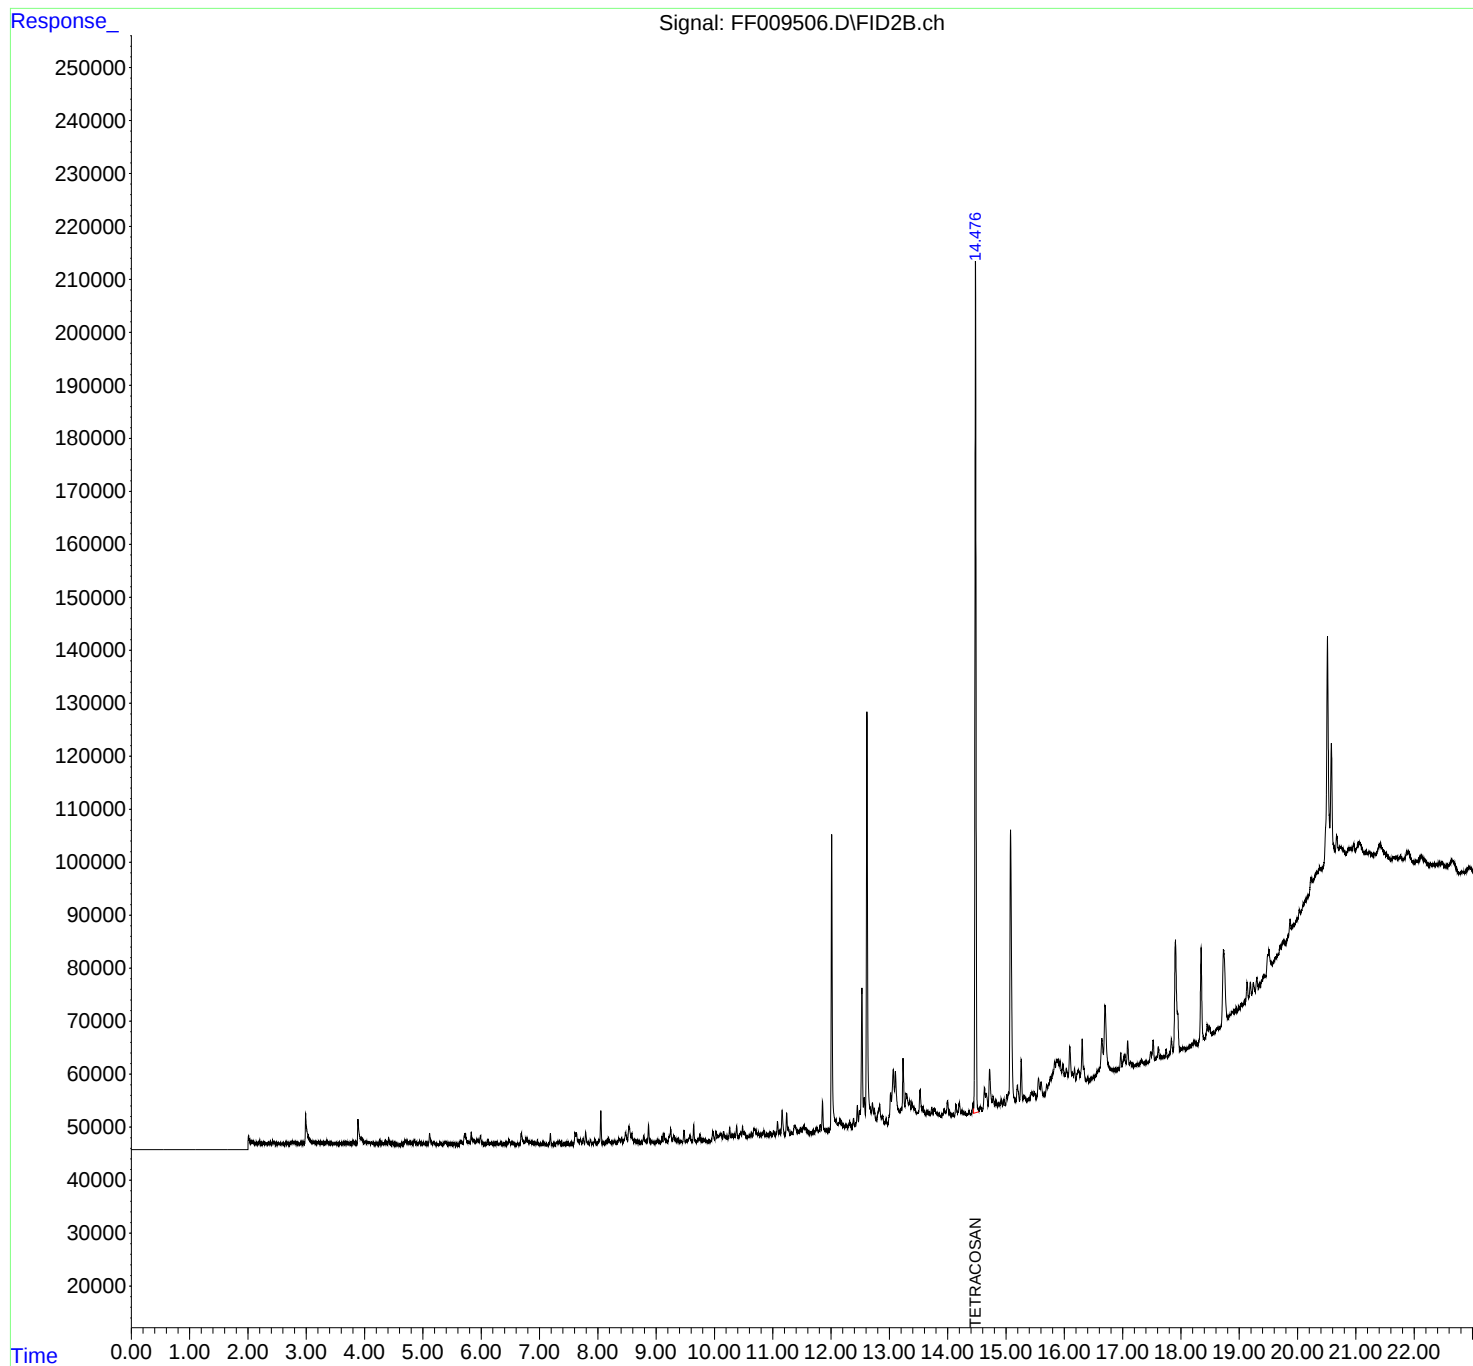

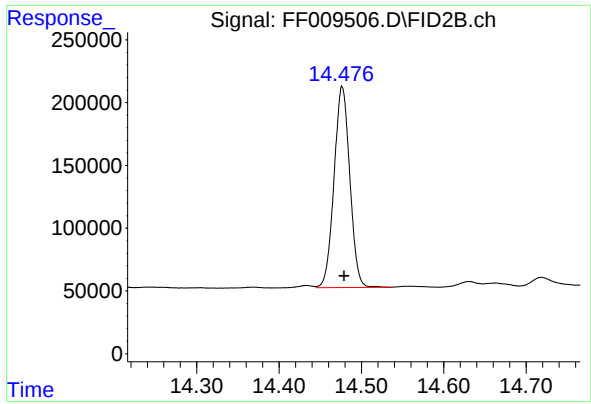

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.476 min
Delta R.T.: -0.003 min
Response: 2130874
Conc: 18.39 ug/ml

Instrument :

FID_F

ClientSampleId :

HB-3-(20-25)-12-17-21