

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122221\
Data File : FF009512.D
Signal(s) : FID2B.ch
Acq On : 22 Dec 2021 13:53
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 00:11:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.256	2917741	20.176 ug/ml
12)	N-OCTACOSANE	16.638	2291863	19.247 ug/ml
13)	N-TRIACONTANE	17.520	49585	0.433 ug/ml
14)	N-DOTRIACONTANE	18.354	56462	0.517 ug/ml
15)	N-TETRATRIACONTANE	19.132	43302	0.409 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122221\
Data File : FF009512.D
Signal(s) : FID2B.ch
Acq On : 22 Dec 2021 13:53
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 00:11:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

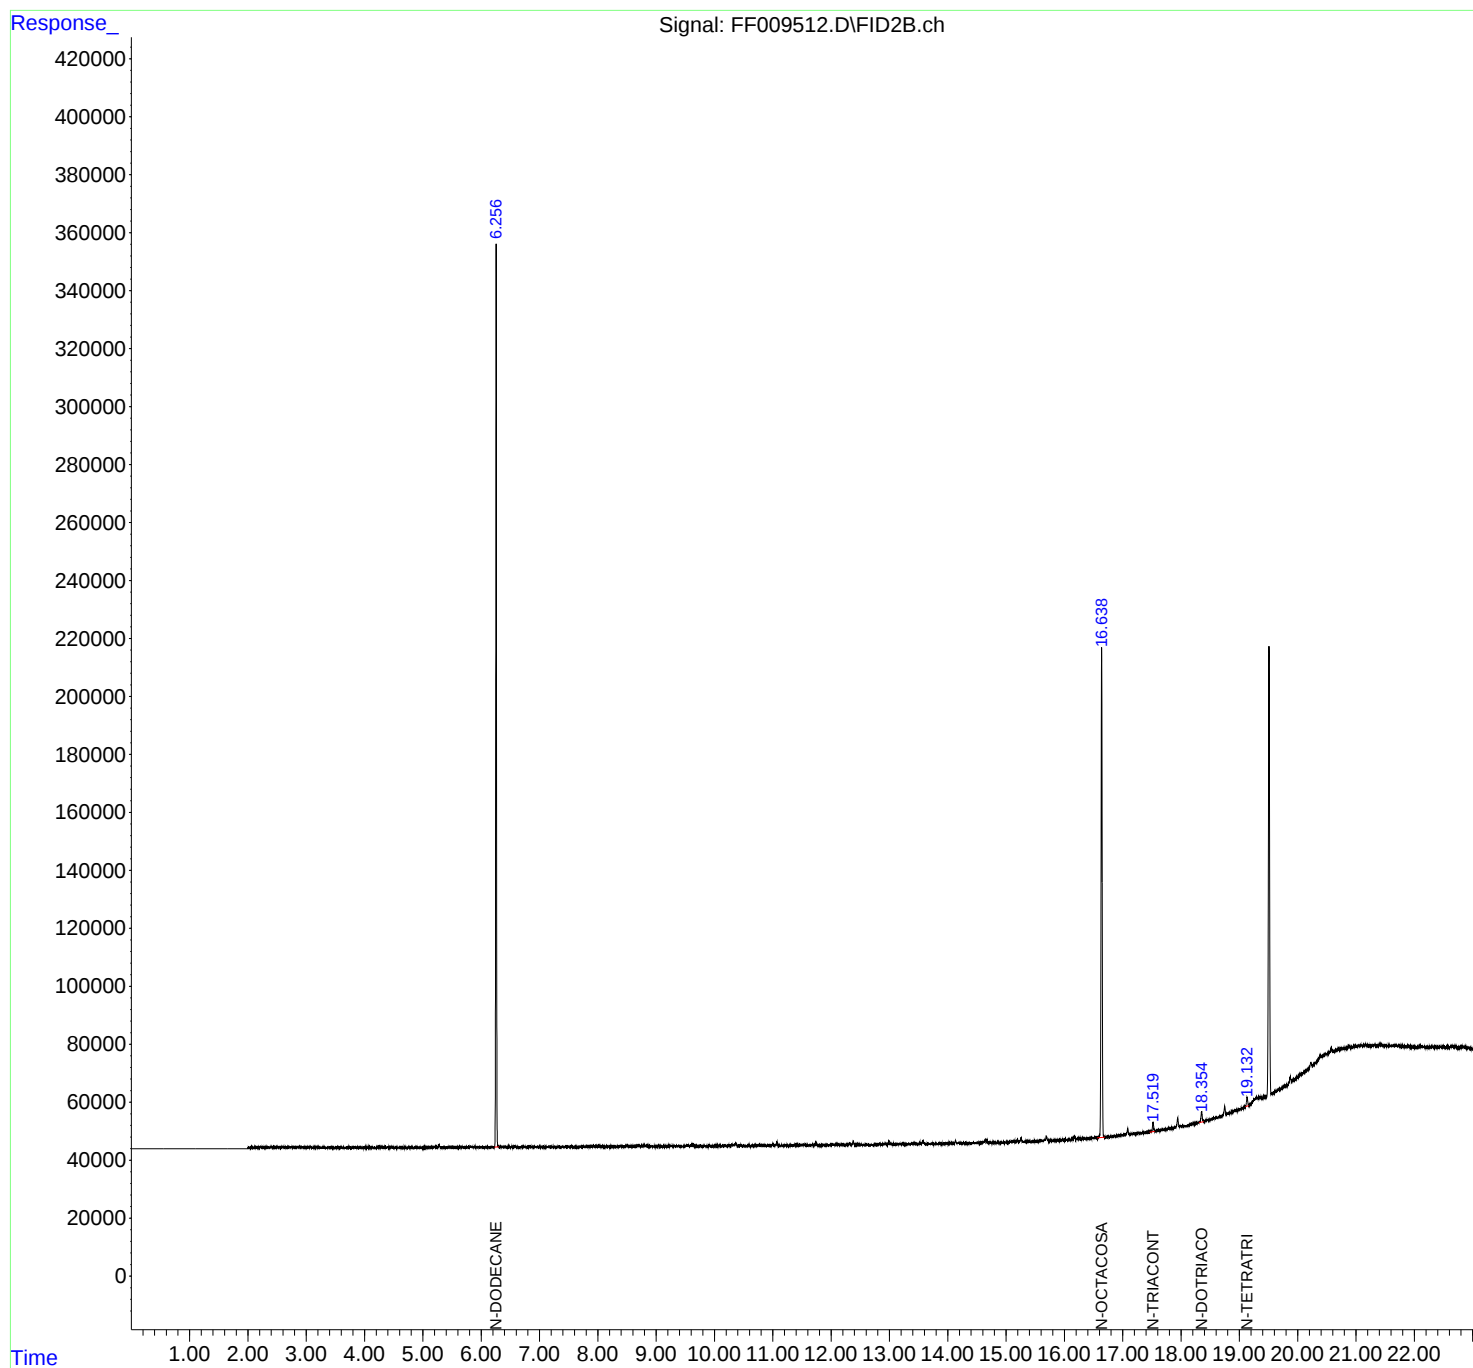


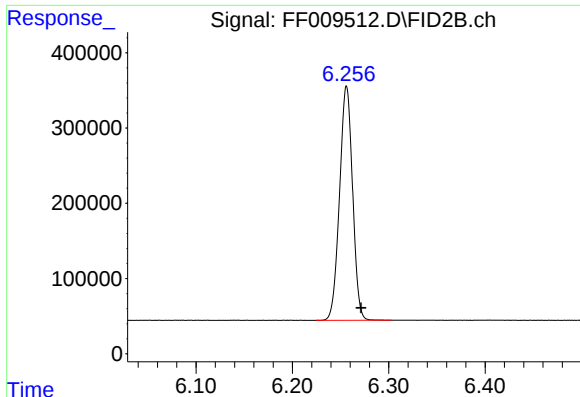

#3 N-DODECANE


R.T.: 6.256 min
Delta R.T.: -0.015 min
Response: 2917741
Conc: 20.18 ug/ml

Instrument :
FID_F
ClientSampleId :

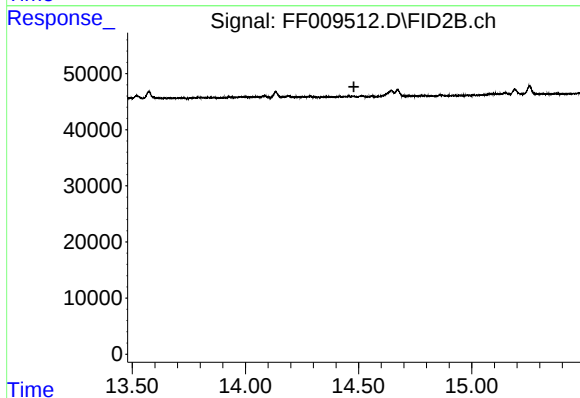


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

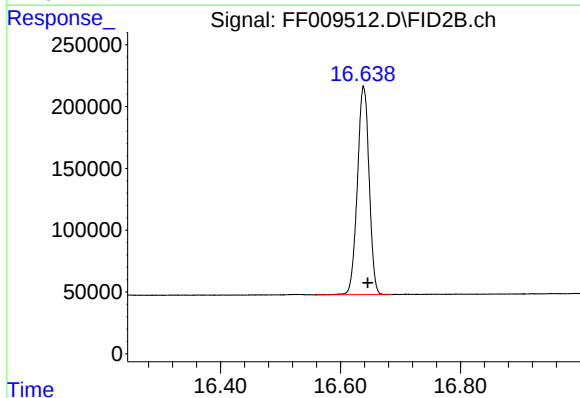


#12 N-OCTACOSANE

R.T.: 16.638 min
Delta R.T.: -0.007 min
Response: 2291863
Conc: 19.25 ug/ml

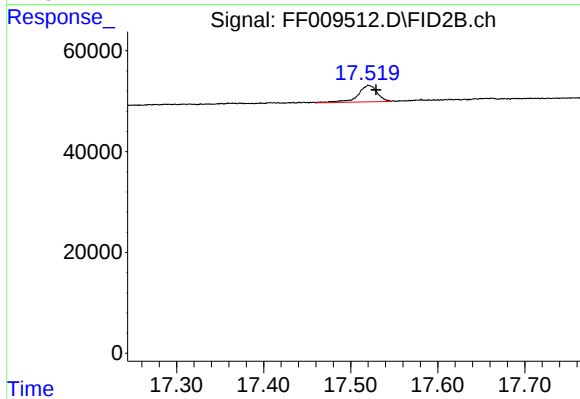

#13 N-TRIACONTANE


R.T.: 17.520 min
Delta R.T.: -0.009 min
Response: 49585
Conc: 0.43 ug/ml

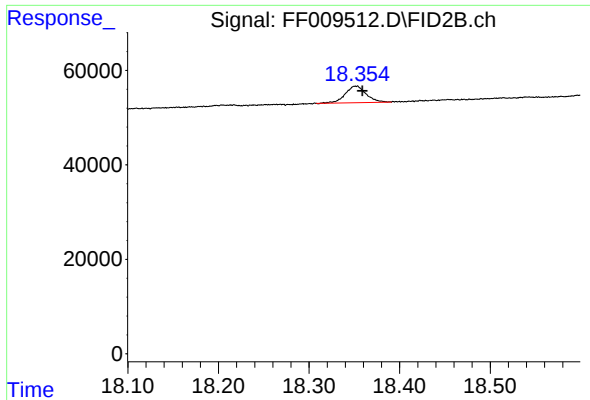

#14 N-DOTRIACONTANE

R.T.: 18.354 min
Delta R.T.: -0.005 min
Response: 56462
Conc: 0.52 ug/ml

Instrument :
FID_F
ClientSampleId :

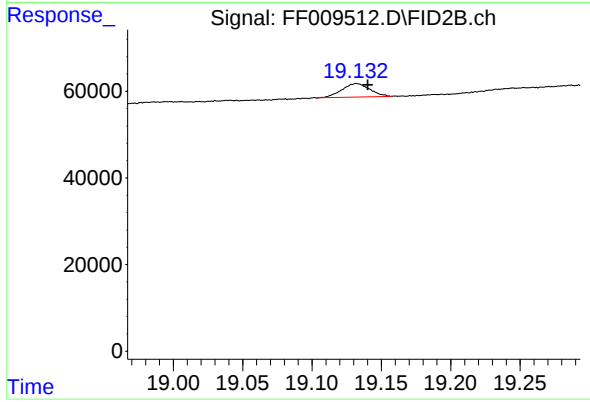

#15 N-TETRATRIACONTANE

R.T.: 19.132 min
Delta R.T.: -0.008 min
Response: 43302
Conc: 0.41 ug/ml