

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122221\
Data File : FF009521.D
Signal(s) : FID2B.ch
Acq On : 22 Dec 2021 18:42
Operator : AJ\MA
Sample : PB141638BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 00:14:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.474	2019330	17.432 ug/ml
Target Compounds				
15)	N-TETRATRIACONTANE	19.135	33198	0.313 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122221\
Data File : FF009521.D
Signal(s) : FID2B.ch
Acq On : 22 Dec 2021 18:42
Operator : AJ\MA
Sample : PB141638BL
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 00:14:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

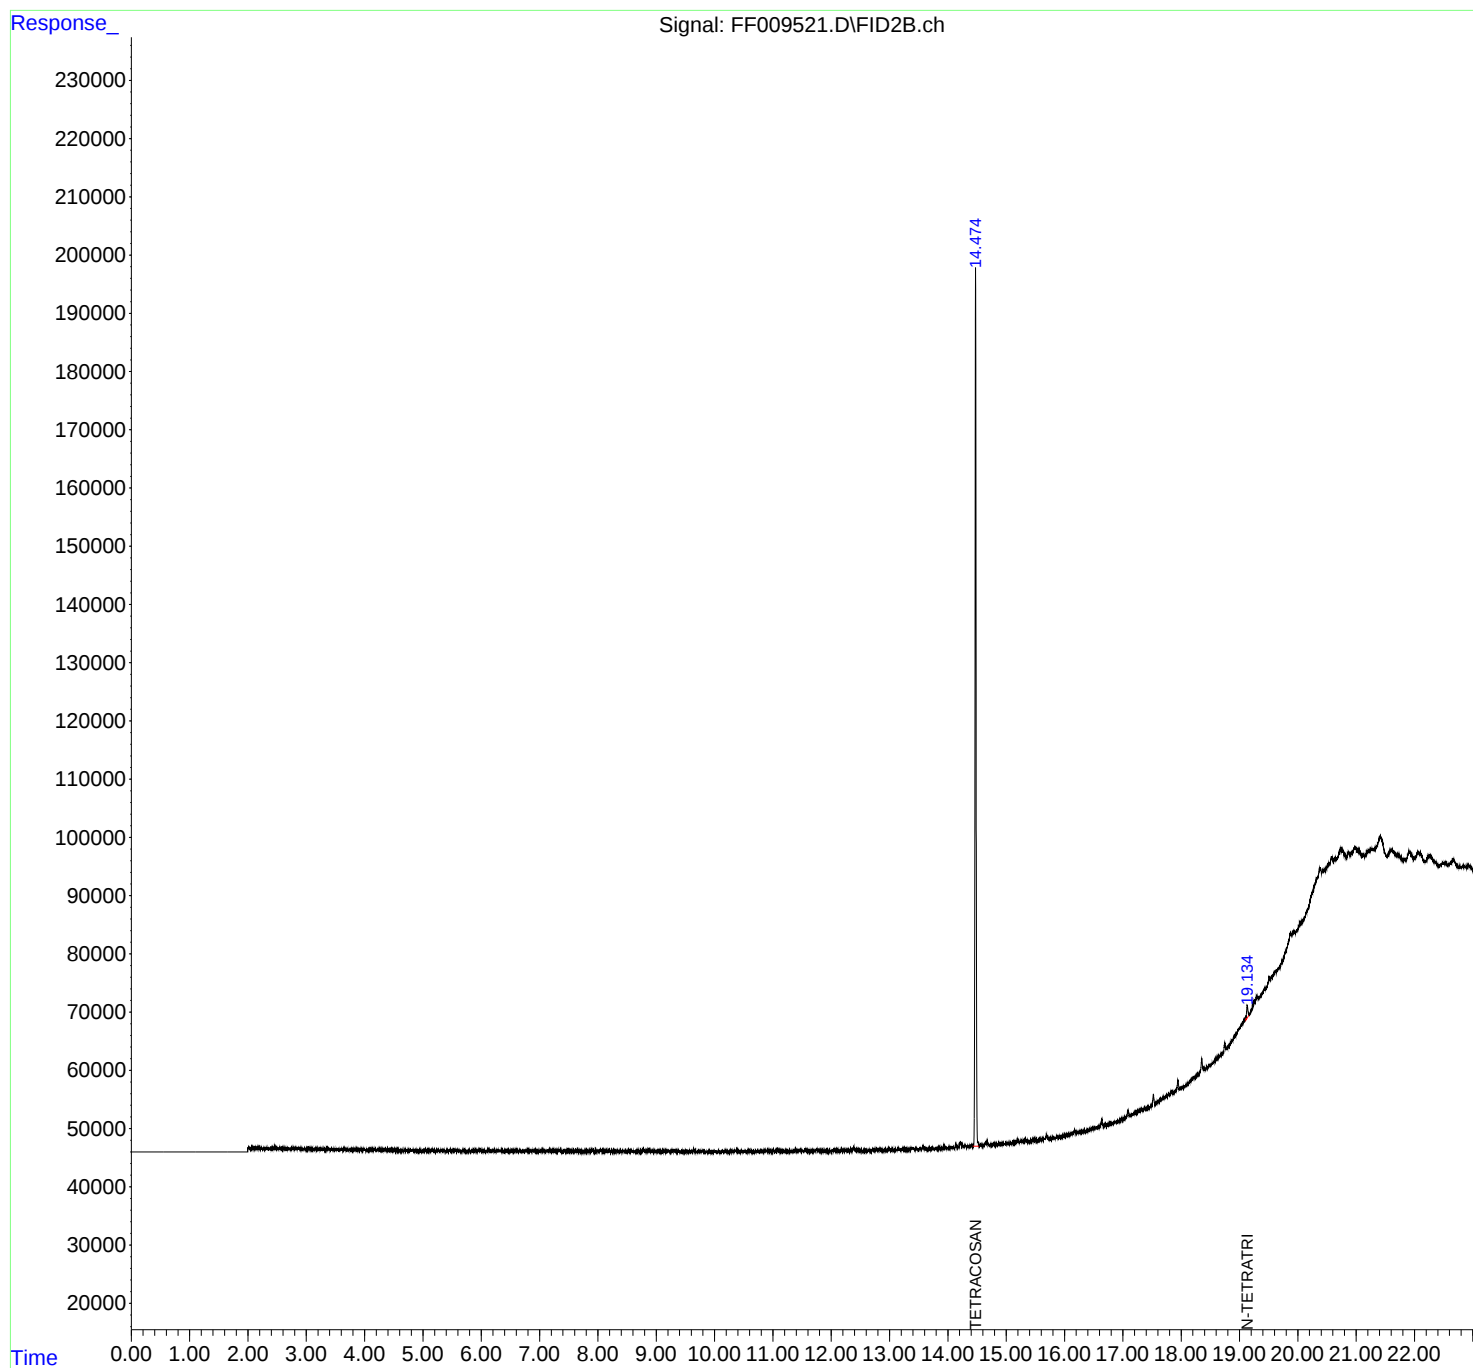


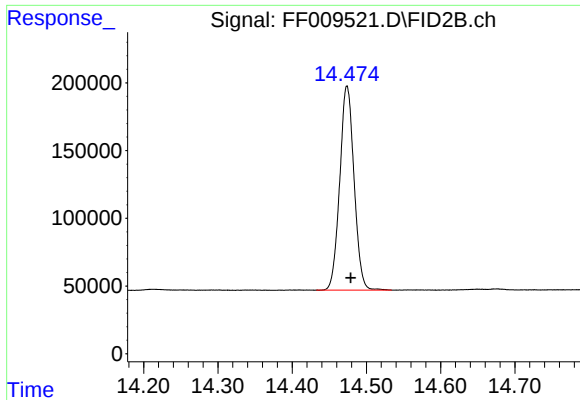

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.474 min
Delta R.T.: -0.005 min
Response: 2019330
Conc: 17.43 ug/ml

Instrument :
FID_F
ClientSampleId :

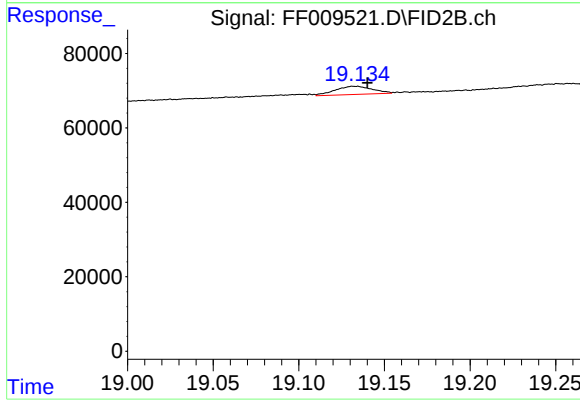

#15 N-TETRATRIACONTANE

R.T.: 19.135 min
Delta R.T.: -0.005 min
Response: 33198
Conc: 0.31 ug/ml