

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122221\
Data File : FF009524.D
Signal(s) : FID2B.ch
Acq On : 22 Dec 2021 20:13
Operator : AJ\MA
Sample : M5182-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 00:15:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.474	2083293	17.984 ug/ml
Target Compounds			
6) N-OCTADECANE	11.079	55076	0.382 ug/ml
7) N-EICOSANE	12.383	733625	5.177 ug/ml
8) N-DOCOSANE	13.577	451753	3.315 ug/ml
10) N-TETRACOSANE	14.674	100446	0.763 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122221\
Data File : FF009524.D
Signal(s) : FID2B.ch
Acq On : 22 Dec 2021 20:13
Operator : AJ\MA
Sample : M5182-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 00:15:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

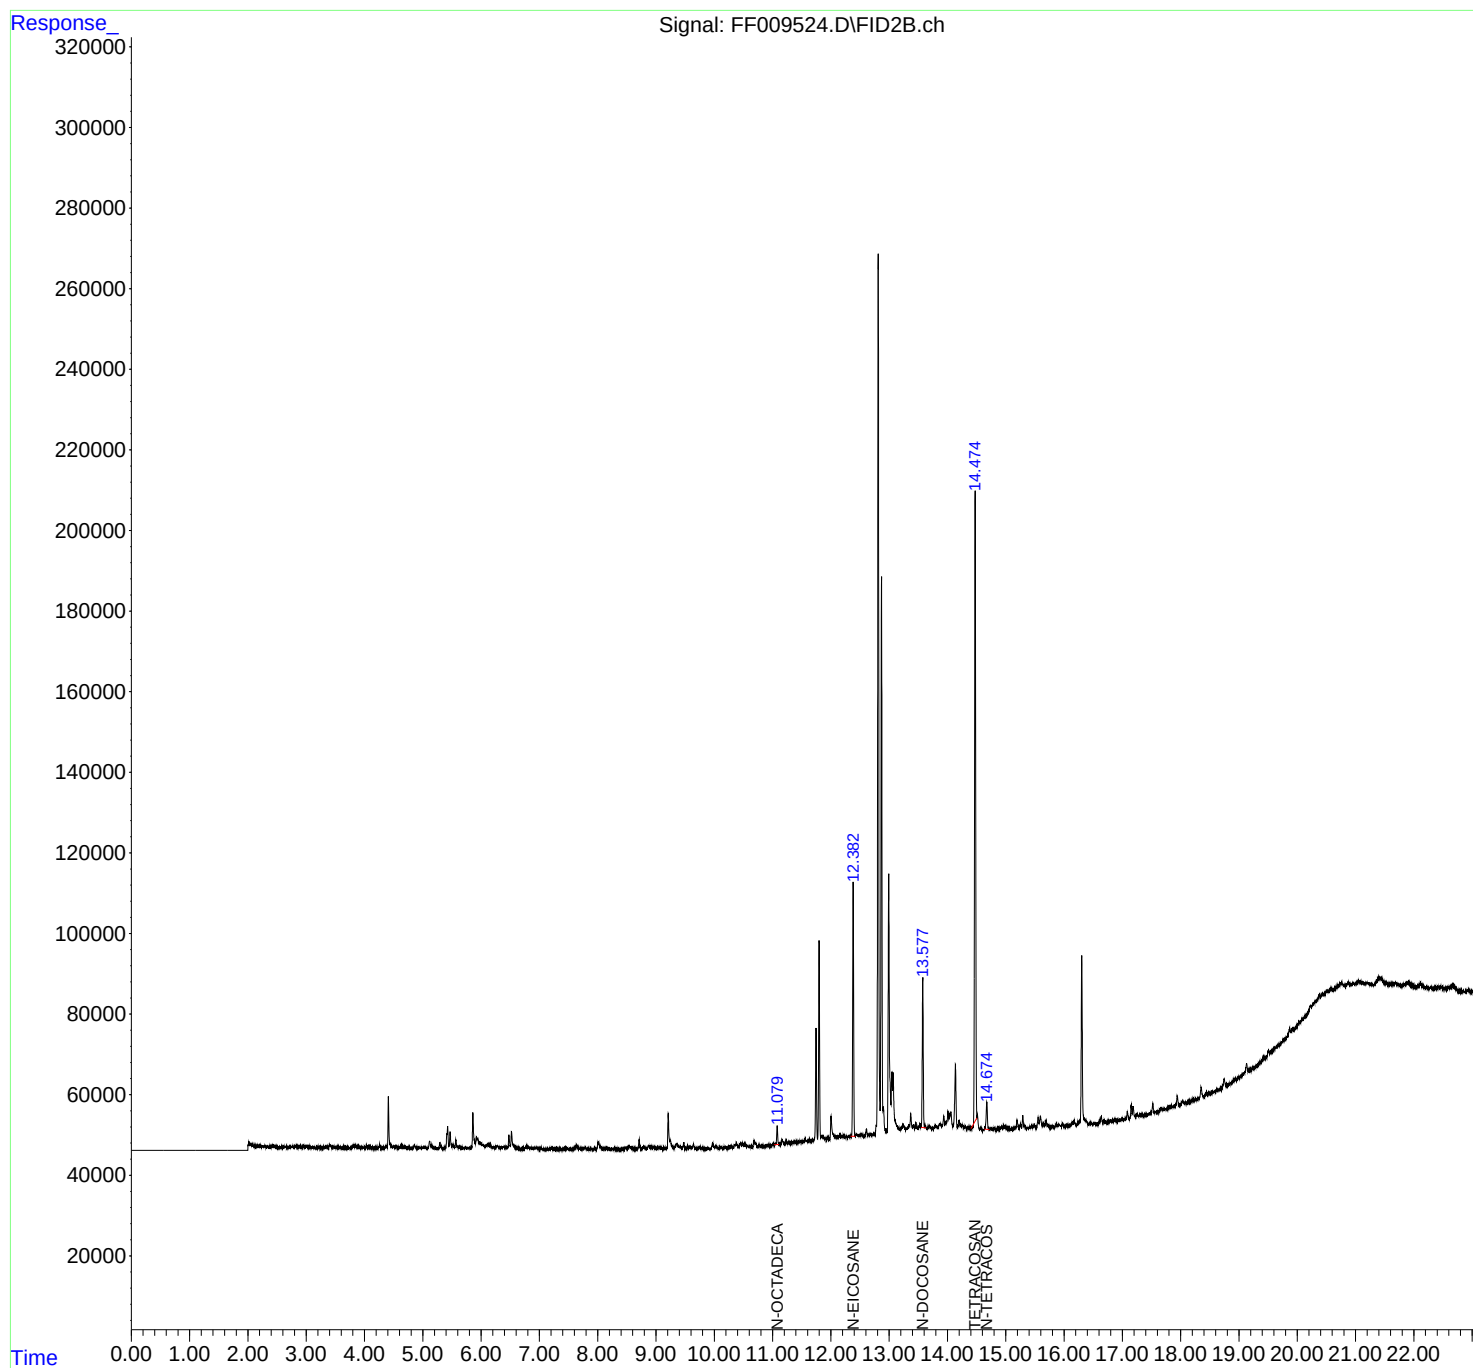


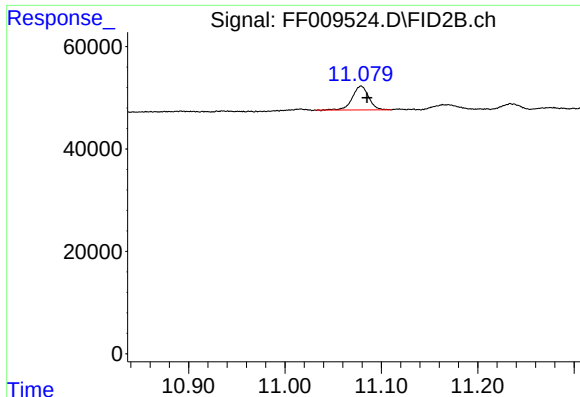

#6 N-OCTADECANE


R.T.: 11.079 min
Delta R.T.: -0.006 min
Response: 55076
Conc: 0.38 ug/ml

Instrument :
FID_F
ClientSampleId :

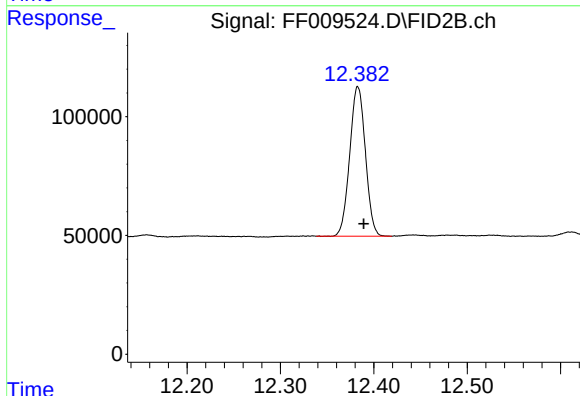


#7 N-EICOSANE

R.T.: 12.383 min
Delta R.T.: -0.007 min
Response: 733625
Conc: 5.18 ug/ml

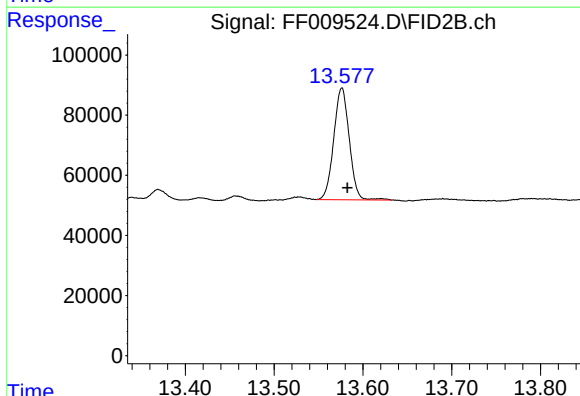


#8 N-DOCOSANE

R.T.: 13.577 min
Delta R.T.: -0.006 min
Response: 451753
Conc: 3.32 ug/ml

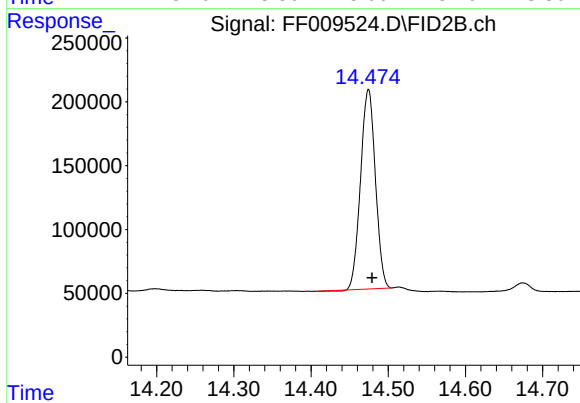

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.474 min
Delta R.T.: -0.005 min
Response: 2083293
Conc: 17.98 ug/ml

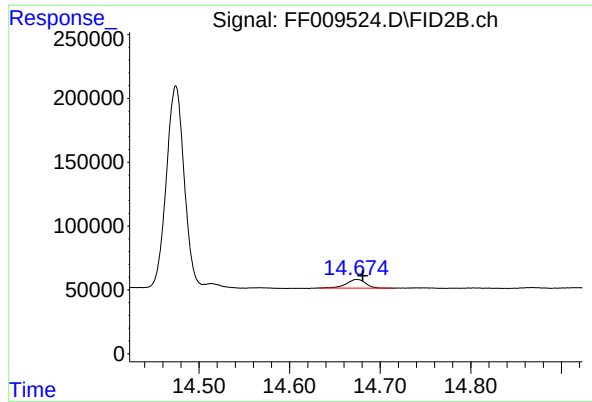

#10 N-TETRACOSANE

R.T.: 14.674 min
Delta R.T.: -0.006 min
Response: 100446
Conc: 0.76 ug/ml

Instrument :
FID_F
ClientSampleId :