

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122221\
Data File : FF009527.D
Signal(s) : FID2B.ch
Acq On : 22 Dec 2021 21:45
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 00:15:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.349	51111	0.468 ug/ml
15) N-TETRATRIACONTANE	19.131	42453	0.401 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122221\
Data File : FF009527.D
Signal(s) : FID2B.ch
Acq On : 22 Dec 2021 21:45
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 23 00:15:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

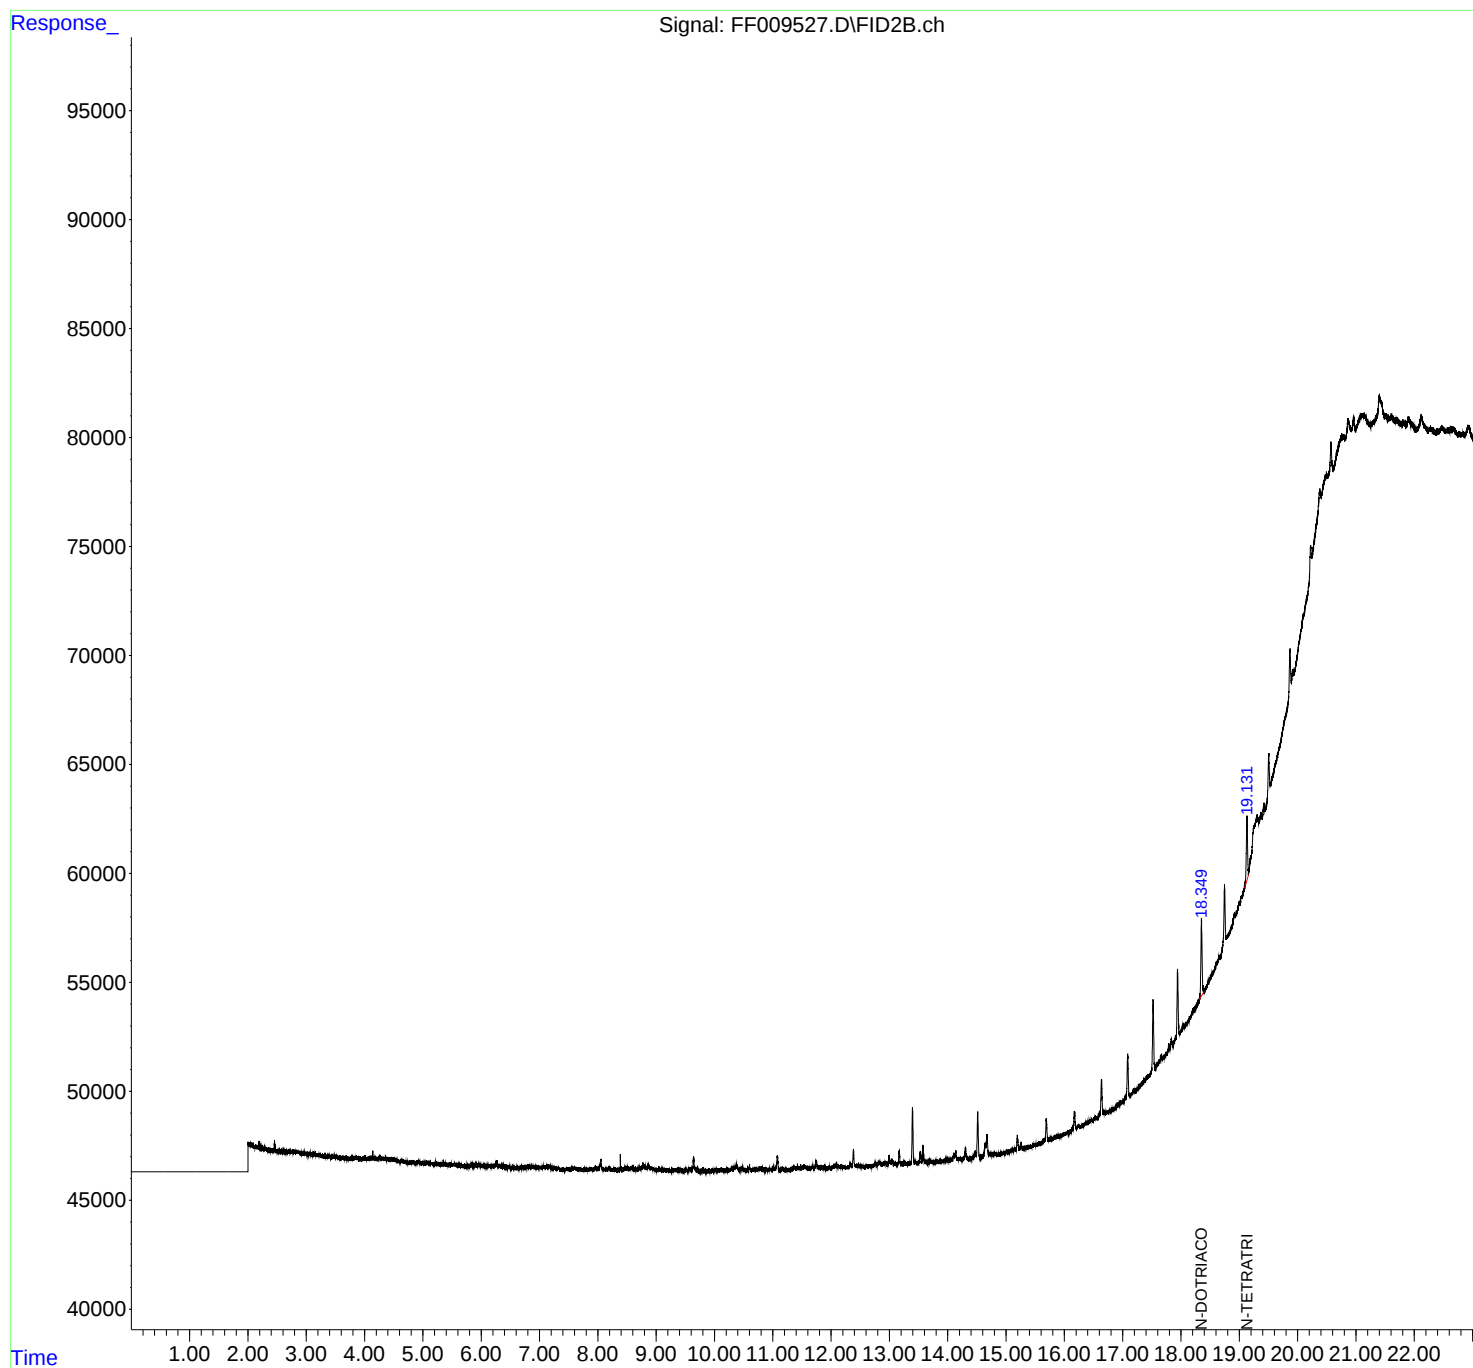


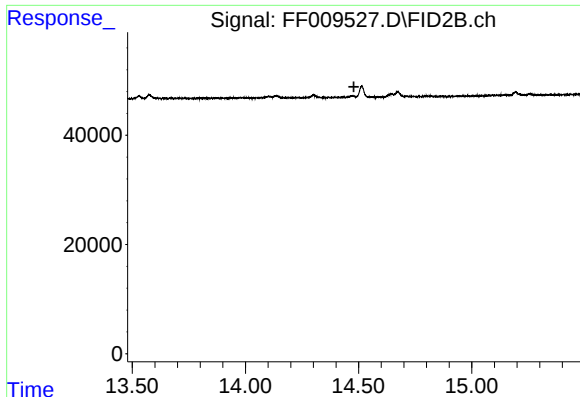

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.479 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

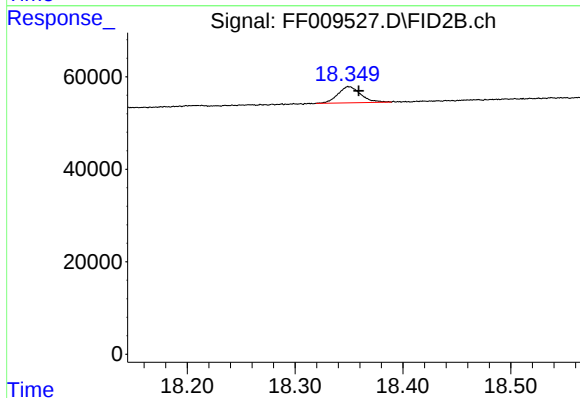

#14 N-DOTRIACONTANE

R.T.: 18.349 min
Delta R.T.: -0.010 min
Response: 51111
Conc: 0.47 ug/ml

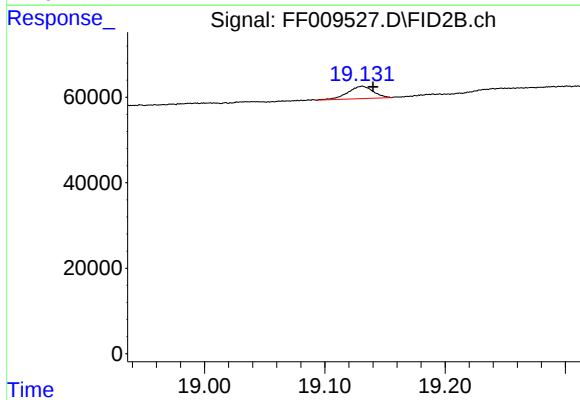

#15 N-TETRATRIACONTANE

R.T.: 19.131 min
Delta R.T.: -0.009 min
Response: 42453
Conc: 0.40 ug/ml