

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122321\
Data File : FF009532.D
Signal(s) : FID2B.ch
Acq On : 23 Dec 2021 10:51
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 24 00:30:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.265	3155339	21.819 ug/ml
12)	N-OCTACOSANE	16.638	2526358	21.216 ug/ml
13)	N-TRIACONTANE	17.519	65217	0.569 ug/ml
14)	N-DOTRIACONTANE	18.349	85651	0.784 ug/ml
15)	N-TETRATRIACONTANE	19.129	69261	0.654 ug/ml
16)	N-HEXATRIACONTANE	19.866	44359	0.443 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122321\
Data File : FF009532.D
Signal(s) : FID2B.ch
Acq On : 23 Dec 2021 10:51
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 24 00:30:08 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

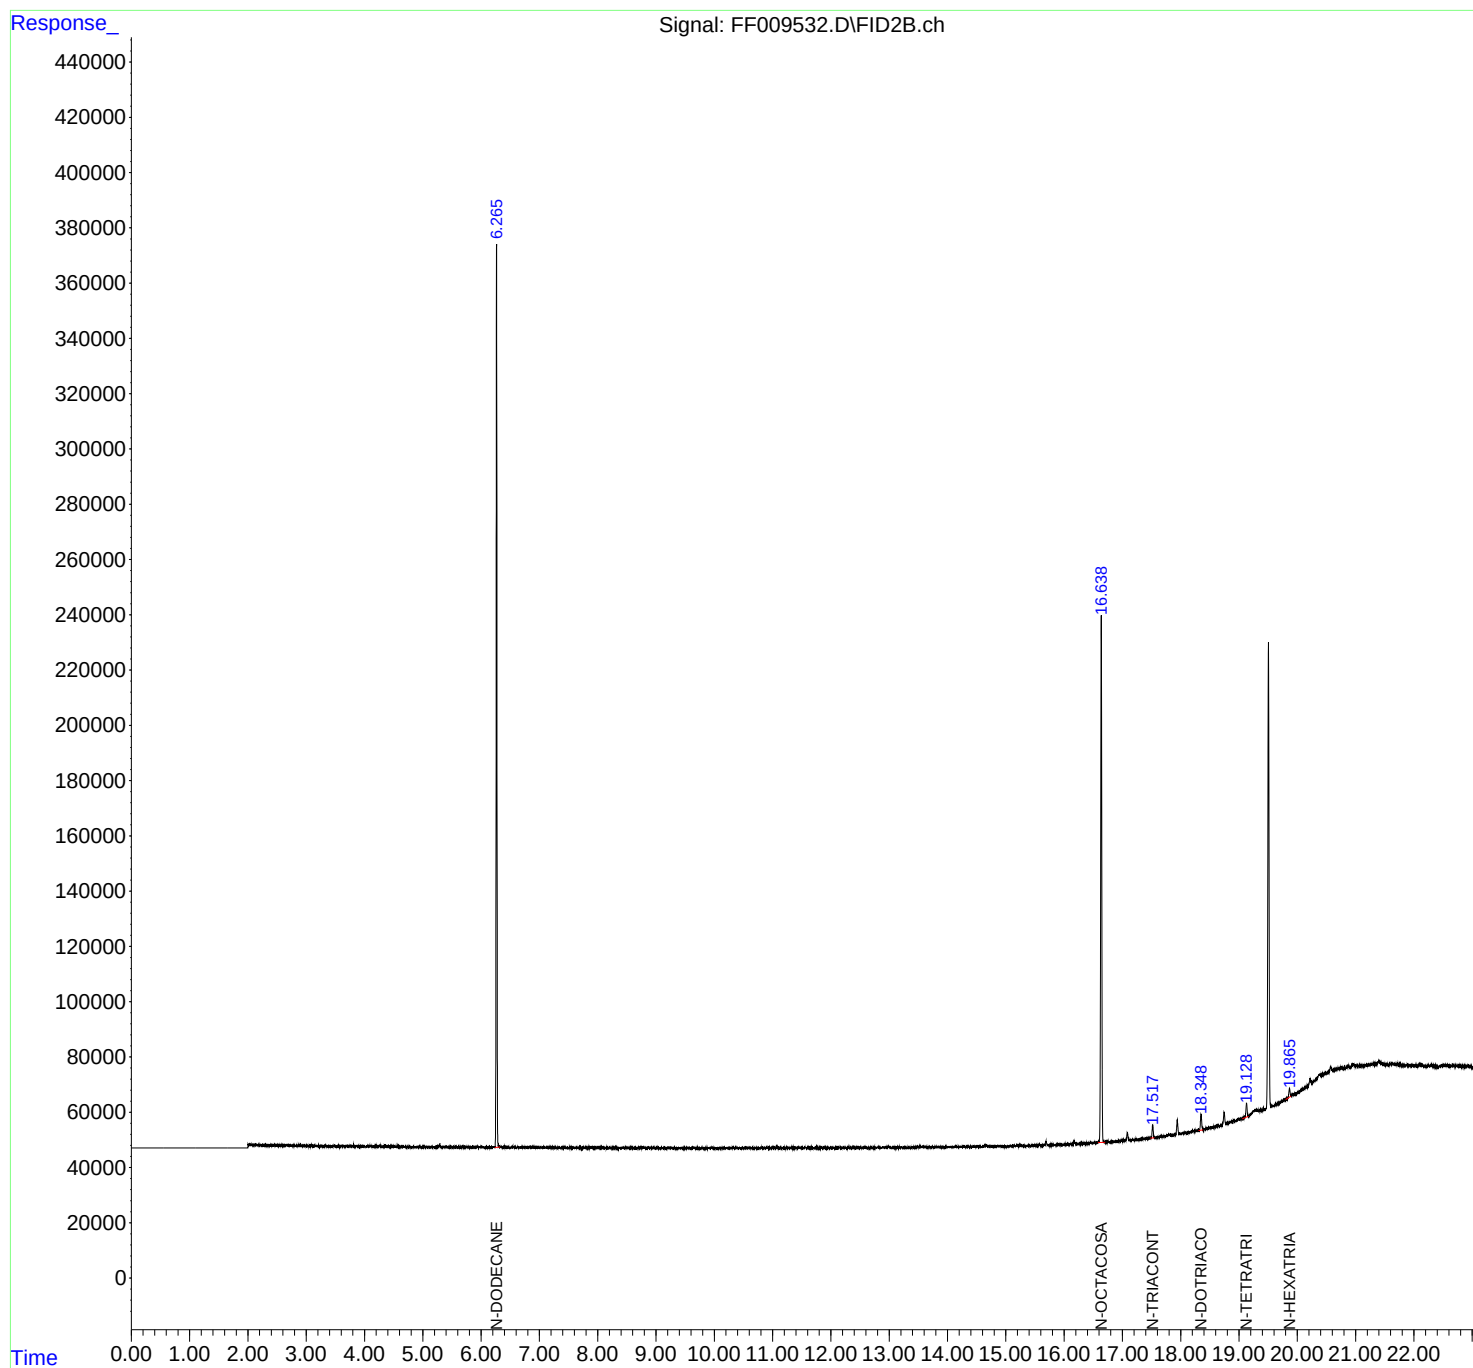


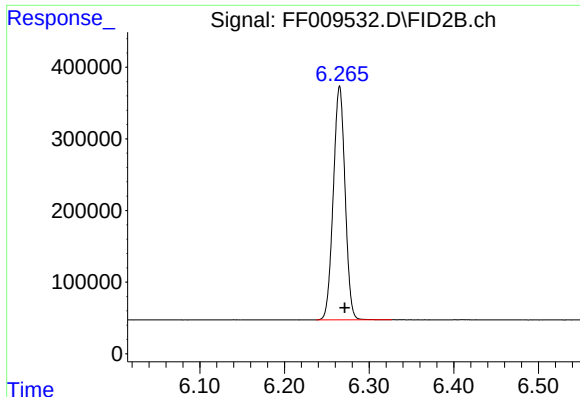

#3 N-DODECANE


R.T.: 6.265 min
Delta R.T.: -0.006 min
Response: 3155339
Conc: 21.82 ug/ml

Instrument :
FID_F
ClientSampleId :

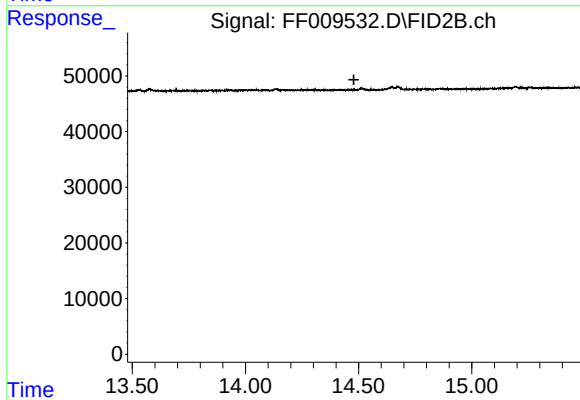


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

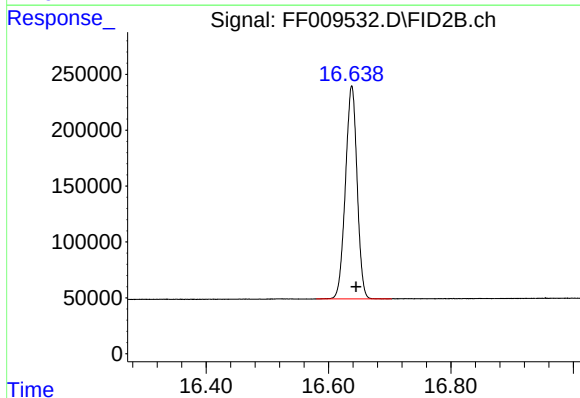


#12 N-OCTACOSANE

R.T.: 16.638 min
Delta R.T.: -0.007 min
Response: 2526358
Conc: 21.22 ug/ml

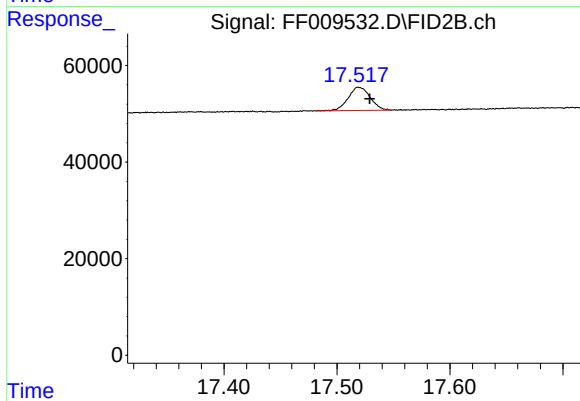

#13 N-TRIACONTANE


R.T.: 17.519 min
Delta R.T.: -0.010 min
Response: 65217
Conc: 0.57 ug/ml

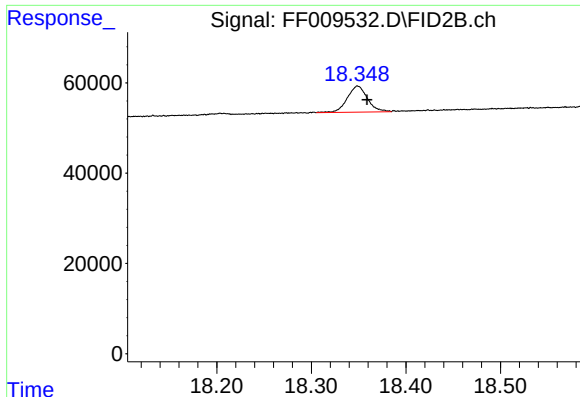

#14 N-DOTRIACONTANE


R.T.: 18.349 min
Delta R.T.: -0.010 min
Response: 85651
Conc: 0.78 ug/ml

Instrument :
FID_F
ClientSampleId :

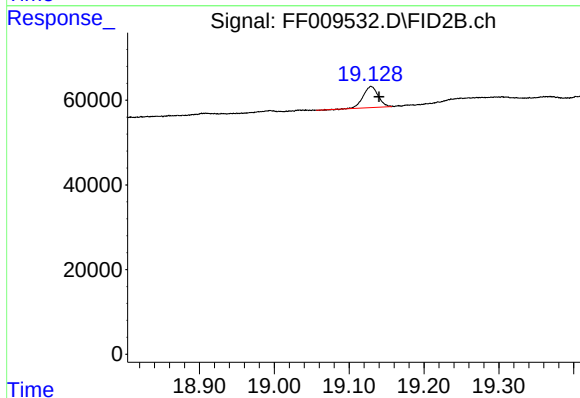

#15 N-TETRATRIACONTANE

R.T.: 19.129 min
Delta R.T.: -0.011 min
Response: 69261
Conc: 0.65 ug/ml

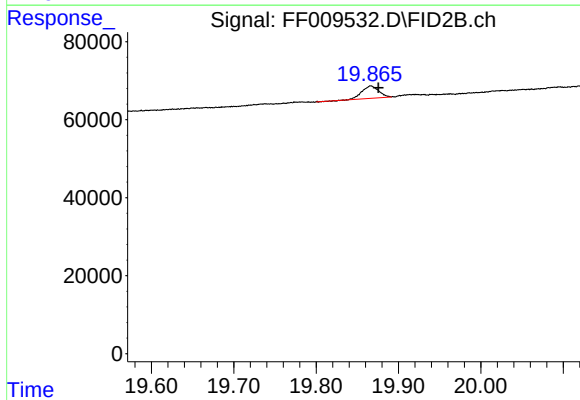

#16 N-HEXATRIACONTANE

R.T.: 19.866 min
Delta R.T.: -0.010 min
Response: 44359
Conc: 0.44 ug/ml