

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122321\
 Data File : FF009547.D
 Signal(s) : FID2B.ch
 Acq On : 23 Dec 2021 18:59
 Operator : AJ\MA
 Sample : M5223-03
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 24 00:34:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.471	1539293	13.288 ug/ml
Target Compounds			
4) N-TETRADECANE	8.048	92943	0.639 ug/ml
6) N-OCTADECANE	11.154f	64475	0.447 ug/ml
10) N-TETRACOSANE	14.715	48267	0.367 ug/ml
11) N-HEXACOSANE	15.685	61139	0.489 ug/ml
13) N-TRIACONTANE	17.517	79632	0.695 ug/ml
14) N-DOTRIACONTANE	18.345	149626	1.369 ug/ml
15) N-TETRATRIACONTANE	19.126	79537	0.751 ug/ml
16) N-HEXATRIACONTANE	19.864	59197	0.591 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122321\
Data File : FF009547.D
Signal(s) : FID2B.ch
Acq On : 23 Dec 2021 18:59
Operator : AJ\MA
Sample : M5223-03
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 24 00:34:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

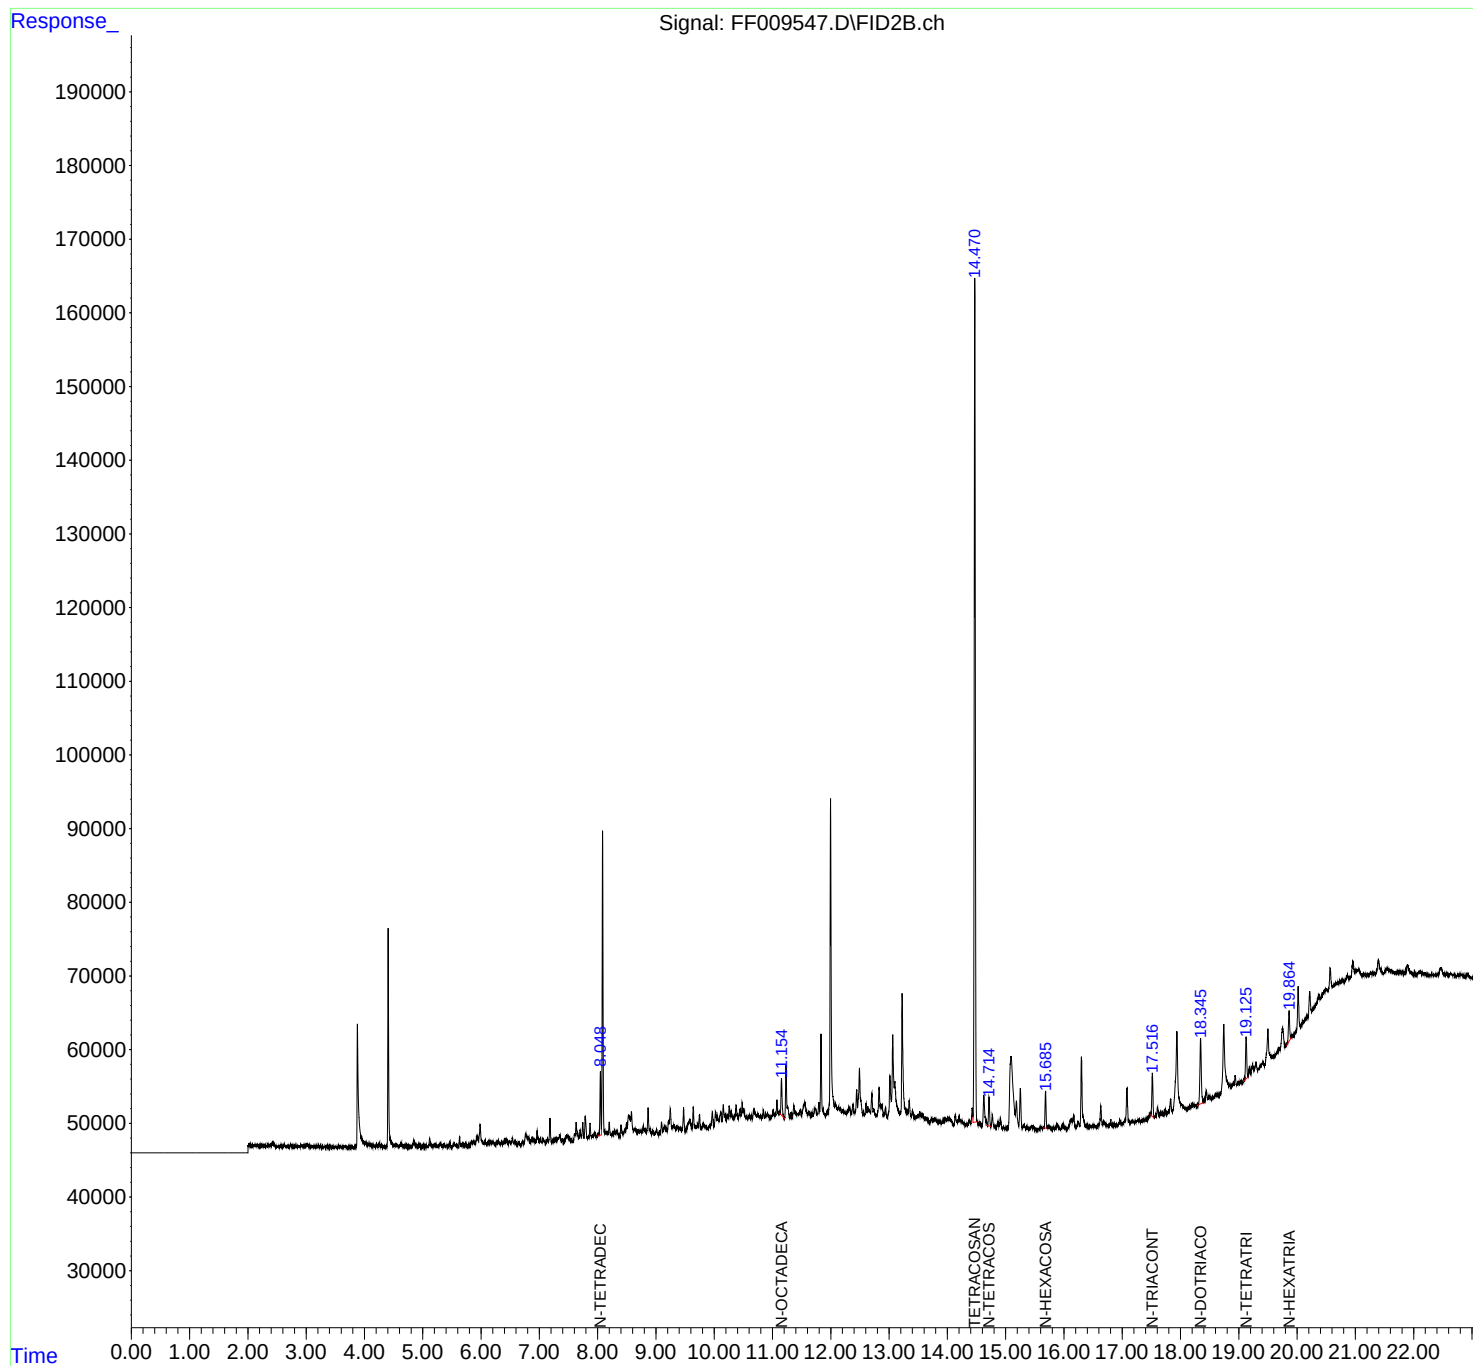


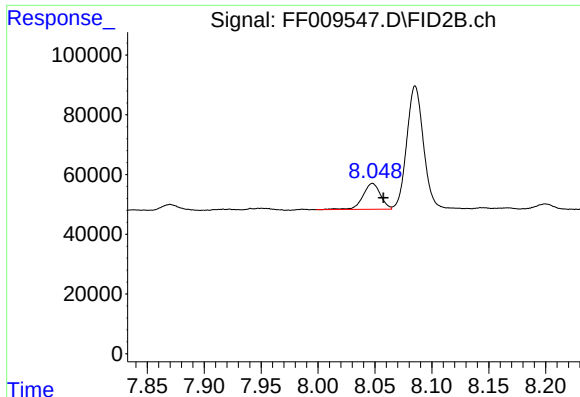

#4 N-TETRADECANE


R.T.: 8.048 min
Delta R.T.: -0.009 min
Response: 92943
Conc: 0.64 ug/ml

Instrument :
FID_F
ClientSampleId :

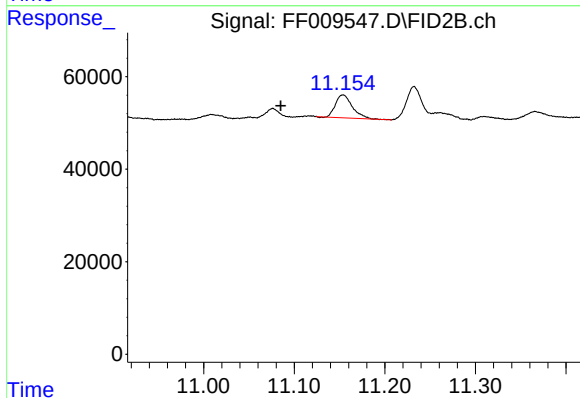


#6 N-OCTADECANE

R.T.: 11.154 min
Delta R.T.: 0.069 min
Response: 64475
Conc: 0.45 ug/ml

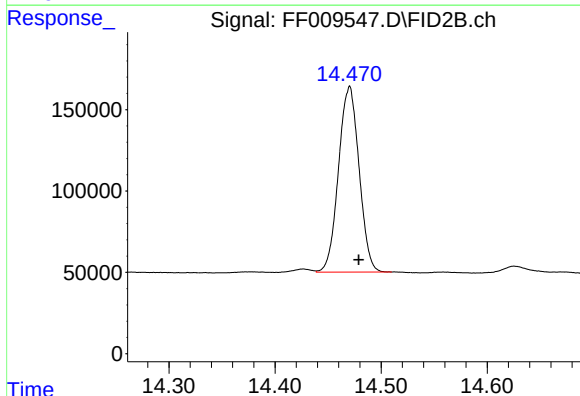


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.471 min
Delta R.T.: -0.009 min
Response: 1539293
Conc: 13.29 ug/ml

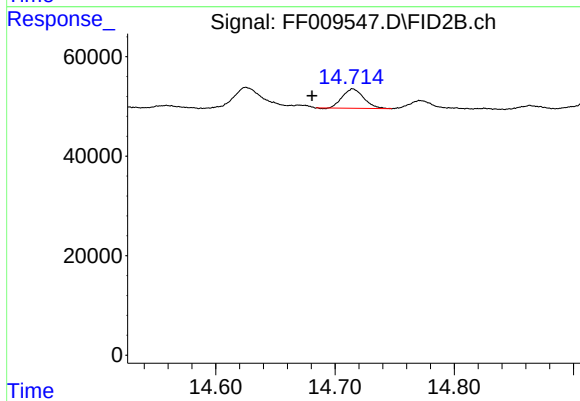

#10 N-TETRACOSANE


R.T.: 14.715 min
Delta R.T.: 0.034 min
Response: 48267
Conc: 0.37 ug/ml

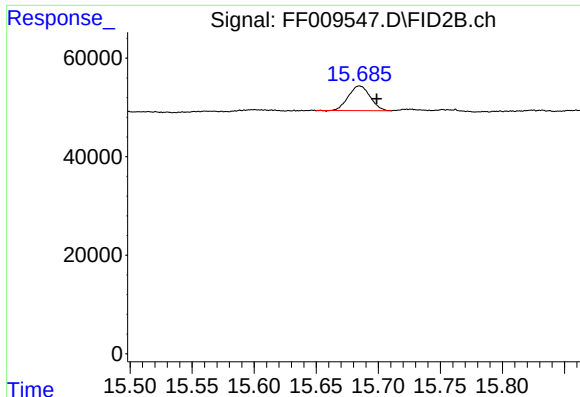

#11 N-HEXACOSANE


R.T.: 15.685 min
Delta R.T.: -0.014 min
Response: 61139
Conc: 0.49 ug/ml

Instrument :
FID_F
ClientSampleId :

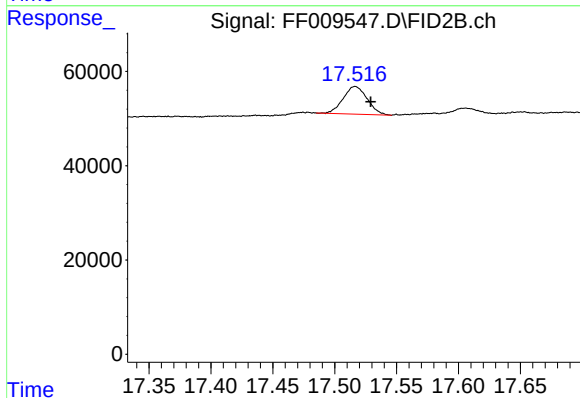


#13 N-TRIACONTANE

R.T.: 17.517 min
Delta R.T.: -0.013 min
Response: 79632
Conc: 0.70 ug/ml

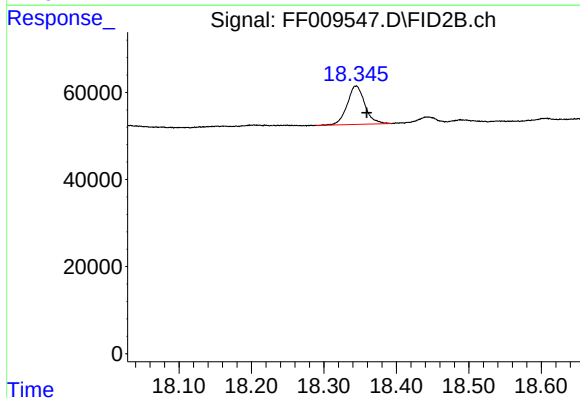


#14 N-DOTRIACONTANE

R.T.: 18.345 min
Delta R.T.: -0.014 min
Response: 149626
Conc: 1.37 ug/ml

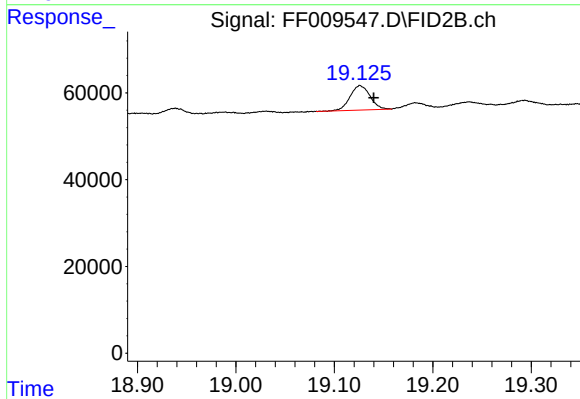

#15 N-TETRATRIACONTANE

R.T.: 19.126 min
Delta R.T.: -0.014 min
Response: 79537
Conc: 0.75 ug/ml

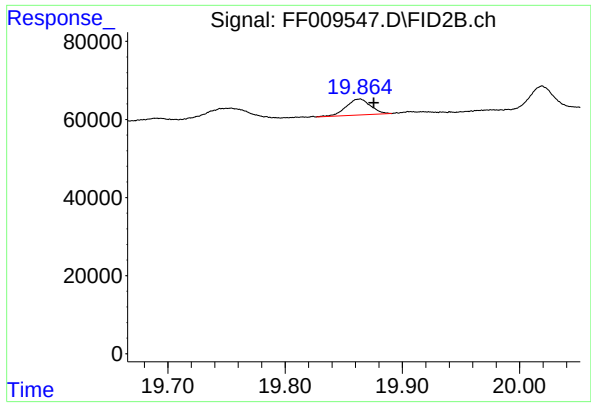

#16 N-HEXATRIACONTANE

R.T.: 19.864 min
Delta R.T.: -0.011 min
Response: 59197
Conc: 0.59 ug/ml

Instrument :

FID_F

ClientSampleId :