

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122321\
Data File : FF009536.D
Signal(s) : FID2B.ch
Acq On : 23 Dec 2021 12:53
Operator : AJ\MA
Sample : M5191-03 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TP-(3.5-7.0)-12-21-2021

Integration File: autoint1.e
Quant Time: Dec 24 00:43:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.471	273481	2.361 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122321\
Data File : FF009536.D
Signal(s) : FID2B.ch
Acq On : 23 Dec 2021 12:53
Operator : AJ\MA
Sample : M5191-03 5X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TP-(3.5-7.0)-12-21-2021

Integration File: autoint1.e
Quant Time: Dec 24 00:43:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

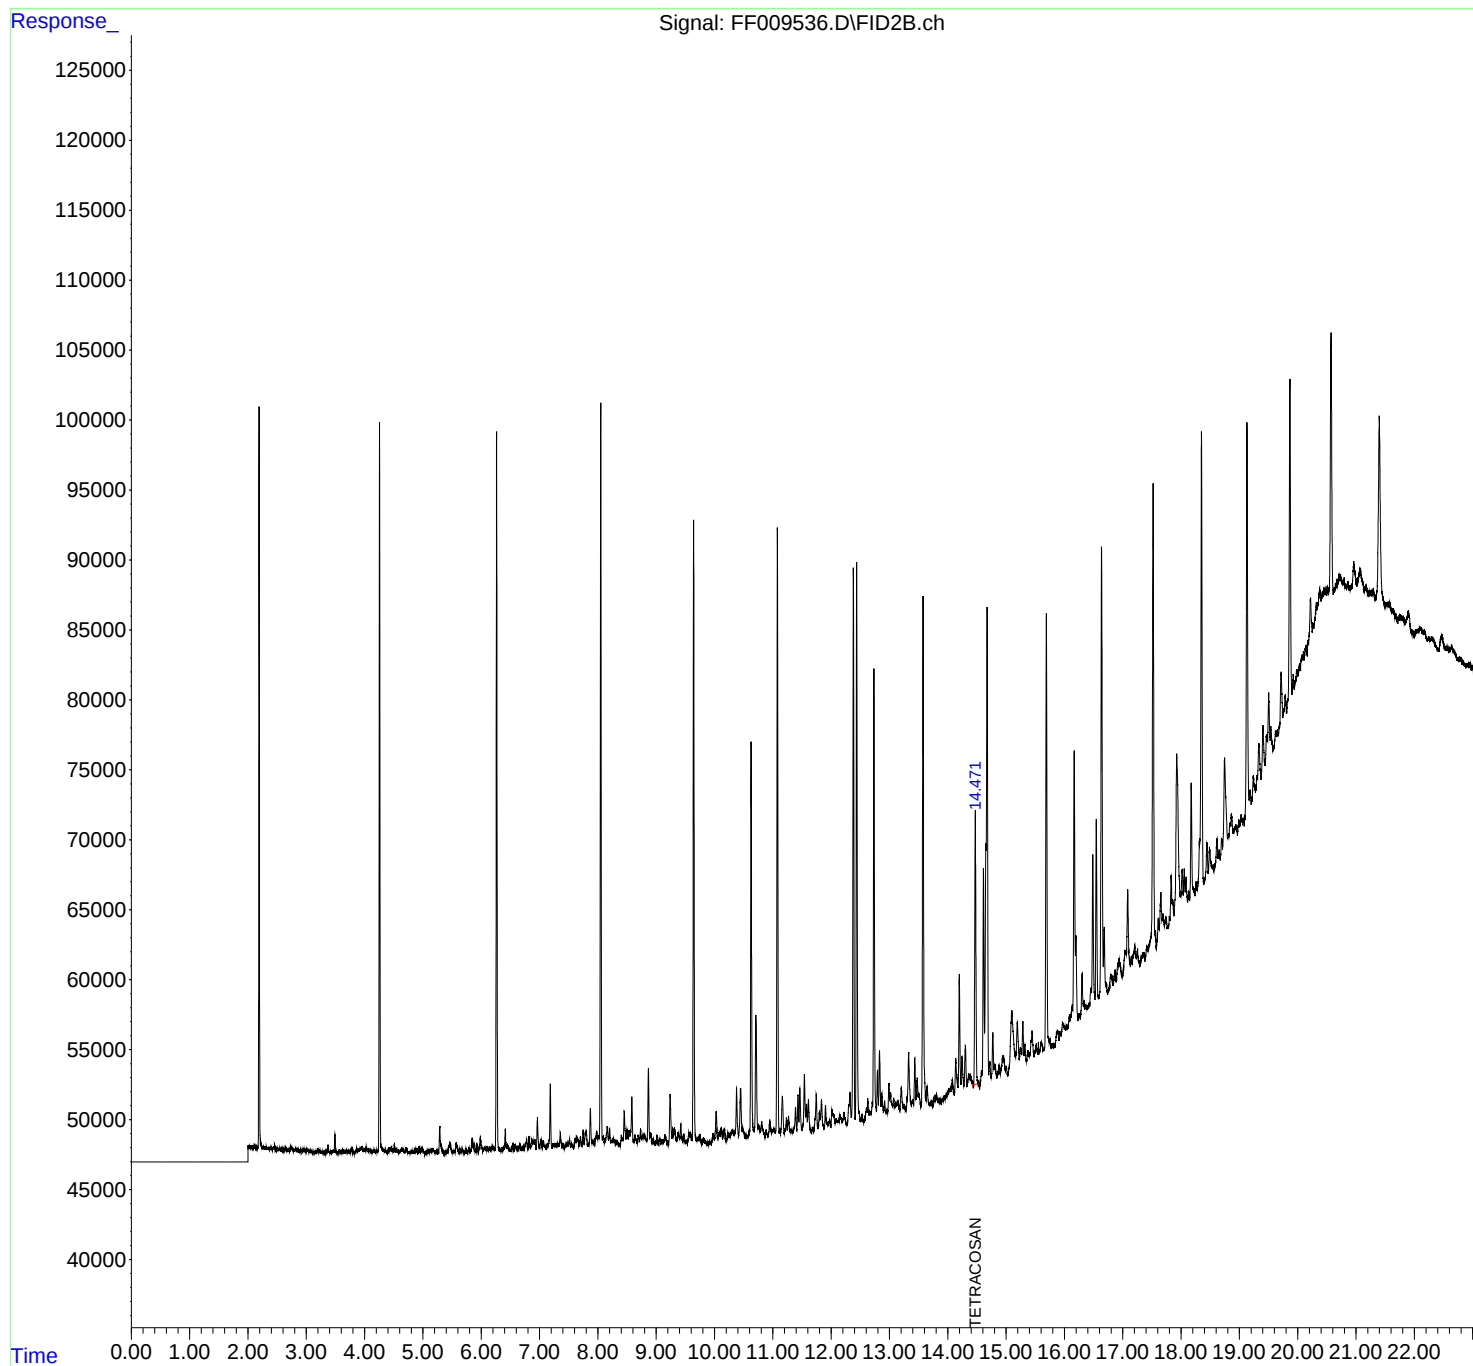

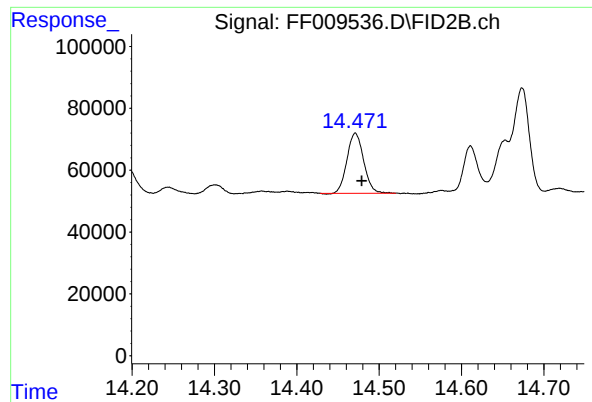

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.471 min
Delta R.T.: -0.008 min
Response: 273481
Conc: 2.36 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-(3.5-7.0)-12-21-2021