

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122619\
 Data File : FF006076.D
 Signal(s) : FID2B.ch
 Acq On : 26 Dec 2019 14:43
 Operator : DD\AJ
 Sample : K6413-06
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 K005-AA-WC-1

Integration File: autoint1.e
 Quant Time: Dec 27 01:12:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.641	3045752	20.964 ug/ml
Target Compounds			
4) N-TETRADECANE	8.265f	1244680	7.340 ug/ml
7) N-EICOSANE	12.608f	691577	4.004 ug/ml
10) N-TETRACOSANE	14.821	392271	2.350 ug/ml
11) N-HEXACOSANE	15.860	172870	1.073 ug/ml
12) N-OCTACOSANE	16.808	295803	1.928 ug/ml
13) N-TRIACONTANE	17.692	514576	3.547 ug/ml
14) N-DOTRIACONTANE	18.522	293694	2.115 ug/ml
15) N-TETRATRIACONTANE	19.309	98573	0.751 ug/ml
17) N-OCTATRIACONTANE	20.766	747894	6.373 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122619\
Data File : FF006076.D
Signal(s) : FID2B.ch
Acq On : 26 Dec 2019 14:43
Operator : DD\AJ
Sample : K6413-06
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
K005-AA-WC-1

Integration File: autoint1.e
Quant Time: Dec 27 01:12:21 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

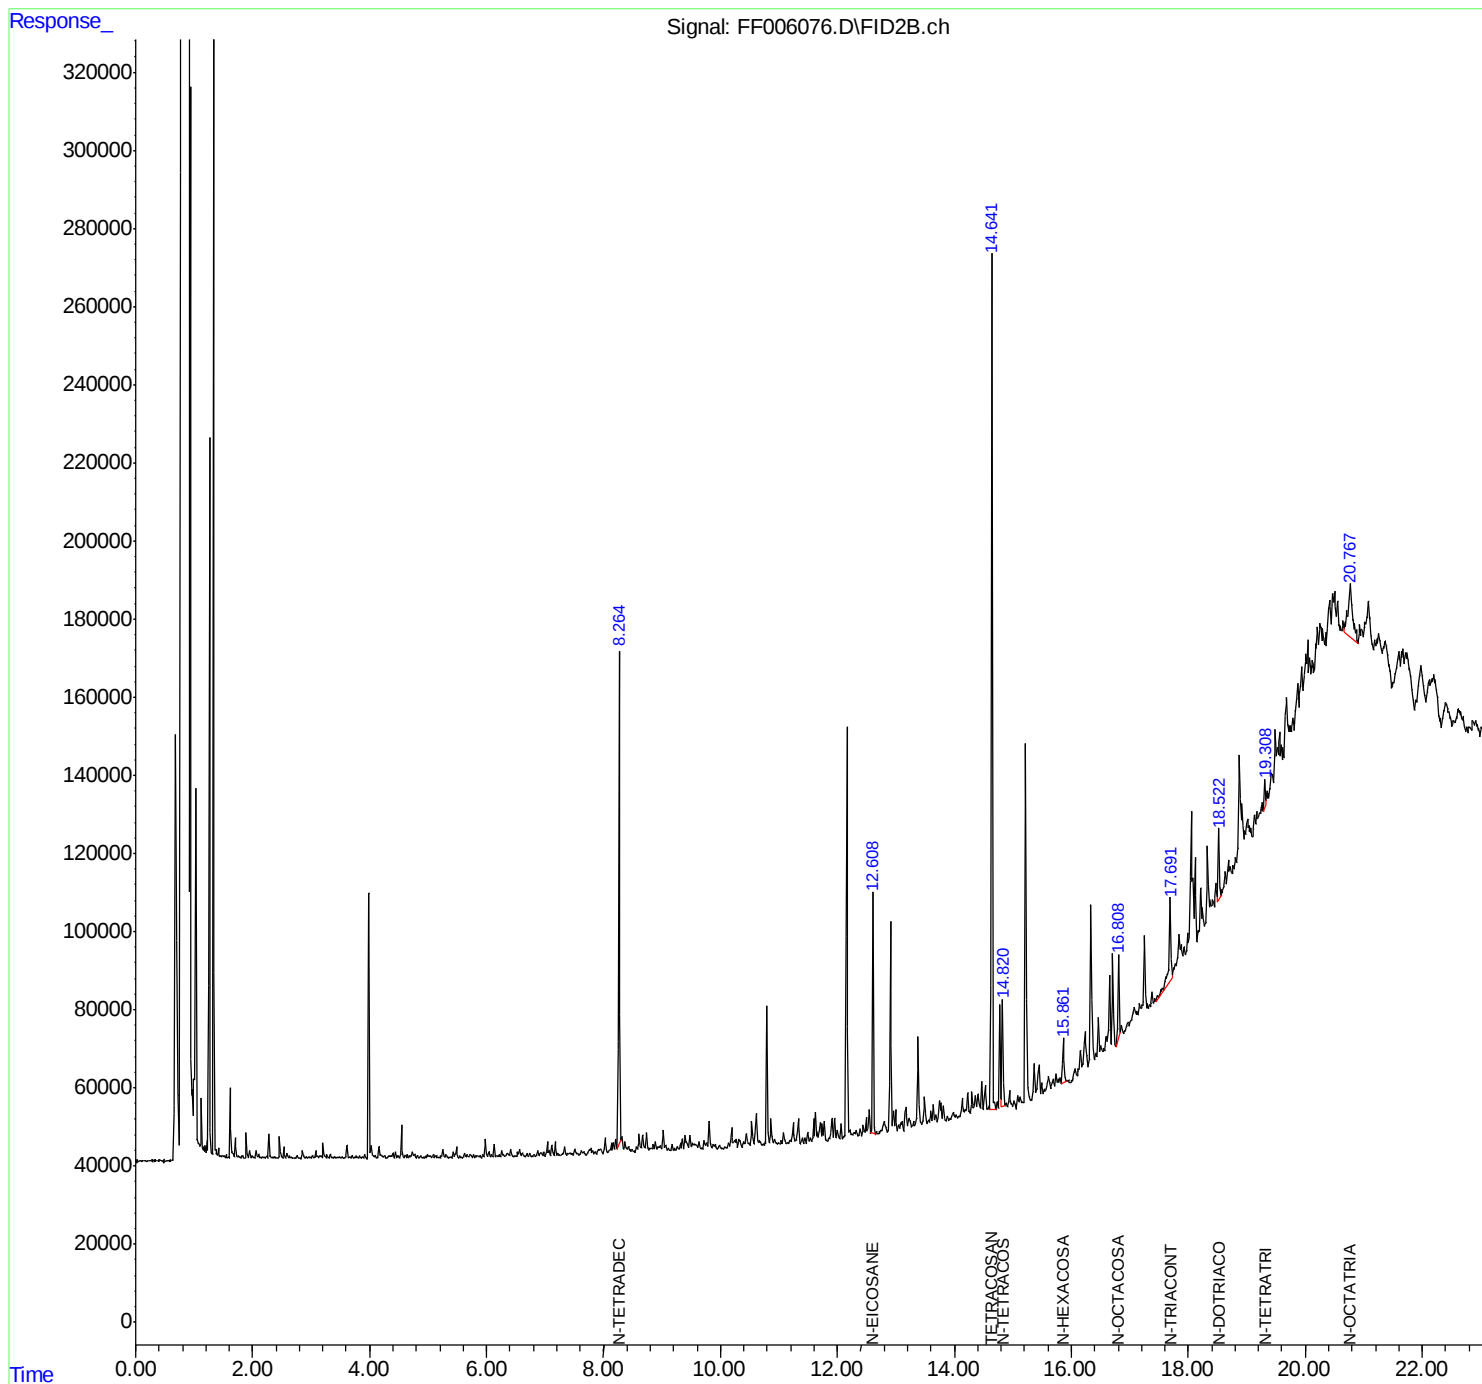


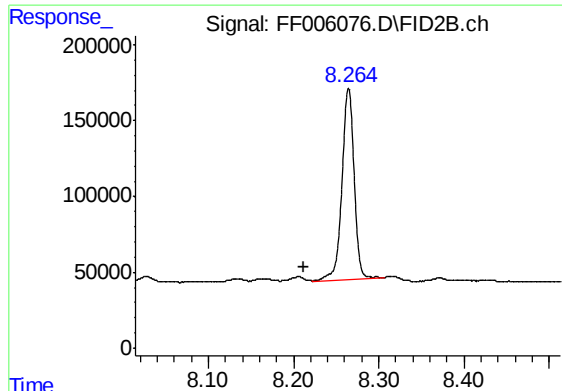

#4 N-TETRADECANE


R.T.: 8.265 min
Delta R.T.: 0.052 min
Response: 1244680
Conc: 7.34 ug/ml

Instrument :
FID_F
ClientSampleId :
K005-AA-WC-1

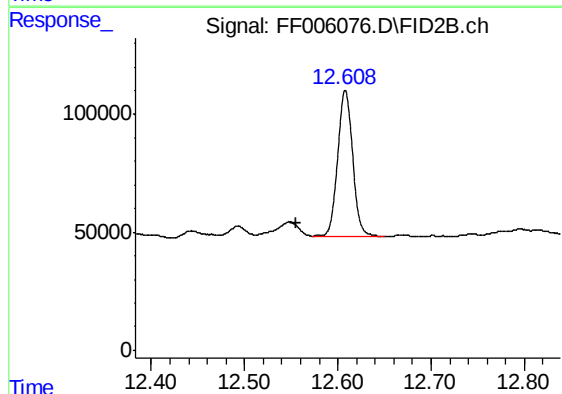


#7 N-EICOSANE

R.T.: 12.608 min
Delta R.T.: 0.053 min
Response: 691577
Conc: 4.00 ug/ml

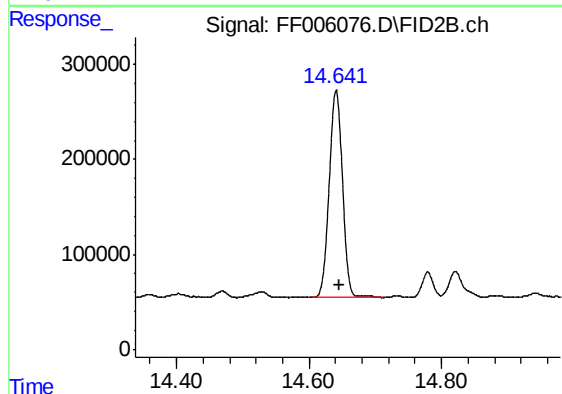


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.641 min
Delta R.T.: -0.006 min
Response: 3045752
Conc: 20.96 ug/ml

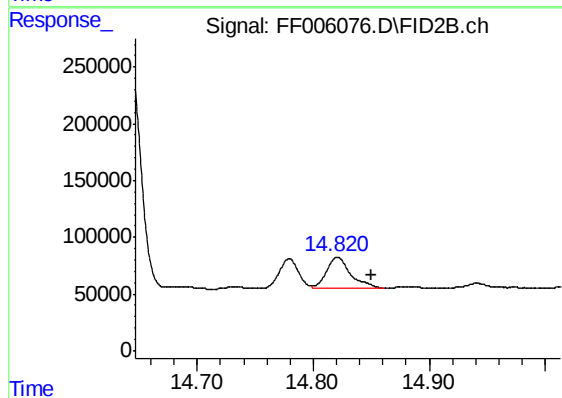

#10 N-TETRACOSANE


R.T.: 14.821 min
Delta R.T.: -0.030 min
Response: 392271
Conc: 2.35 ug/ml

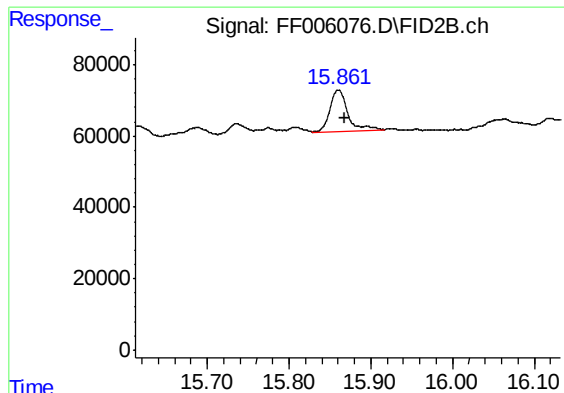

#11 N-HEXACOSANE


R.T.: 15.860 min
Delta R.T.: -0.008 min
Response: 172870
Conc: 1.07 ug/ml

Instrument :
FID_F
ClientSampleId :
K005-AA-WC-1

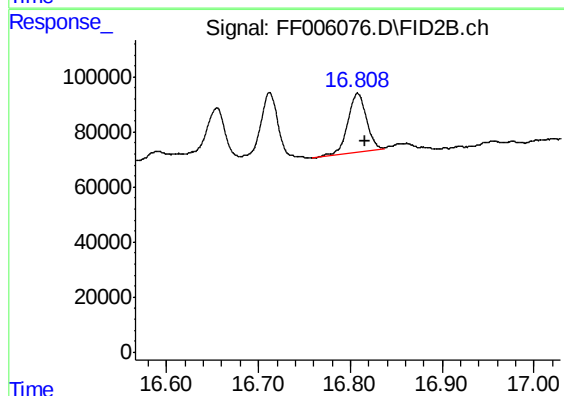


#12 N-OCTACOSANE

R.T.: 16.808 min
Delta R.T.: -0.008 min
Response: 295803
Conc: 1.93 ug/ml

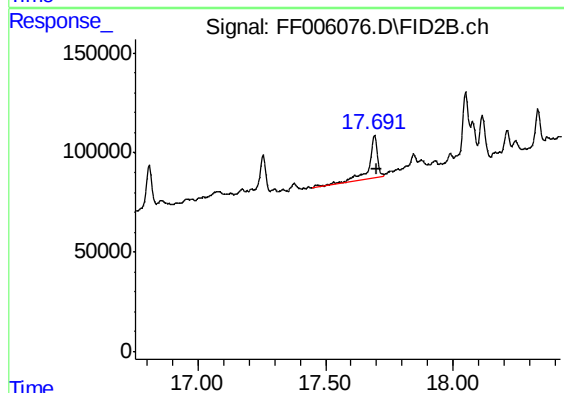


#13 N-TRIACONTANE

R.T.: 17.692 min
Delta R.T.: -0.009 min
Response: 514576
Conc: 3.55 ug/ml

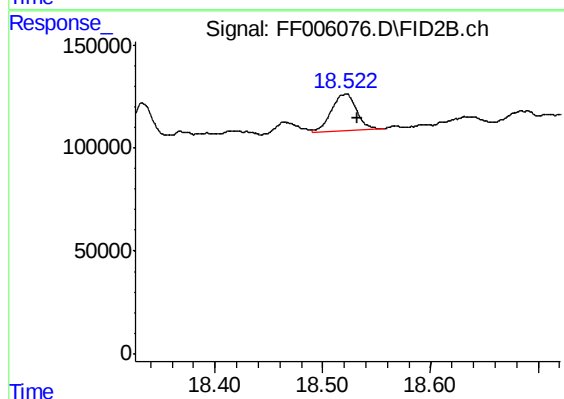

#14 N-DOTRIACONTANE


R.T.: 18.522 min
Delta R.T.: -0.011 min
Response: 293694
Conc: 2.11 ug/ml

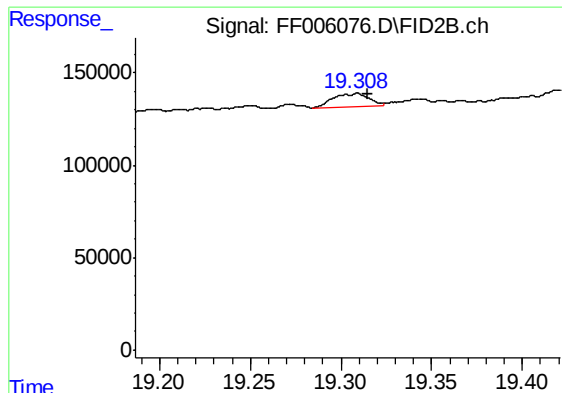

#15 N-TETRATRIACONTANE

R.T.: 19.309 min
Delta R.T.: -0.006 min
Response: 98573
Conc: 0.75 ug/ml

Instrument :
FID_F
ClientSampleId :
K005-AA-WC-1

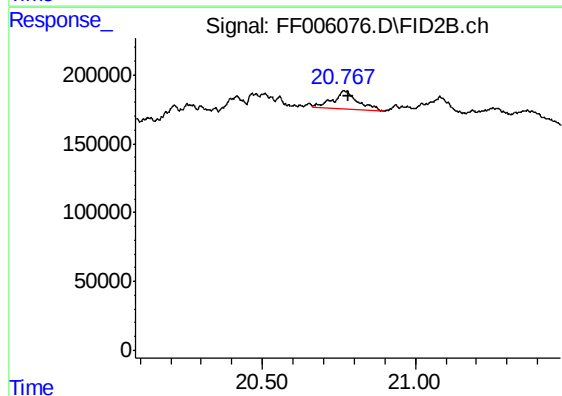

#17 N-OCTATRIACONTANE

R.T.: 20.766 min
Delta R.T.: -0.015 min
Response: 747894
Conc: 6.37 ug/ml