

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122619\
 Data File : FF006078.D
 Signal(s) : FID2B.ch
 Acq On : 26 Dec 2019 15:43
 Operator : DD\AJ
 Sample : K6413-07 2X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 K005-AA-WC-2

Integration File: autoint1.e
 Quant Time: Dec 27 01:12:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.639	1082072	7.448 ug/ml
Target Compounds			
4) N-TETRADECANE	8.264f	523339	3.086 ug/ml
7) N-EICOSANE	12.608f	834287	4.831 ug/ml
10) N-TETRACOSANE	14.822	469115	2.811 ug/ml
11) N-HEXACOSANE	15.863	543072	3.372 ug/ml
12) N-OCTACOSANE	16.811	1477308	9.630 ug/ml
13) N-TRIACONTANE	17.694	1434935	9.891 ug/ml
14) N-DOTRIACONTANE	18.524	610161	4.394 ug/ml
15) N-TETRATRIACONTANE	19.310	90282	0.688 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122619\
Data File : FF006078.D
Signal(s) : FID2B.ch
Acq On : 26 Dec 2019 15:43
Operator : DD\AJ
Sample : K6413-07 2X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
K005-AA-WC-2

Integration File: autoint1.e
Quant Time: Dec 27 01:12:47 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

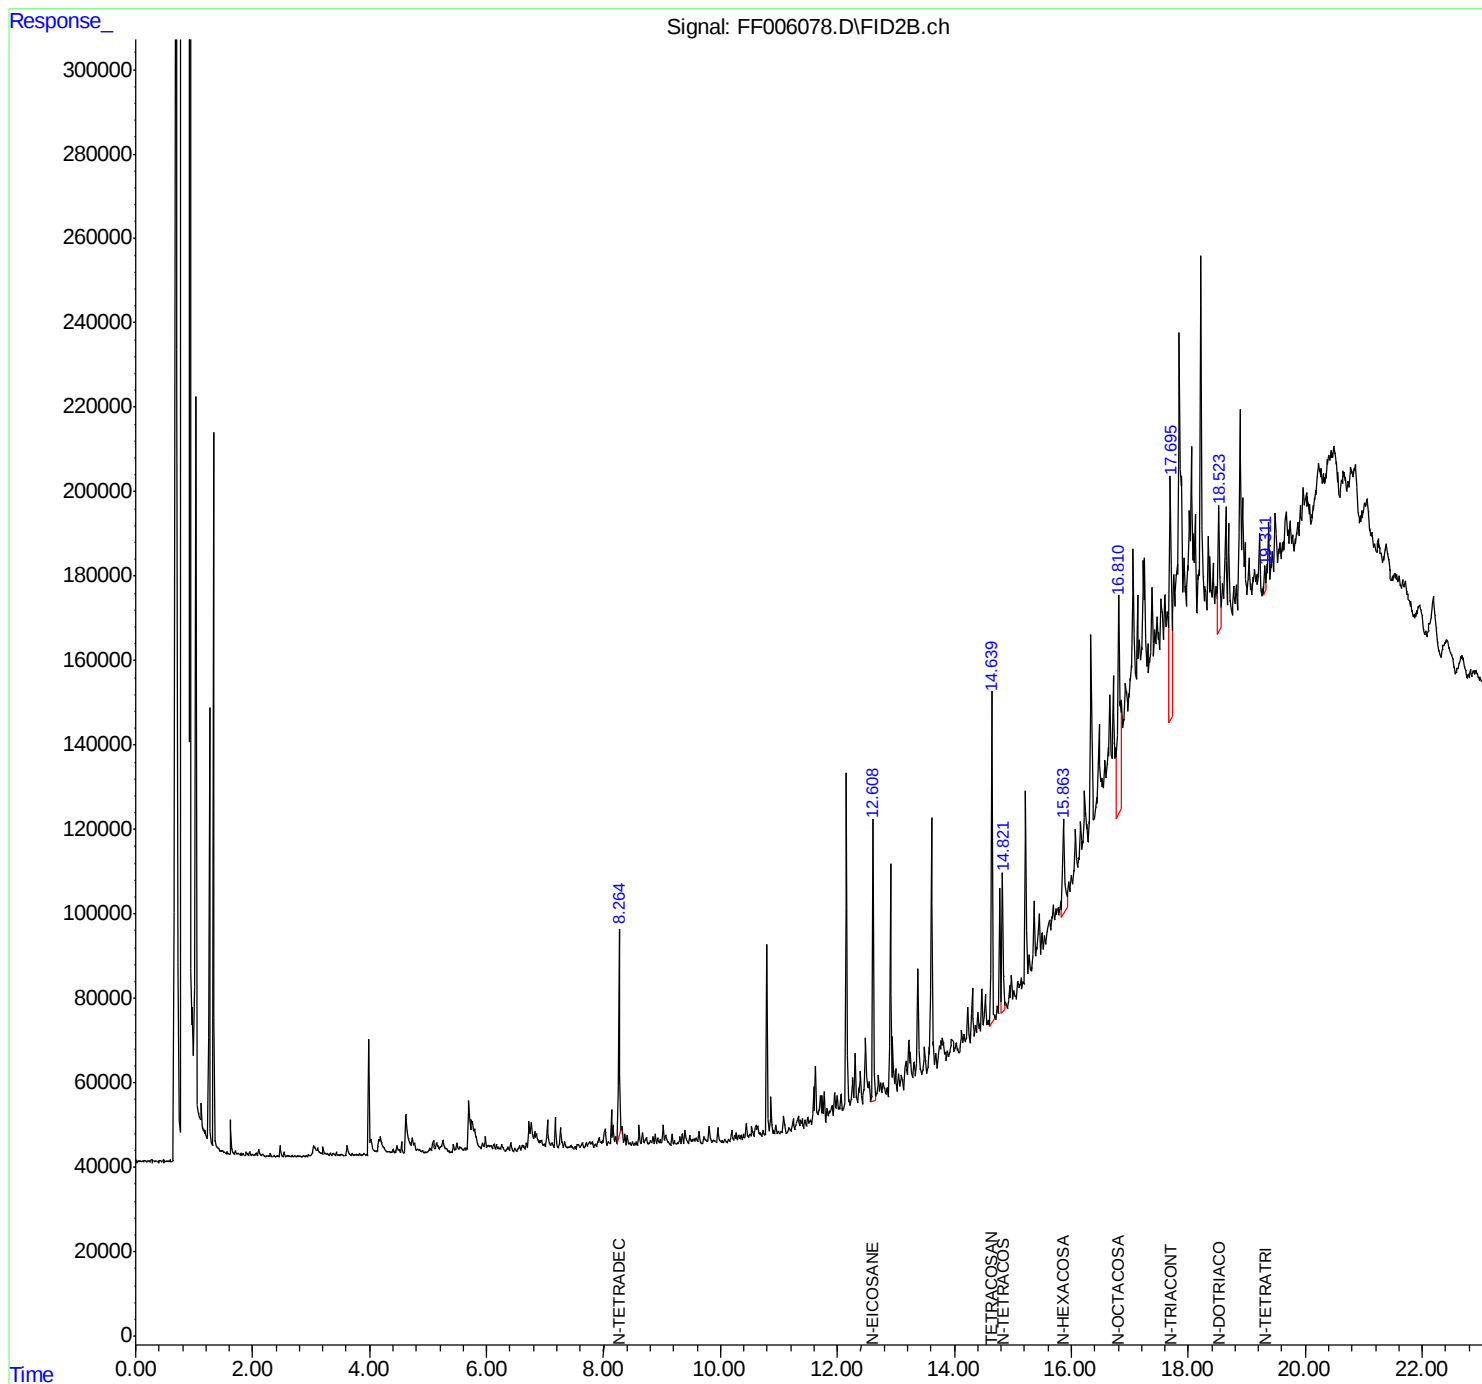


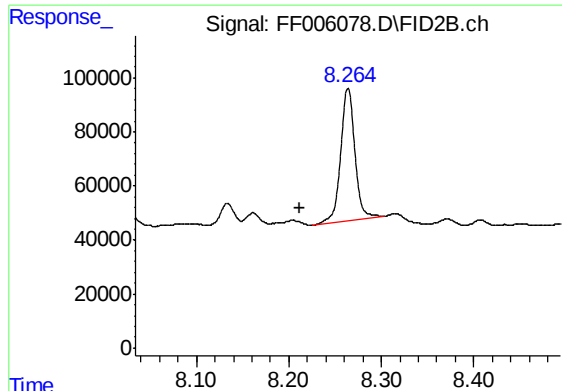

#4 N-TETRADECANE


R.T.: 8.264 min
Delta R.T.: 0.051 min
Response: 523339
Conc: 3.09 ug/ml

Instrument :
FID_F
ClientSampleId :
K005-AA-WC-2

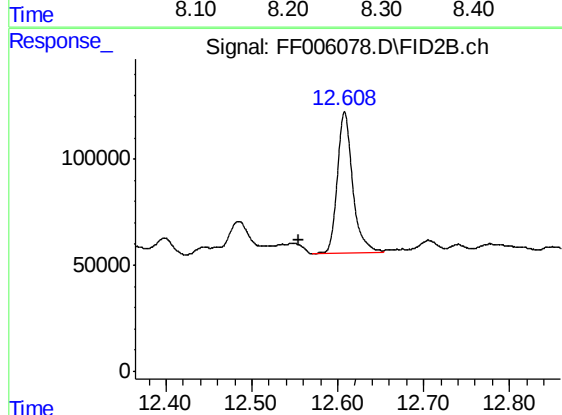


#7 N-EICOSANE

R.T.: 12.608 min
Delta R.T.: 0.053 min
Response: 834287
Conc: 4.83 ug/ml

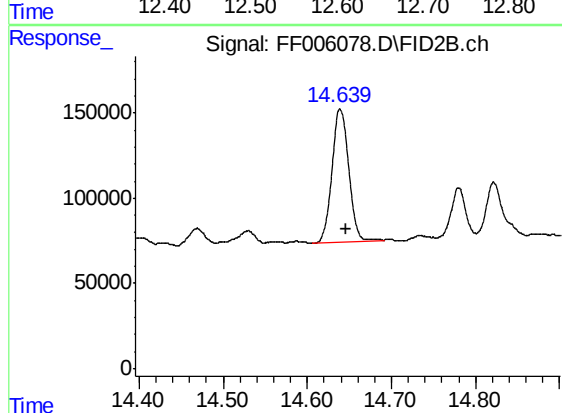


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.639 min
Delta R.T.: -0.008 min
Response: 1082072
Conc: 7.45 ug/ml

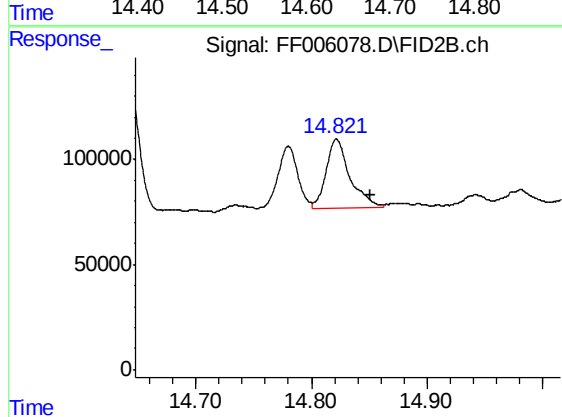

#10 N-TETRACOSANE


R.T.: 14.822 min
Delta R.T.: -0.029 min
Response: 469115
Conc: 2.81 ug/ml

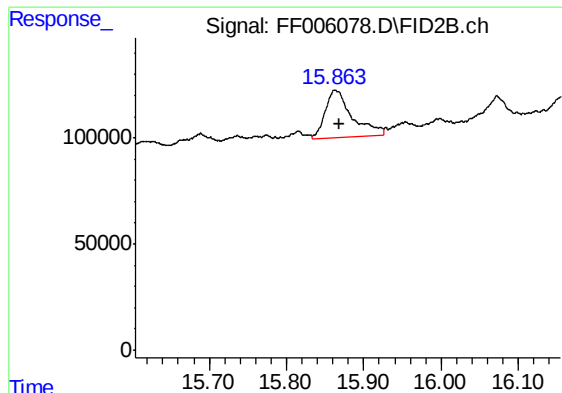

#11 N-HEXACOSANE


R.T.: 15.863 min
Delta R.T.: -0.006 min
Response: 543072
Conc: 3.37 ug/ml

Instrument :
FID_F
ClientSampleId :
K005-AA-WC-2

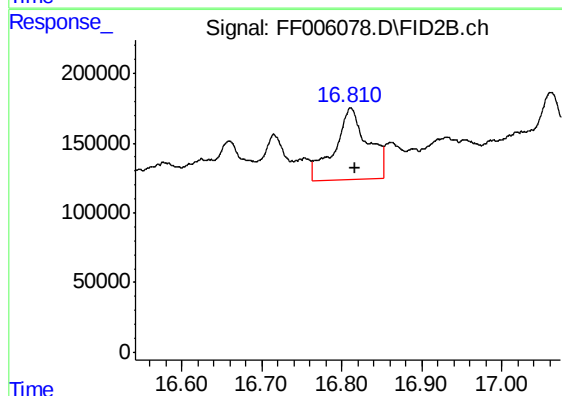


#12 N-OCTACOSANE

R.T.: 16.811 min
Delta R.T.: -0.005 min
Response: 1477308
Conc: 9.63 ug/ml

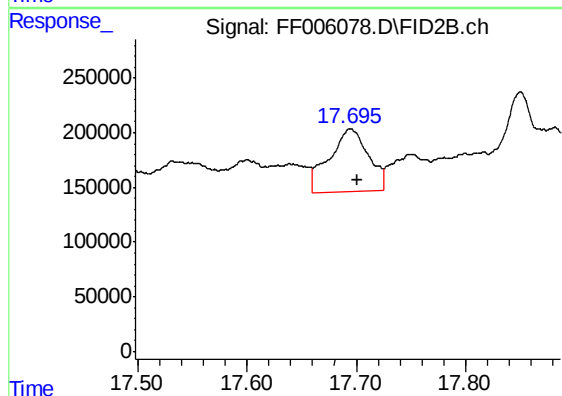


#13 N-TRIACONTANE

R.T.: 17.694 min
Delta R.T.: -0.006 min
Response: 1434935
Conc: 9.89 ug/ml

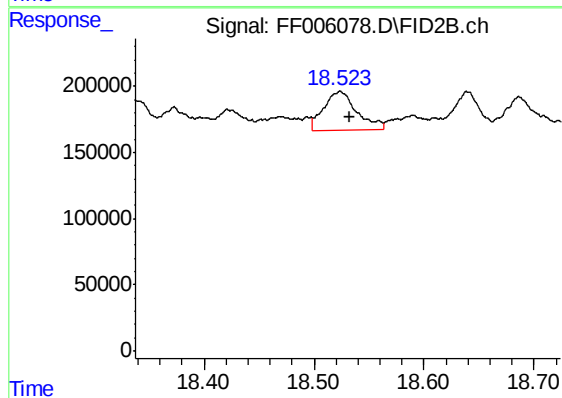

#14 N-DOTRIACONTANE

R.T.: 18.524 min
Delta R.T.: -0.009 min
Response: 610161
Conc: 4.39 ug/ml

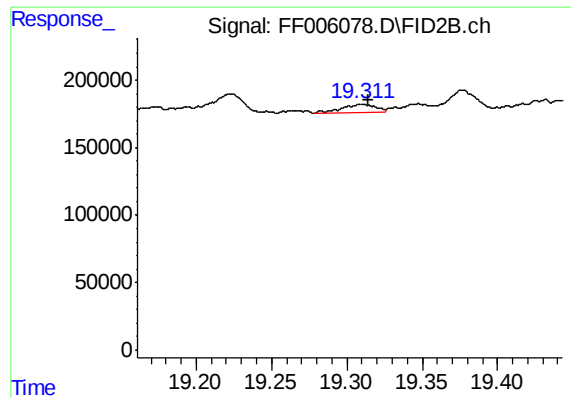

#15 N-TETRATRIACONTANE

R.T.: 19.310 min
Delta R.T.: -0.004 min
Response: 90282
Conc: 0.69 ug/ml

Instrument :
FID_F
ClientSampleId :
K005-AA-WC-2