

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122619\
 Data File : FF006081.D
 Signal(s) : FID2B.ch
 Acq On : 26 Dec 2019 17:14
 Operator : DD\AJ
 Sample : K6414-08
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 K183-WC-02

Integration File: autoint1.e
 Quant Time: Dec 27 01:13:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.639	2518356	17.334 ug/ml
Target Compounds			
4) N-TETRADECANE	8.242	68088	0.402 ug/ml
7) N-EICOSANE	12.607f	985621	5.707 ug/ml
8) N-DOCOSANE	13.741	91821	0.539 ug/ml
10) N-TETRACOSANE	14.838	212773	1.275 ug/ml
11) N-HEXACOSANE	15.859	467009	2.900 ug/ml
12) N-OCTACOSANE	16.806	578210	3.769 ug/ml
13) N-TRIACONTANE	17.689	475462	3.277 ug/ml
14) N-DOTRIACONTANE	18.515	394591	2.842 ug/ml
15) N-TETRATRIACONTANE	19.302	94946	0.724 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122619\
Data File : FF006081.D
Signal(s) : FID2B.ch
Acq On : 26 Dec 2019 17:14
Operator : DD\AJ
Sample : K6414-08
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
K183-WC-02

Integration File: autoint1.e
Quant Time: Dec 27 01:13:27 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

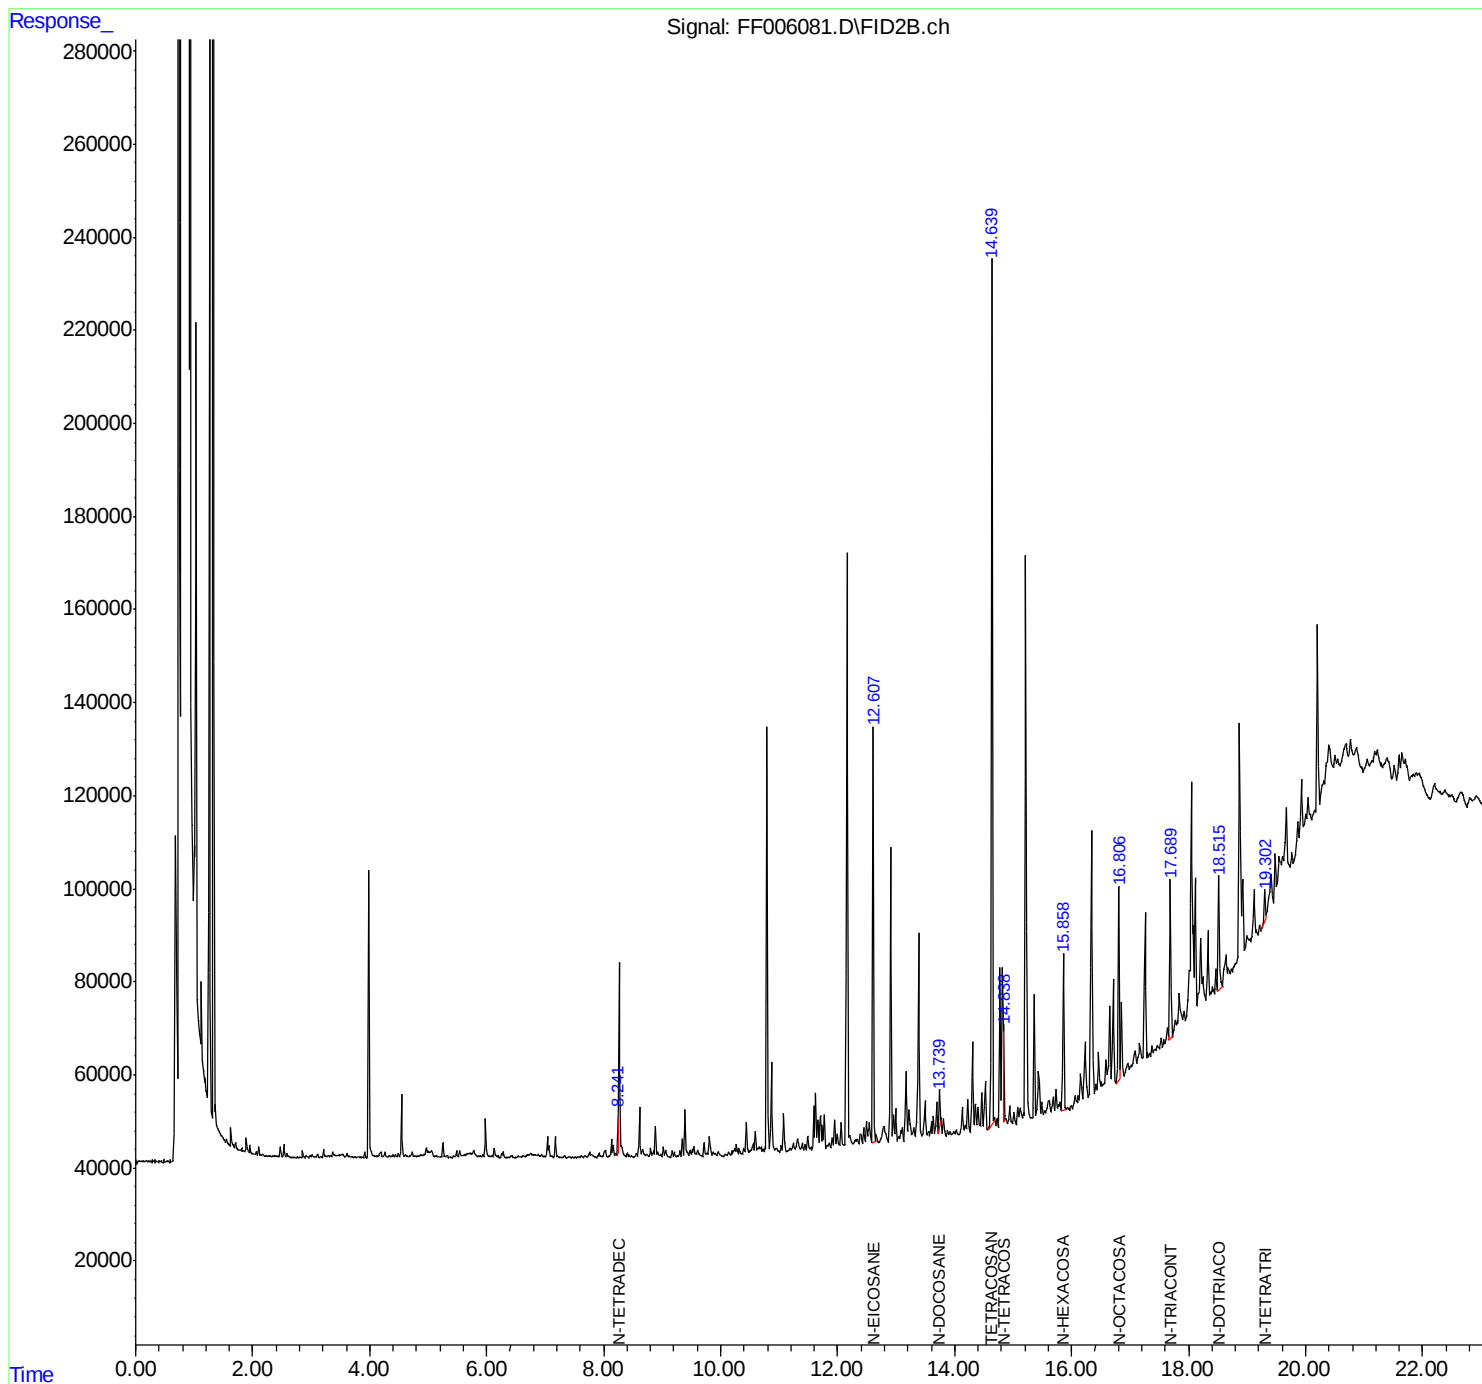


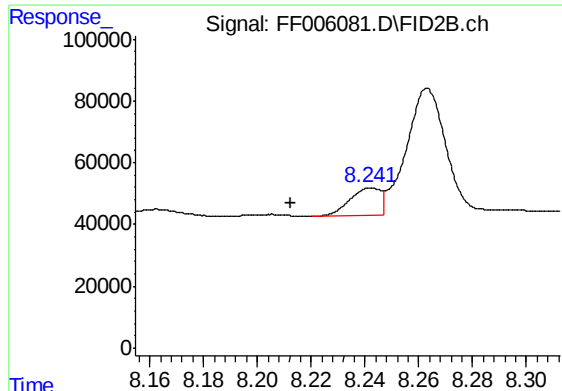

#4 N-TETRADECANE


R.T.: 8.242 min
Delta R.T.: 0.030 min
Response: 68088
Conc: 0.40 ug/ml

Instrument :
FID_F
ClientSampleId :
K183-WC-02

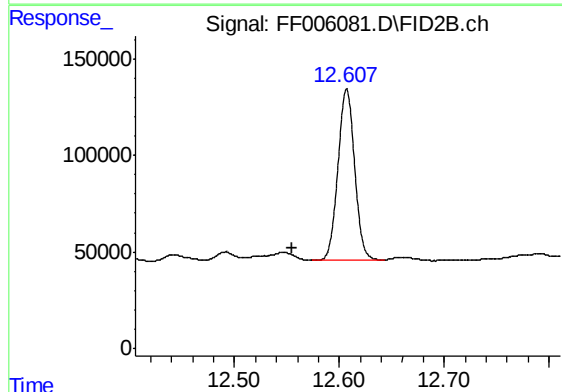


#7 N-EICOSANE

R.T.: 12.607 min
Delta R.T.: 0.052 min
Response: 985621
Conc: 5.71 ug/ml

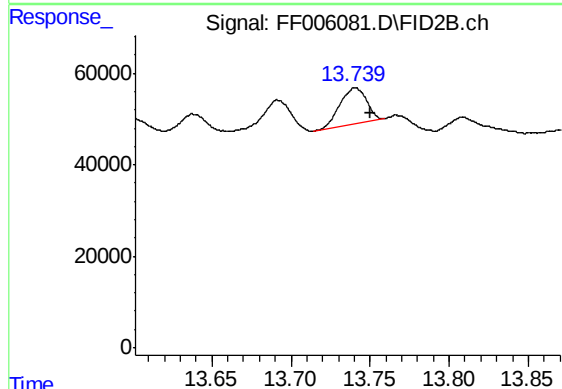


#8 N-DOCOSANE

R.T.: 13.741 min
Delta R.T.: -0.009 min
Response: 91821
Conc: 0.54 ug/ml

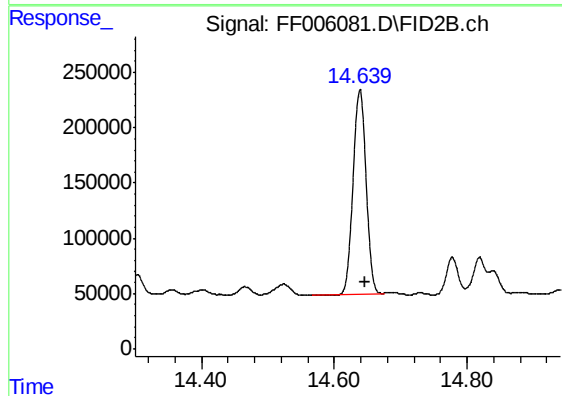

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.639 min
Delta R.T.: -0.008 min
Response: 2518356
Conc: 17.33 ug/ml

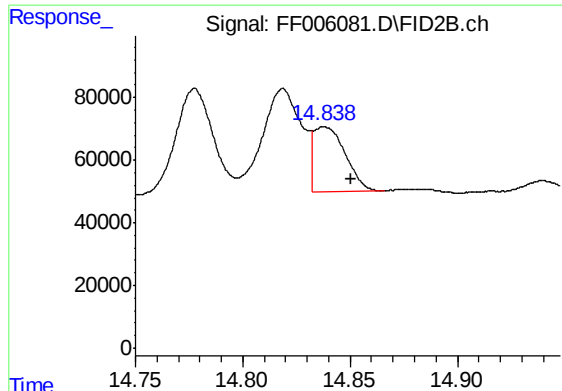

#10 N-TETRACOSANE


R.T.: 14.838 min
Delta R.T.: -0.012 min
Response: 212773
Conc: 1.27 ug/ml

Instrument :
FID_F
ClientSampleId :
K183-WC-02

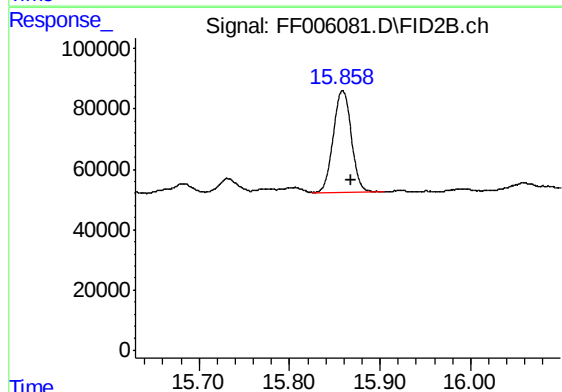


#11 N-HEXACOSANE

R.T.: 15.859 min
Delta R.T.: -0.010 min
Response: 467009
Conc: 2.90 ug/ml

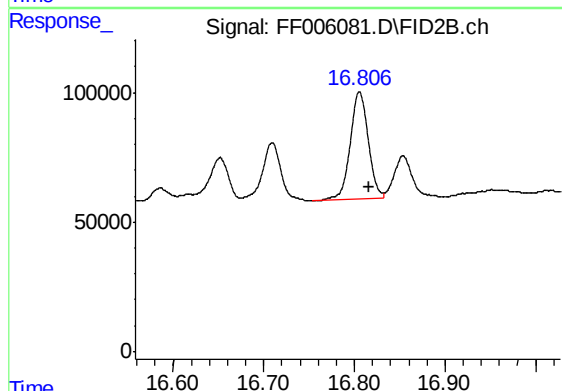


#12 N-OCTACOSANE

R.T.: 16.806 min
Delta R.T.: -0.010 min
Response: 578210
Conc: 3.77 ug/ml

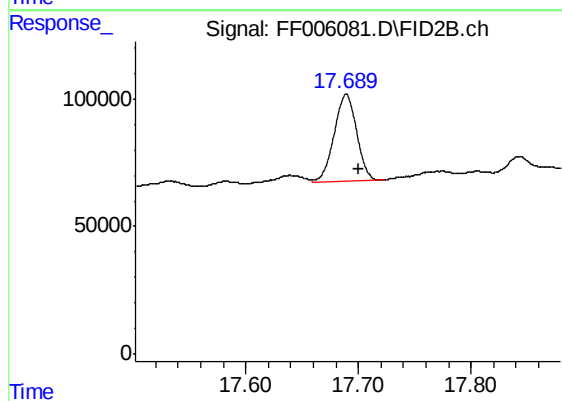

#13 N-TRIACONTANE


R.T.: 17.689 min
Delta R.T.: -0.011 min
Response: 475462
Conc: 3.28 ug/ml

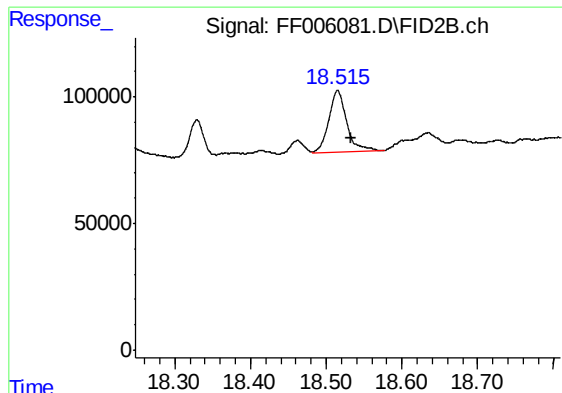

#14 N-DOTRIACONTANE

R.T.: 18.515 min
Delta R.T.: -0.017 min
Response: 394591
Conc: 2.84 ug/ml

Instrument :
FID_F
ClientSampleId :
K183-WC-02

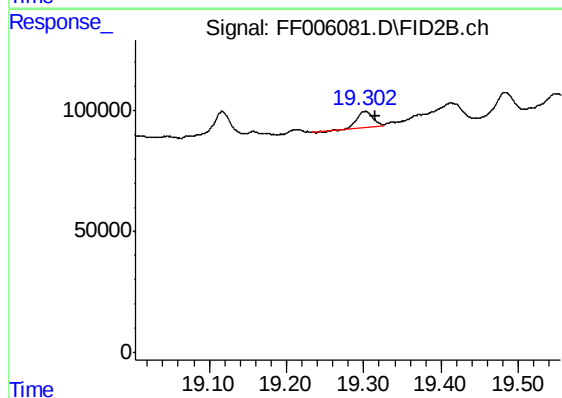

#15 N-TETRATRIACONTANE

R.T.: 19.302 min
Delta R.T.: -0.013 min
Response: 94946
Conc: 0.72 ug/ml