

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122718\
 Data File : FF003079.D
 Signal(s) : FID2B.ch
 Acq On : 27 Dec 2018 09:44
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 27 23:51:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.634	6252090	48.158 ug/ml
Target Compounds			
2) N-DECANE	4.362	8737232	55.769 ug/ml
3) N-DODECANE	6.384	8543179	53.799 ug/ml
4) N-TETRADECANE	8.177	8259809	51.531 ug/ml
5) N-HEXADECANE	9.777	8016590	50.058 ug/ml
6) N-OCTADECANE	11.220	7758444	48.975 ug/ml
7) N-EICOSANE	12.532	7421731	48.121 ug/ml
8) N-DOCOSANE	13.732	7151657	47.828 ug/ml
10) N-TETRACOSANE	14.838	7009233	48.502 ug/ml
11) N-HEXACOSANE	15.861	6840580	49.009 ug/ml
12) N-OCTACOSANE	16.812	6836039	51.020 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122718\
Data File : FF003079.D
Signal(s) : FID2B.ch
Acq On : 27 Dec 2018 09:44
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 27 23:51:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

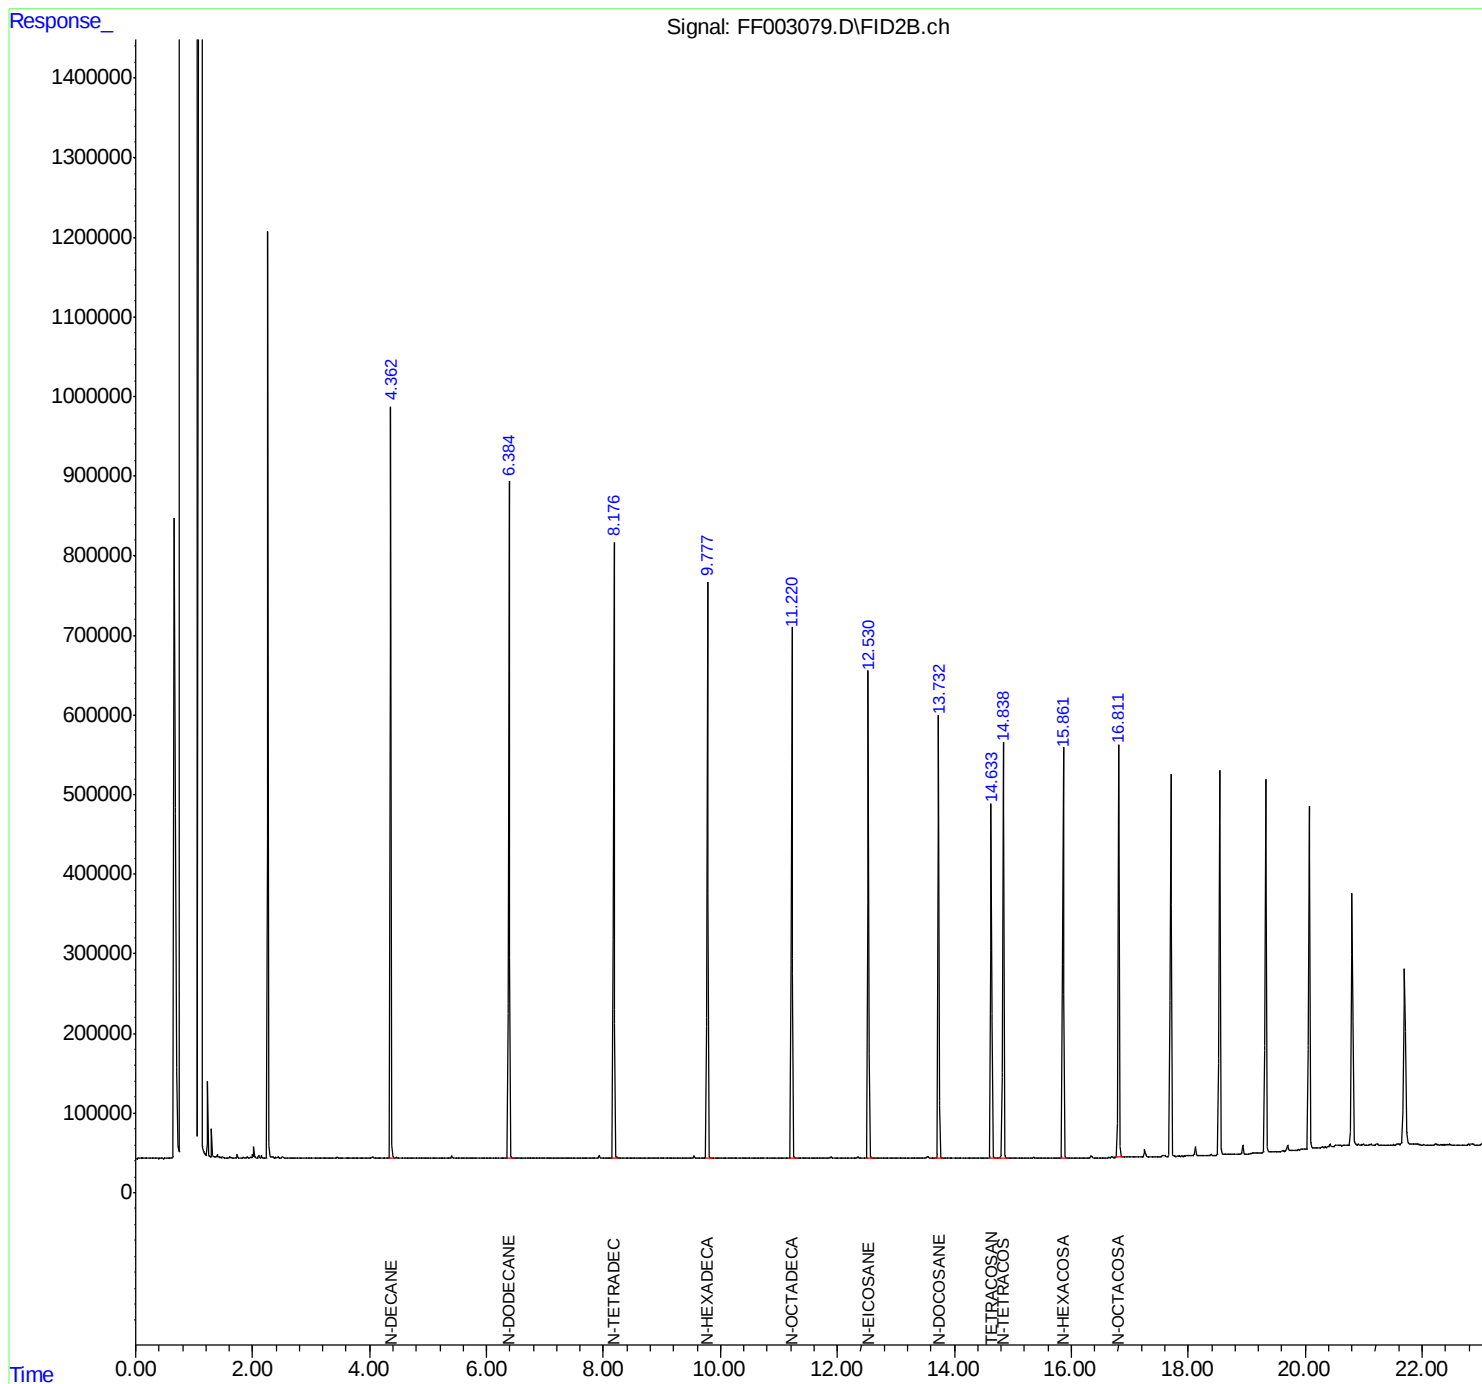

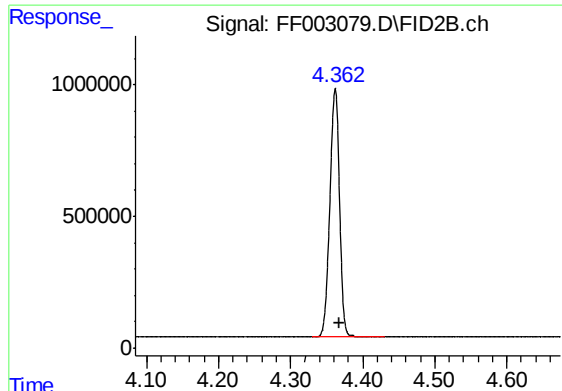


#2 N-DECANE

R.T.: 4.362 min
Delta R.T.: -0.006 min
Response: 8737232
Conc: 55.77 ug/ml

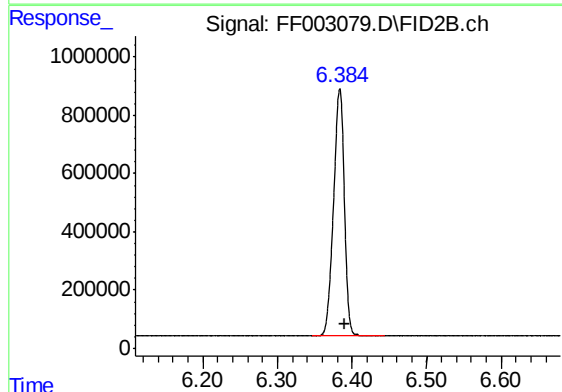


#3 N-DODECANE

R.T.: 6.384 min
Delta R.T.: -0.007 min
Response: 8543179
Conc: 53.80 ug/ml

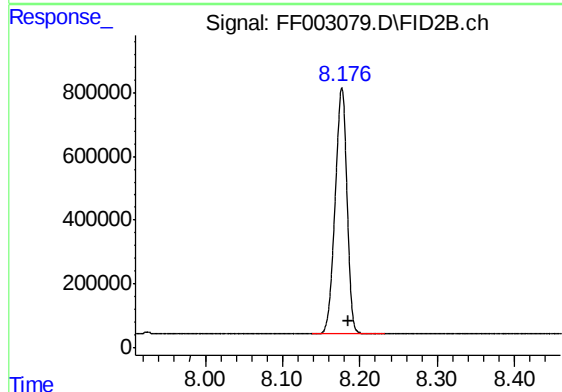


#4 N-TETRADECANE

R.T.: 8.177 min
Delta R.T.: -0.009 min
Response: 8259809
Conc: 51.53 ug/ml

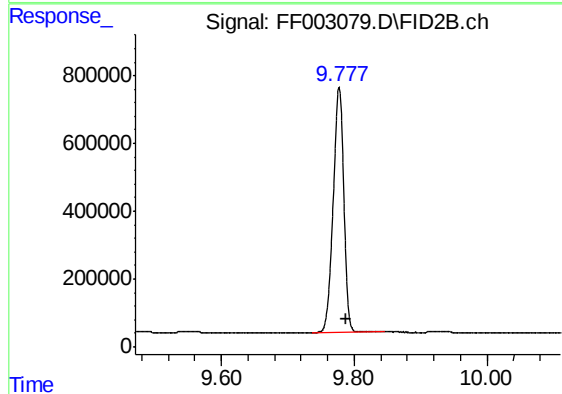


#5 N-HEXADECANE

R.T.: 9.777 min
Delta R.T.: -0.010 min
Response: 8016590
Conc: 50.06 ug/ml

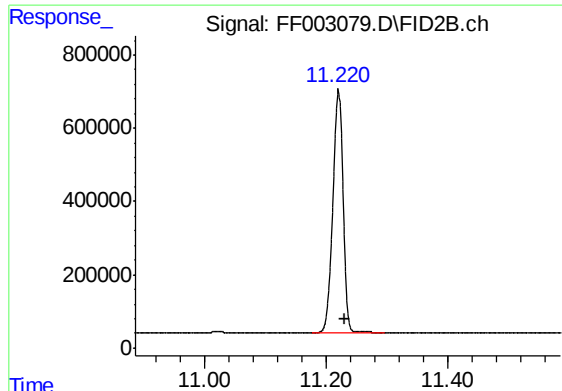


#6 N-OCTADECANE

R.T.: 11.220 min
Delta R.T.: -0.011 min
Response: 7758444
Conc: 48.97 ug/ml

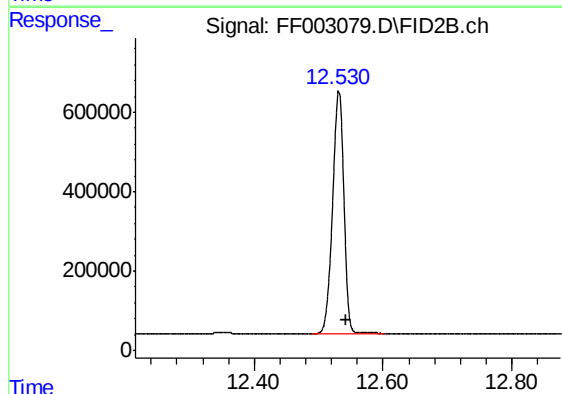


#7 N-EICOSANE

R.T.: 12.532 min
Delta R.T.: -0.012 min
Response: 7421731
Conc: 48.12 ug/ml

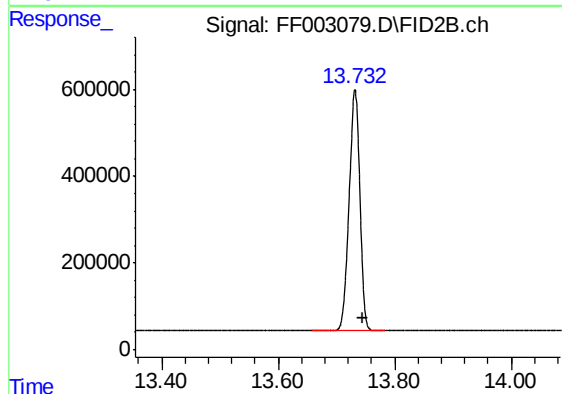


#8 N-DOCOSANE

R.T.: 13.732 min
Delta R.T.: -0.012 min
Response: 7151657
Conc: 47.83 ug/ml

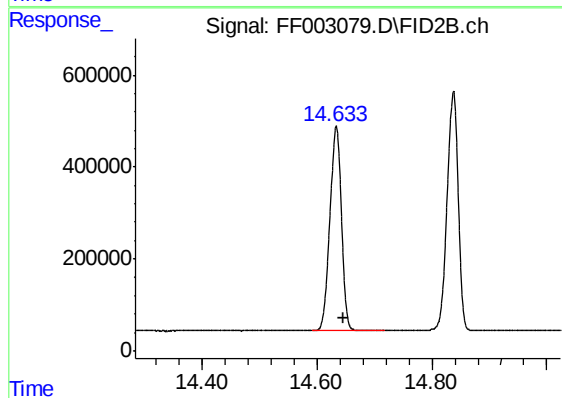


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.634 min
Delta R.T.: -0.012 min
Response: 6252090
Conc: 48.16 ug/ml

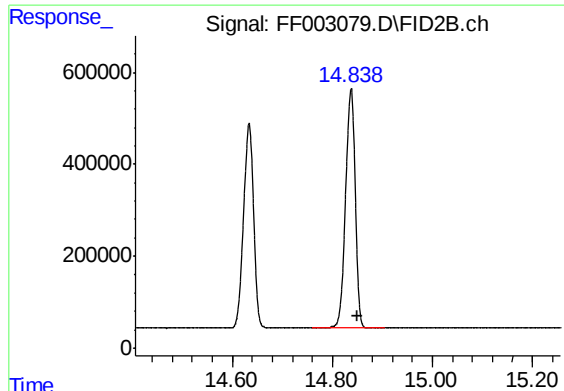


#10 N-TETRACOSANE

R.T.: 14.838 min
Delta R.T.: -0.012 min
Response: 7009233
Conc: 48.50 ug/ml

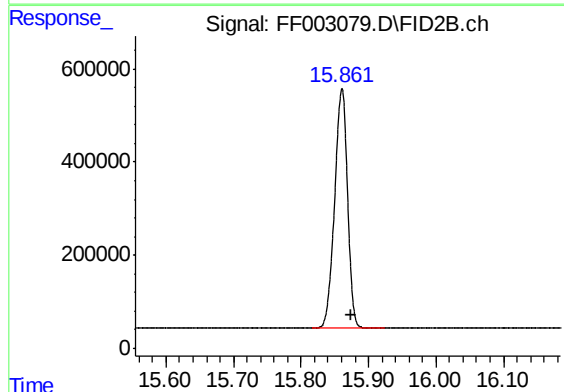

#11 N-HEXACOSANE

R.T.: 15.861 min
Delta R.T.: -0.013 min
Response: 6840580
Conc: 49.01 ug/ml

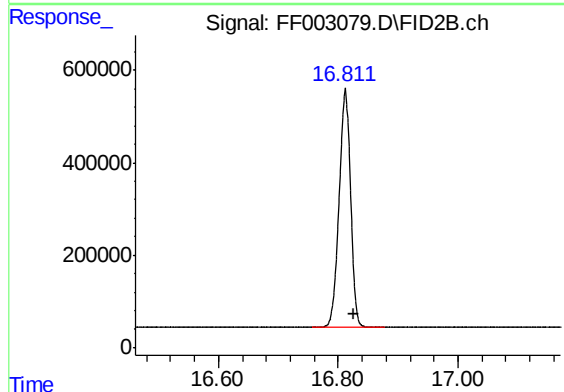

#12 N-OCTACOSANE

R.T.: 16.812 min
Delta R.T.: -0.013 min
Response: 6836039
Conc: 51.02 ug/ml