

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122718\
 Data File : FF003090.D
 Signal(s) : FID2B.ch
 Acq On : 27 Dec 2018 15:11
 Operator : AJ\SJ
 Sample : PB116009BS
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 27 23:54:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	2039167	15.707 ug/ml
Target Compounds			
2) N-DECANE	4.360	2847614	18.176 ug/ml
3) N-DODECANE	6.381	2766379	17.421 ug/ml
4) N-TETRADECANE	8.173	2660960	16.601 ug/ml
5) N-HEXADECANE	9.774	2578904	16.103 ug/ml
6) N-OCTADECANE	11.216	2500672	15.785 ug/ml
7) N-EICOSANE	12.528	2398893	15.554 ug/ml
8) N-DOCOSANE	13.728	2318395	15.505 ug/ml
10) N-TETRACOSANE	14.833	2329671	16.121 ug/ml
11) N-HEXACOSANE	15.857	2235495	16.016 ug/ml
12) N-OCTACOSANE	16.809	2251735	16.806 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122718\
Data File : FF003090.D
Signal(s) : FID2B.ch
Acq On : 27 Dec 2018 15:11
Operator : AJ\SJ
Sample : PB116009BS
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 27 23:54:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

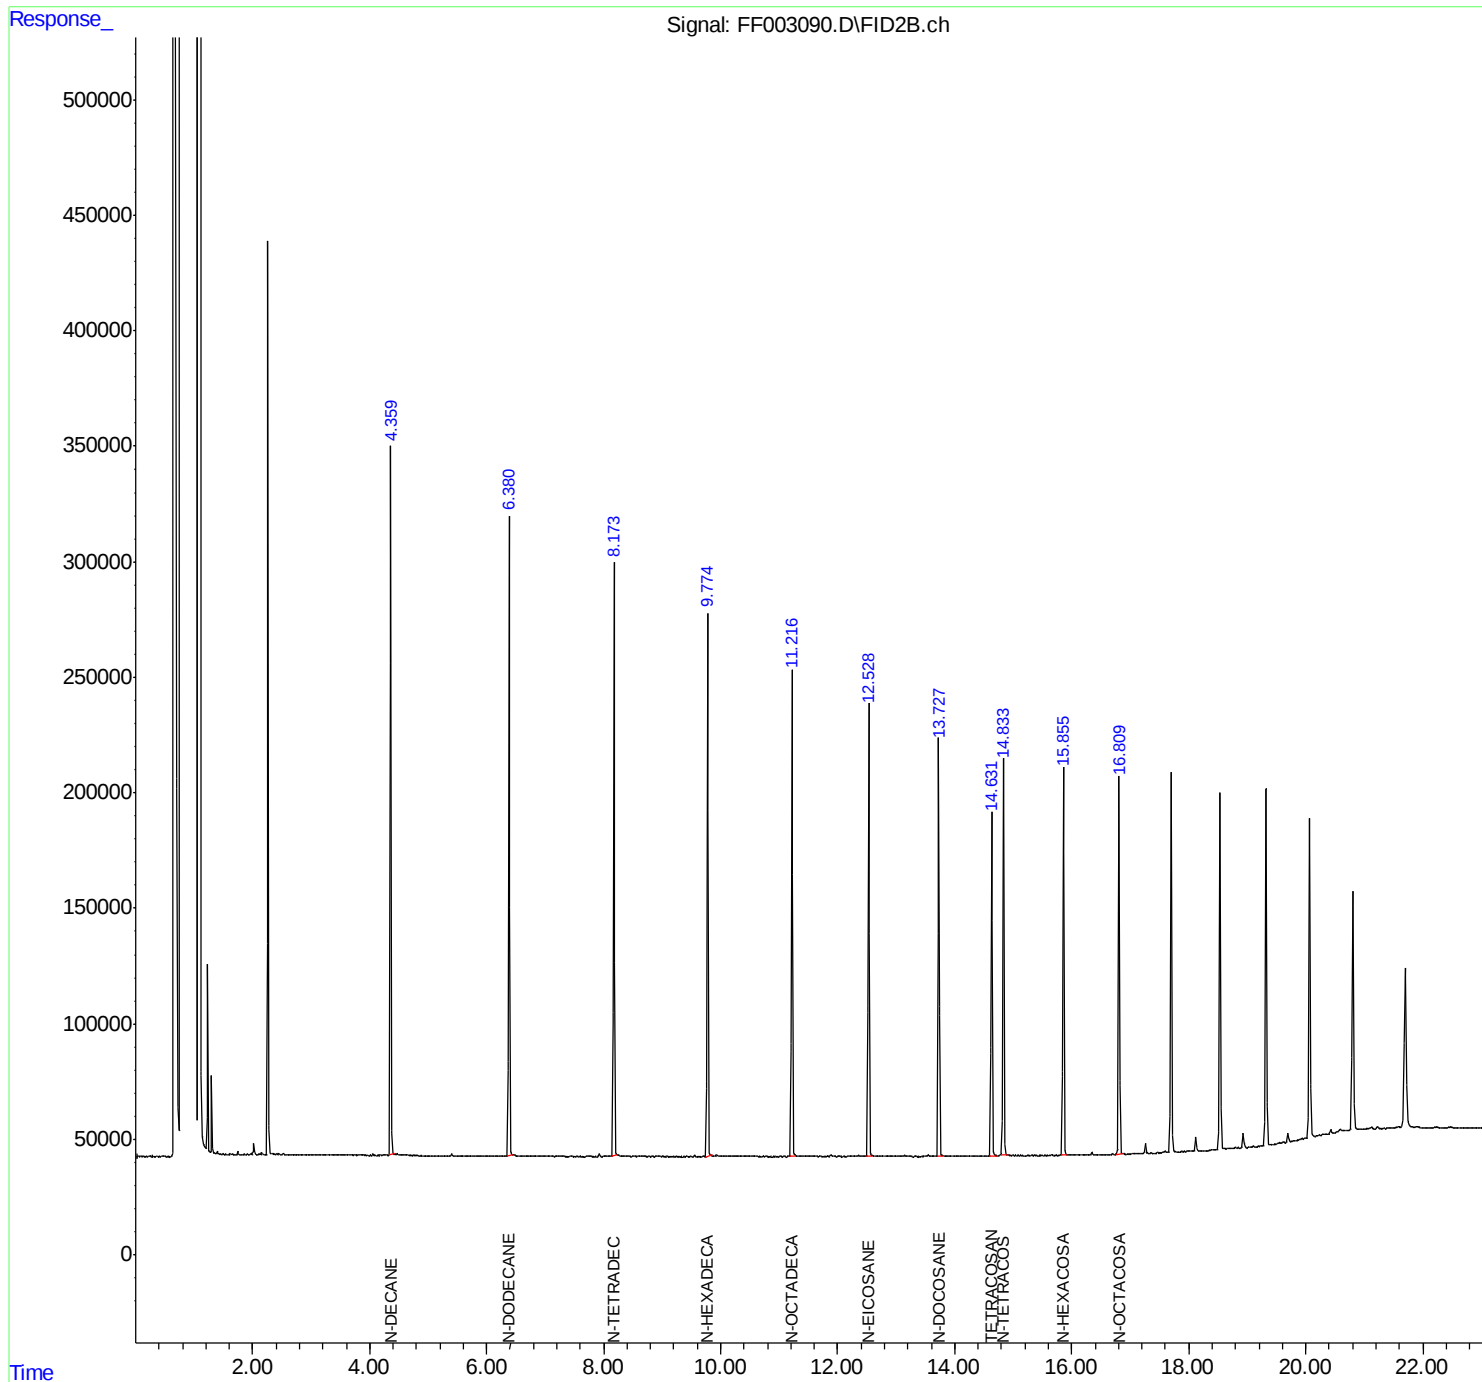

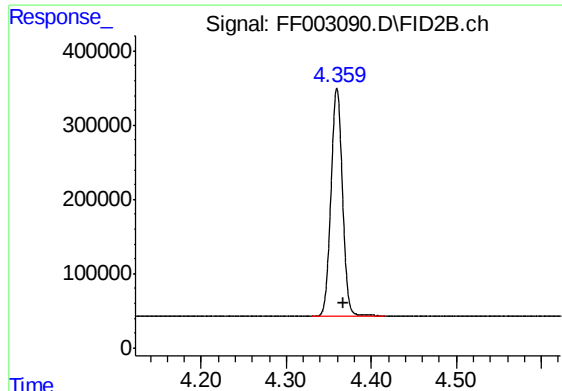


#2 N-DECANE

R.T.: 4.360 min
Delta R.T.: -0.008 min
Response: 2847614
Conc: 18.18 ug/ml

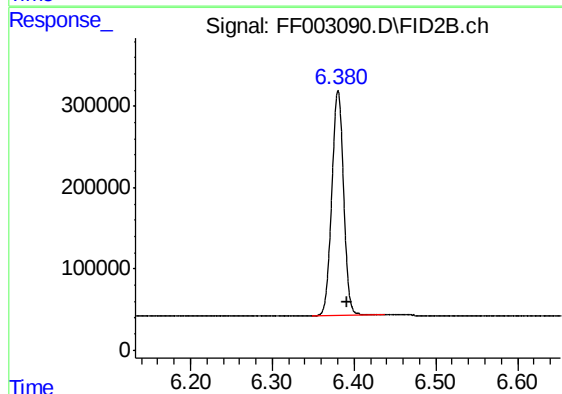


#3 N-DODECANE

R.T.: 6.381 min
Delta R.T.: -0.010 min
Response: 2766379
Conc: 17.42 ug/ml

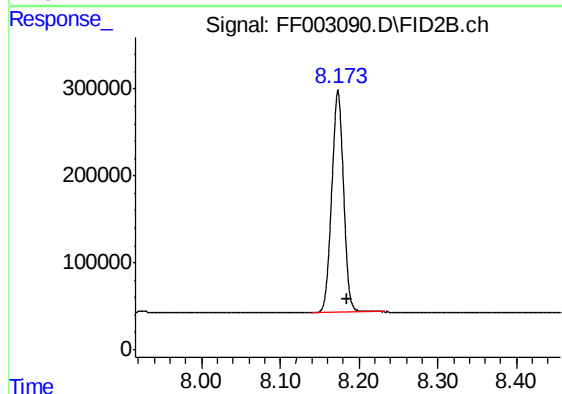


#4 N-TETRADECANE

R.T.: 8.173 min
Delta R.T.: -0.012 min
Response: 2660960
Conc: 16.60 ug/ml

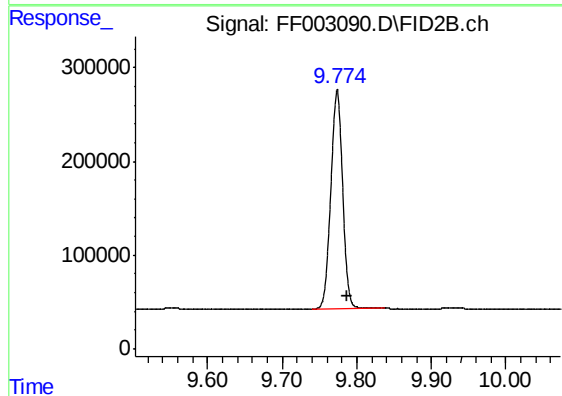


#5 N-HEXADECANE

R.T.: 9.774 min
Delta R.T.: -0.014 min
Response: 2578904
Conc: 16.10 ug/ml

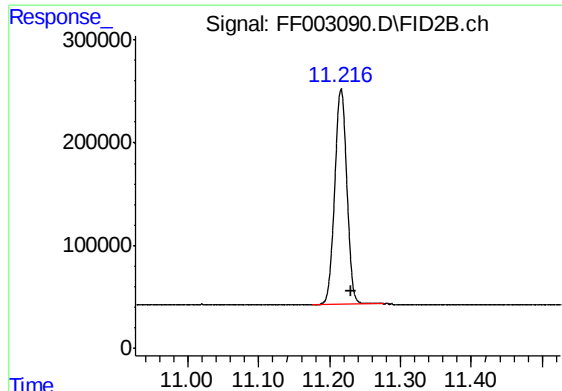


#6 N-OCTADECANE

R.T.: 11.216 min
Delta R.T.: -0.015 min
Response: 2500672
Conc: 15.79 ug/ml

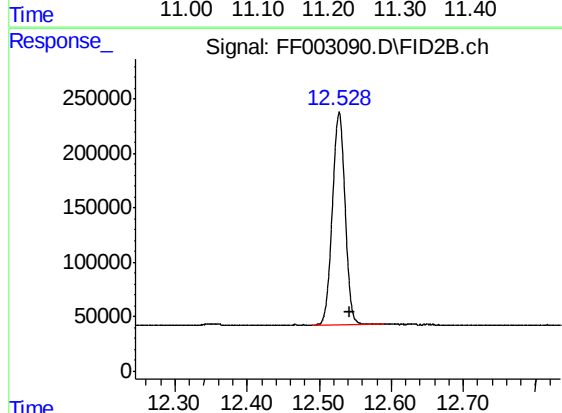


#7 N-EICOSANE

R.T.: 12.528 min
Delta R.T.: -0.016 min
Response: 2398893
Conc: 15.55 ug/ml

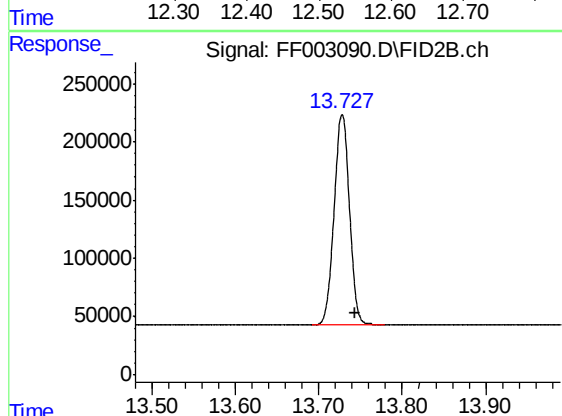


#8 N-DOCOSANE

R.T.: 13.728 min
Delta R.T.: -0.016 min
Response: 2318395
Conc: 15.50 ug/ml

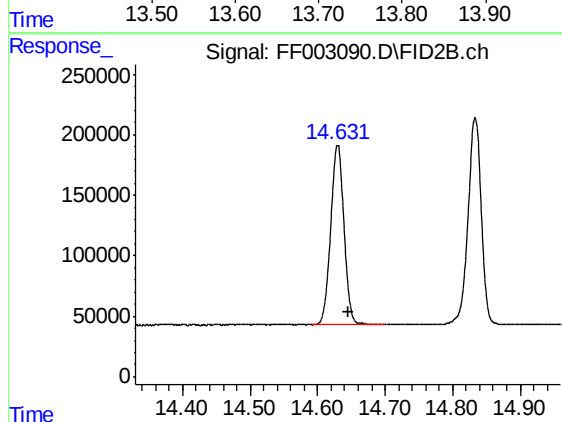


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.630 min
Delta R.T.: -0.016 min
Response: 2039167
Conc: 15.71 ug/ml

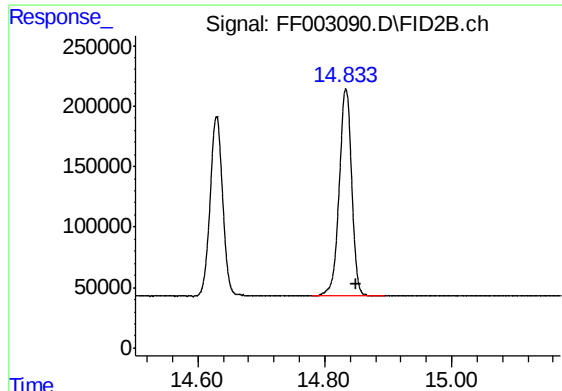


#10 N-TETRACOSANE

R.T.: 14.833 min
Delta R.T.: -0.016 min
Response: 2329671
Conc: 16.12 ug/ml

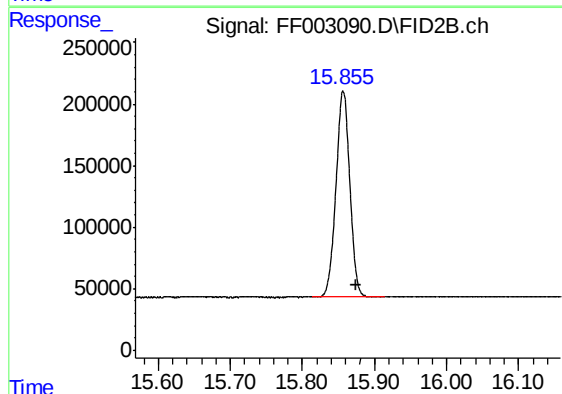

#11 N-HEXACOSANE

R.T.: 15.857 min
Delta R.T.: -0.018 min
Response: 2235495
Conc: 16.02 ug/ml

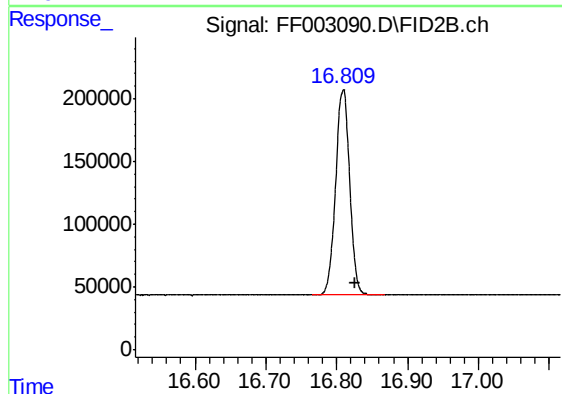

#12 N-OCTACOSANE

R.T.: 16.809 min
Delta R.T.: -0.016 min
Response: 2251735
Conc: 16.81 ug/ml