

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122718\
 Data File : FF003092.D
 Signal(s) : FID2B.ch
 Acq On : 27 Dec 2018 16:11
 Operator : AJ\SJ
 Sample : J6195-11MS 5X
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 27 23:55:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.629	677784	5.221 ug/mlm
Target Compounds			
2) N-DECANE	4.359	623243	3.978 ug/ml
3) N-DODECANE	6.380	1273187	8.018 ug/ml
4) N-TETRADECANE	8.172	1524020	9.508 ug/mlm
5) N-HEXADECANE	9.773	1744726	10.895 ug/mlm
6) N-OCTADECANE	11.215	1379419	8.708 ug/mlm
7) N-EICOSANE	12.527	1304978	8.461 ug/mlm
8) N-DOCOSANE	13.729	1097917	7.342 ug/mlm
10) N-TETRACOSANE	14.831	809575	5.602 ug/mlm
11) N-HEXACOSANE	15.858	1001847	7.178 ug/mlm
12) N-OCTACOSANE	16.809	1382474	10.318 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122718\
Data File : FF003092.D
Signal(s) : FID2B.ch
Acq On : 27 Dec 2018 16:11
Operator : AJ\SJ
Sample : J6195-11MS 5X
Misc :
ALS Vial : 64 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 27 23:55:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

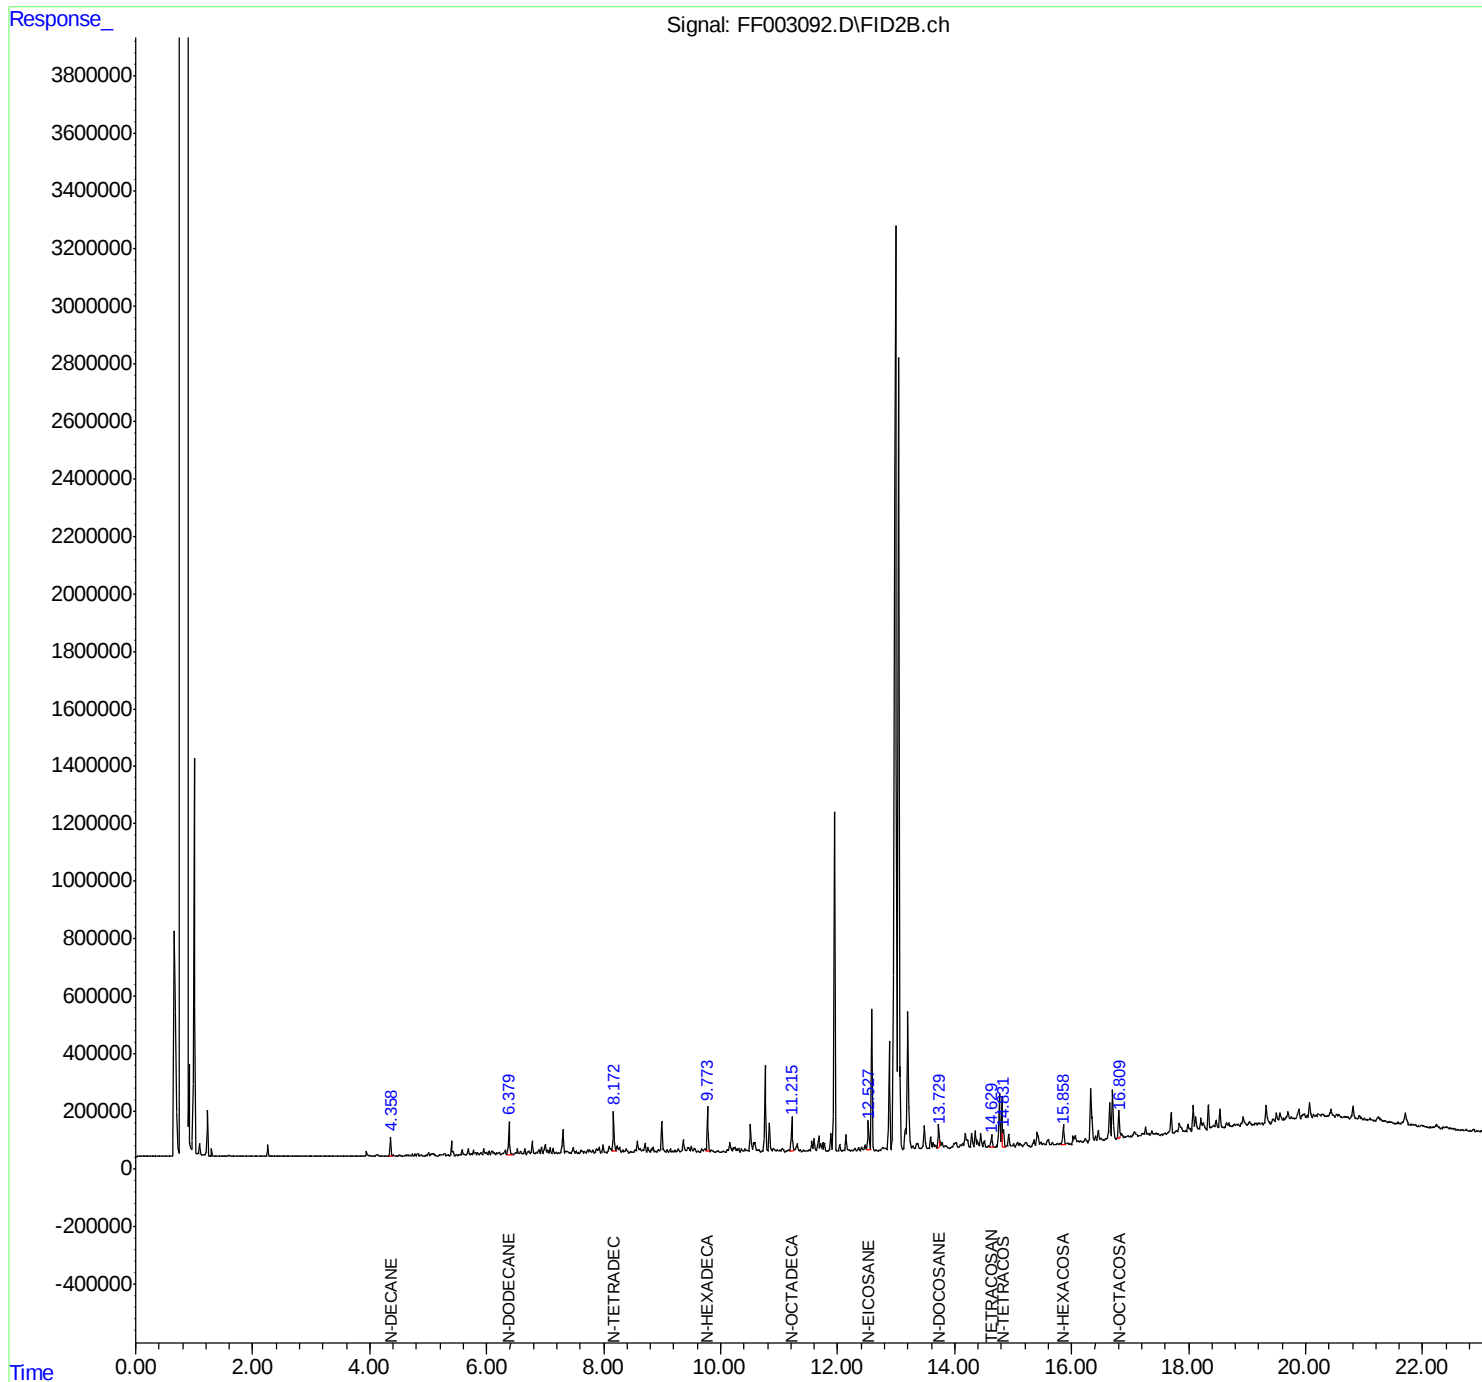

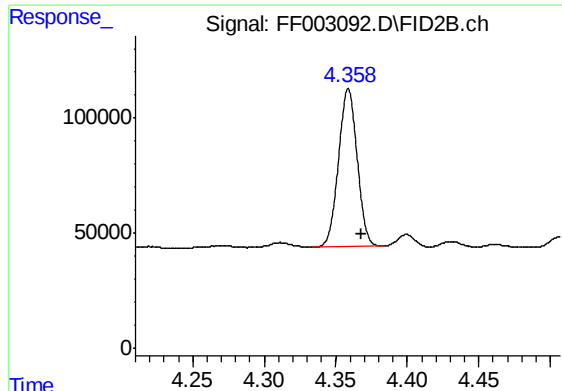


#2 N-DECANE

R.T.: 4.359 min
Delta R.T.: -0.009 min
Response: 623243
Conc: 3.98 ug/ml

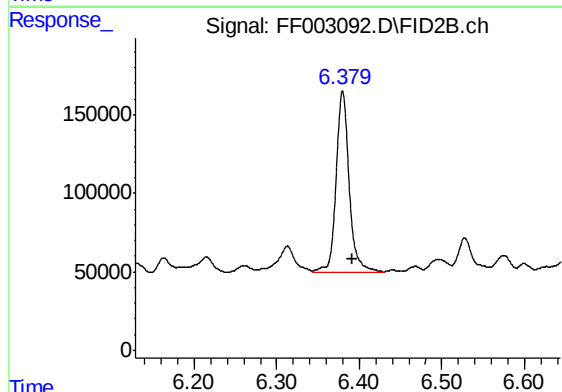


#3 N-DODECANE

R.T.: 6.380 min
Delta R.T.: -0.011 min
Response: 1273187
Conc: 8.02 ug/ml

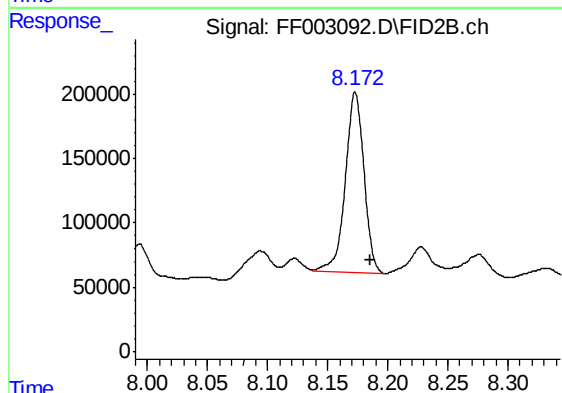


#4 N-TETRADECANE

R.T.: 8.172 min
Delta R.T.: -0.013 min
Response: 1524020
Conc: 9.51 ug/ml m

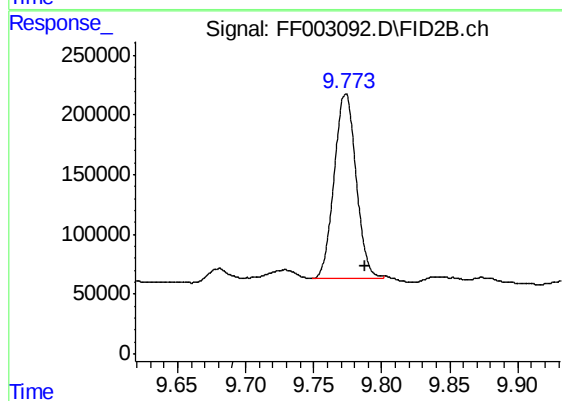


#5 N-HEXADECANE

R.T.: 9.773 min
Delta R.T.: -0.014 min
Response: 1744726
Conc: 10.89 ug/ml m

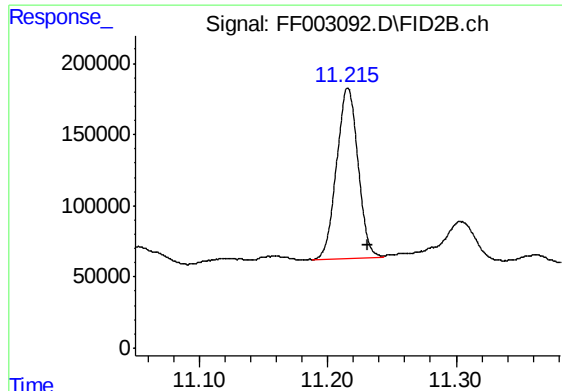


#6 N-OCTADECANE

R.T.: 11.215 min
Delta R.T.: -0.016 min
Response: 1379419
Conc: 8.71 ug/ml m

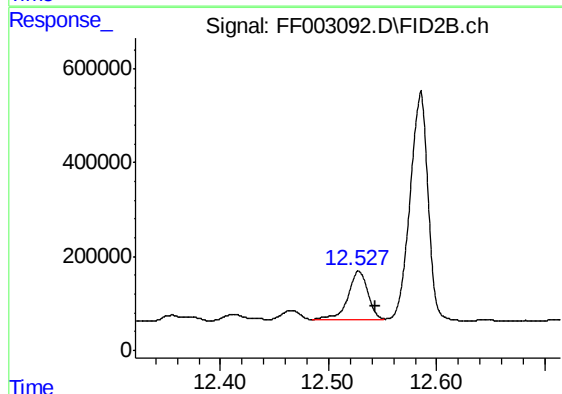


#7 N-EICOSANE

R.T.: 12.527 min
Delta R.T.: -0.017 min
Response: 1304978
Conc: 8.46 ug/ml m

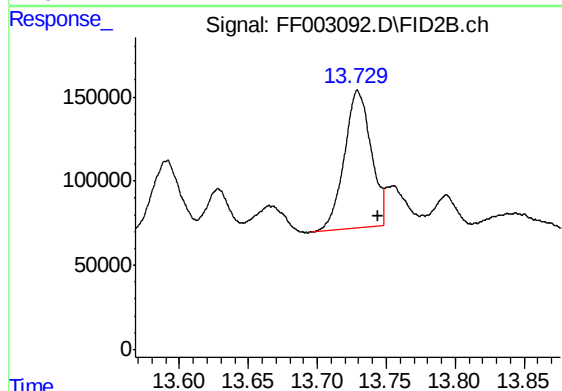


#8 N-DOCOSANE

R.T.: 13.729 min
Delta R.T.: -0.015 min
Response: 1097917
Conc: 7.34 ug/ml m

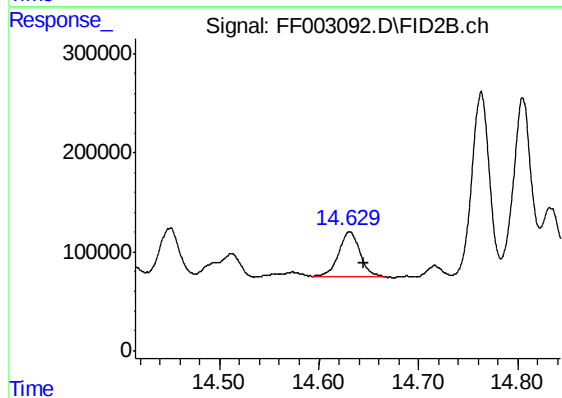


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.629 min
Delta R.T.: -0.016 min
Response: 677784
Conc: 5.22 ug/ml m

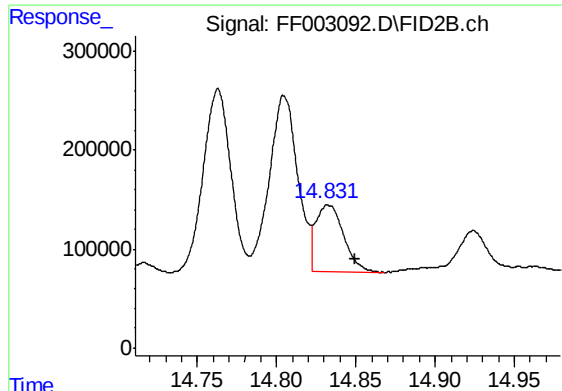


#10 N-TETRACOSANE

R.T.: 14.831 min
Delta R.T.: -0.018 min
Response: 809575
Conc: 5.60 ug/ml m

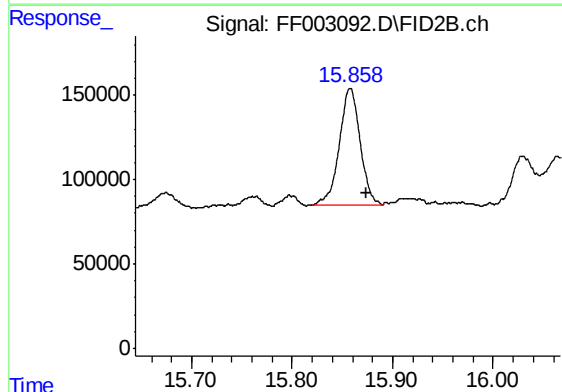

#11 N-HEXACOSANE

R.T.: 15.858 min
Delta R.T.: -0.016 min
Response: 1001847
Conc: 7.18 ug/ml m

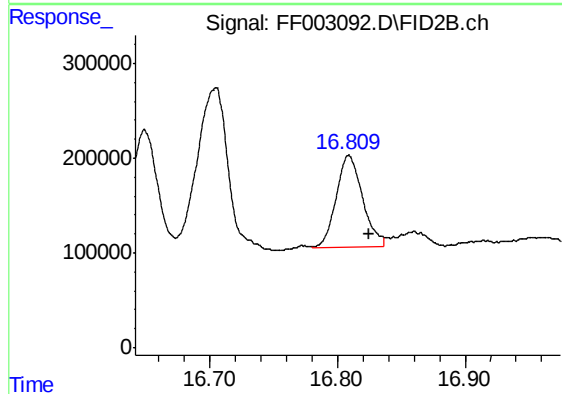

#12 N-OCTACOSANE

R.T.: 16.809 min
Delta R.T.: -0.016 min
Response: 1382474
Conc: 10.32 ug/ml m