

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
 Data File : FF006107.D
 Signal(s) : FID2B.ch
 Acq On : 27 Dec 2019 22:09
 Operator : DD\AJ
 Sample : K6441-06 5X
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 27 23:27:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
 Quant Title :
 QLast Update : Fri Dec 06 13:20:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.635	518724	3.570 ug/ml
Target Compounds			
4) N-TETRADECANE	8.262	74578	0.440 ug/ml
5) N-HEXADECANE	9.811	145087	0.842 ug/ml
7) N-EICOSANE	12.551	157711	0.913 ug/ml
8) N-DOCOSANE	13.767	434820	2.554 ug/ml
10) N-TETRACOSANE	14.819	1693935	10.150 ug/ml
11) N-HEXACOSANE	15.869	167844	1.042 ug/ml
12) N-OCTACOSANE	16.809	538271	3.509 ug/ml
13) N-TRIACONTANE	17.686	422679	2.913 ug/ml
14) N-DOTRIACONTANE	18.514	128065	0.922 ug/ml
15) N-TETRATRIACONTANE	19.292	39063	0.298 ug/ml
17) N-OCTATRIACONTANE	20.788	153708	1.310 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122719\
Data File : FF006107.D
Signal(s) : FID2B.ch
Acq On : 27 Dec 2019 22:09
Operator : DD\AJ
Sample : K6441-06 5X
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 27 23:27:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

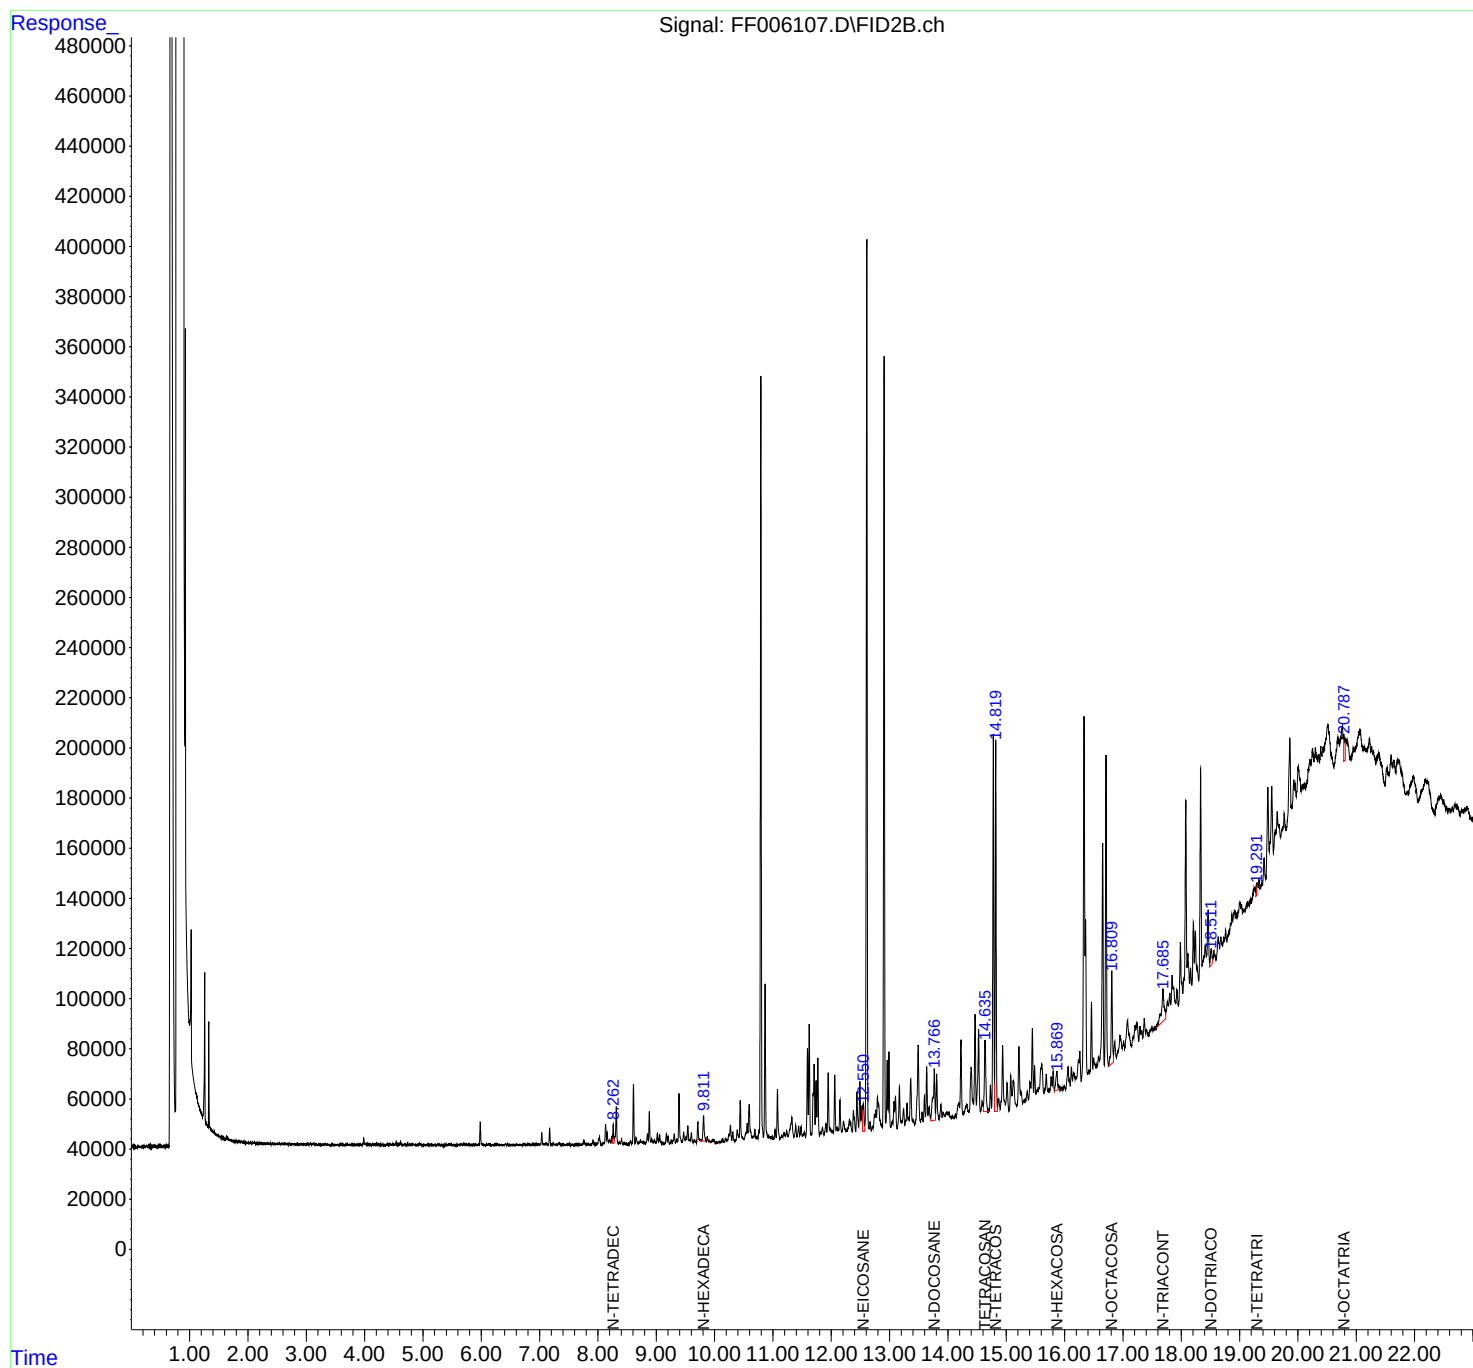


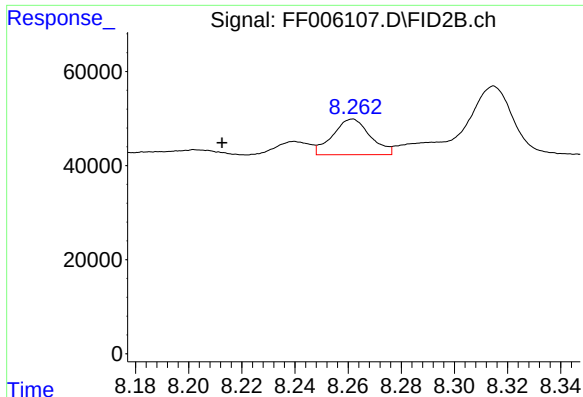

#4 N-TETRADECANE


R.T.: 8.262 min
Delta R.T.: 0.049 min
Response: 74578
Conc: 0.44 ug/ml

Instrument :
FID_F
ClientSampleId :

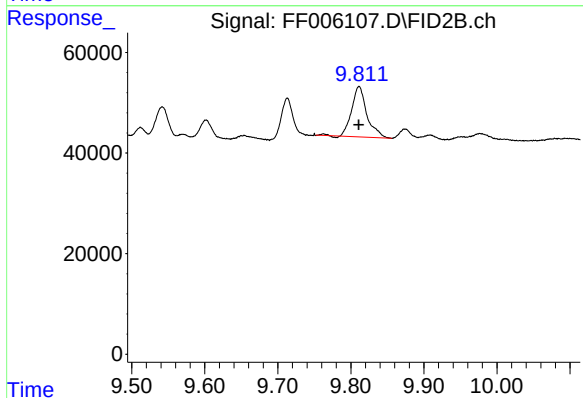


#5 N-HEXADECANE

R.T.: 9.811 min
Delta R.T.: 0.000 min
Response: 145087
Conc: 0.84 ug/ml

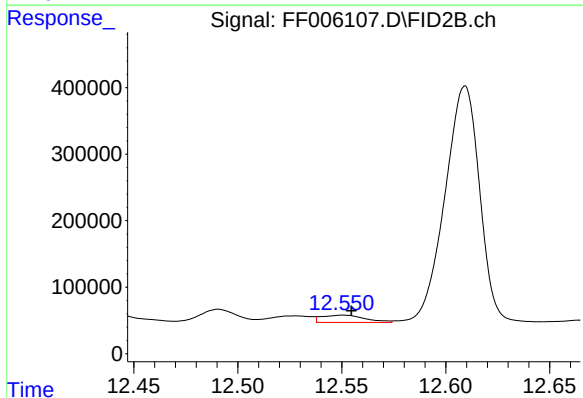


#7 N-EICOSANE

R.T.: 12.551 min
Delta R.T.: -0.004 min
Response: 157711
Conc: 0.91 ug/ml

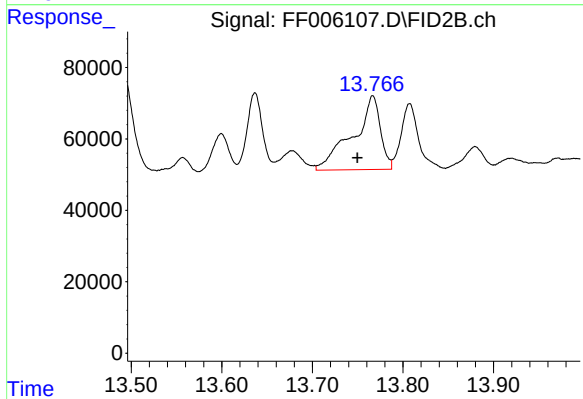

#8 N-DOCOSANE


R.T.: 13.767 min
Delta R.T.: 0.017 min
Response: 434820
Conc: 2.55 ug/ml

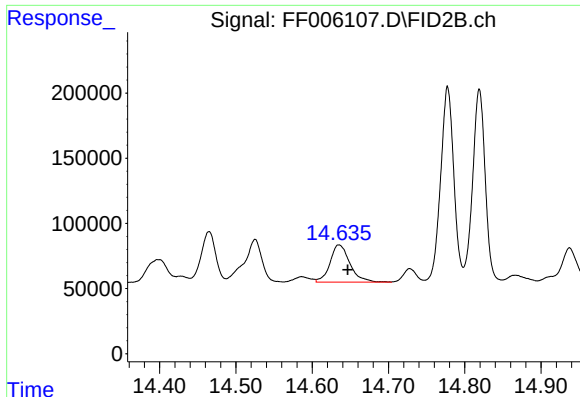

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.635 min
Delta R.T.: -0.011 min
Response: 518724
Conc: 3.57 ug/ml

Instrument :
FID_F
ClientSampleId :

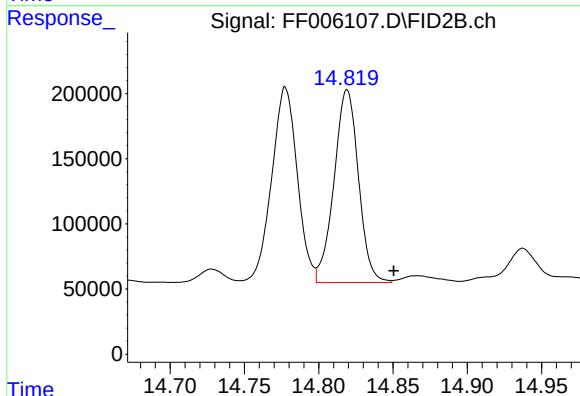


#10 N-TETRACOSANE

R.T.: 14.819 min
Delta R.T.: -0.031 min
Response: 1693935
Conc: 10.15 ug/ml

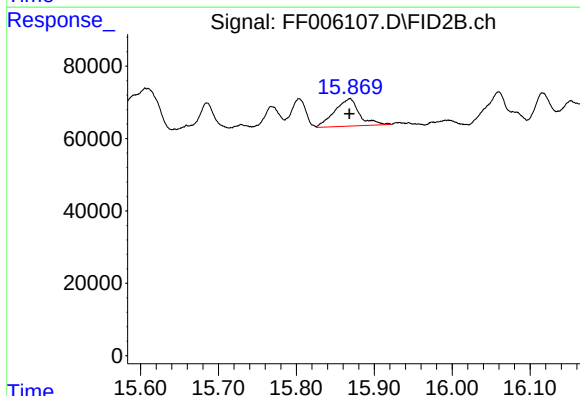


#11 N-HEXACOSANE

R.T.: 15.869 min
Delta R.T.: 0.000 min
Response: 167844
Conc: 1.04 ug/ml

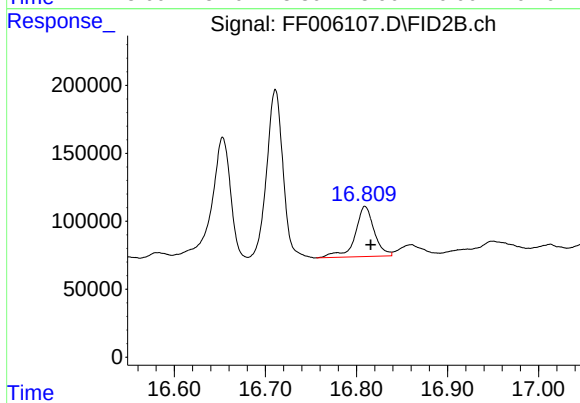

#12 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: -0.006 min
Response: 538271
Conc: 3.51 ug/ml

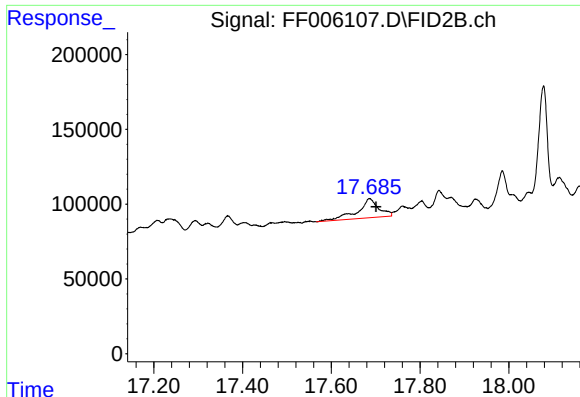

#13 N-TRIACONTANE


R.T.: 17.686 min
Delta R.T.: -0.014 min
Response: 422679
Conc: 2.91 ug/ml

Instrument :
FID_F
ClientSampleId :

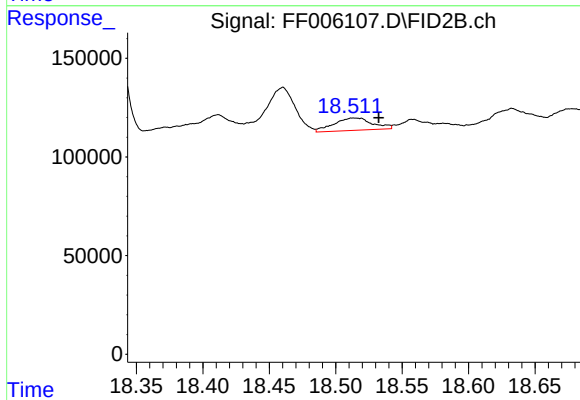


#14 N-DOTRIACONTANE

R.T.: 18.514 min
Delta R.T.: -0.019 min
Response: 128065
Conc: 0.92 ug/ml

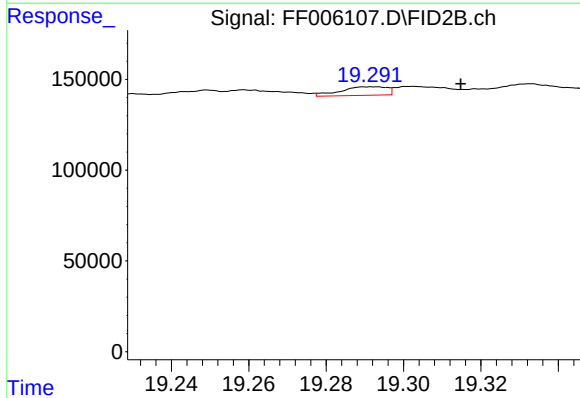

#15 N-TETRATRIACONTANE

R.T.: 19.292 min
Delta R.T.: -0.023 min
Response: 39063
Conc: 0.30 ug/ml

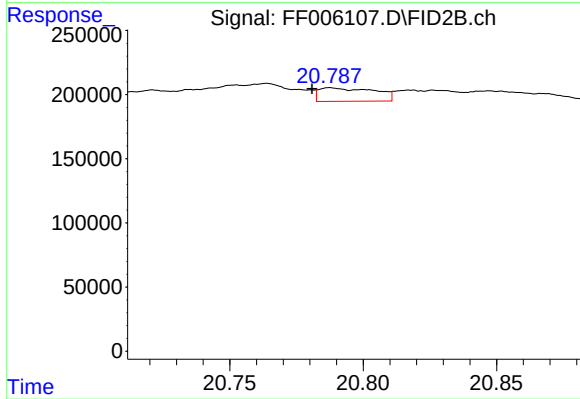

#17 N-OCTATRIACONTANE

R.T.: 20.788 min
Delta R.T.: 0.007 min
Response: 153708
Conc: 1.31 ug/ml