

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122818\
 Data File : FF003106.D
 Signal(s) : FID2B.ch
 Acq On : 28 Dec 2018 11:07
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 28 21:02:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds				
3) N-DODECANE	6.375	6035374	38.007	ug/ml
10) N-TETRACOSANE	14.809	160265	1.109	ug/ml
11) N-HEXACOSANE	15.857	95143	0.682	ug/ml
12) N-OCTACOSANE	16.813	5305287	39.596	ug/ml
13) N-TRIACONTANE	17.700	733512	5.725	ug/ml
14) N-DOTRIACONTANE	18.538	1059037	8.868	ug/ml
15) N-TETRATRIACONTANE	19.326	617271	5.446	ug/ml
16) N-HEXATRIACONTANE	20.071	320796	2.973	ug/ml
17) N-OCTATRIACONTANE	20.809	263879	2.600	ug/ml
18) N-TETRACONTANE	21.707	386260	3.675	ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122818\
Data File : FF003106.D
Signal(s) : FID2B.ch
Acq On : 28 Dec 2018 11:07
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 28 21:02:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

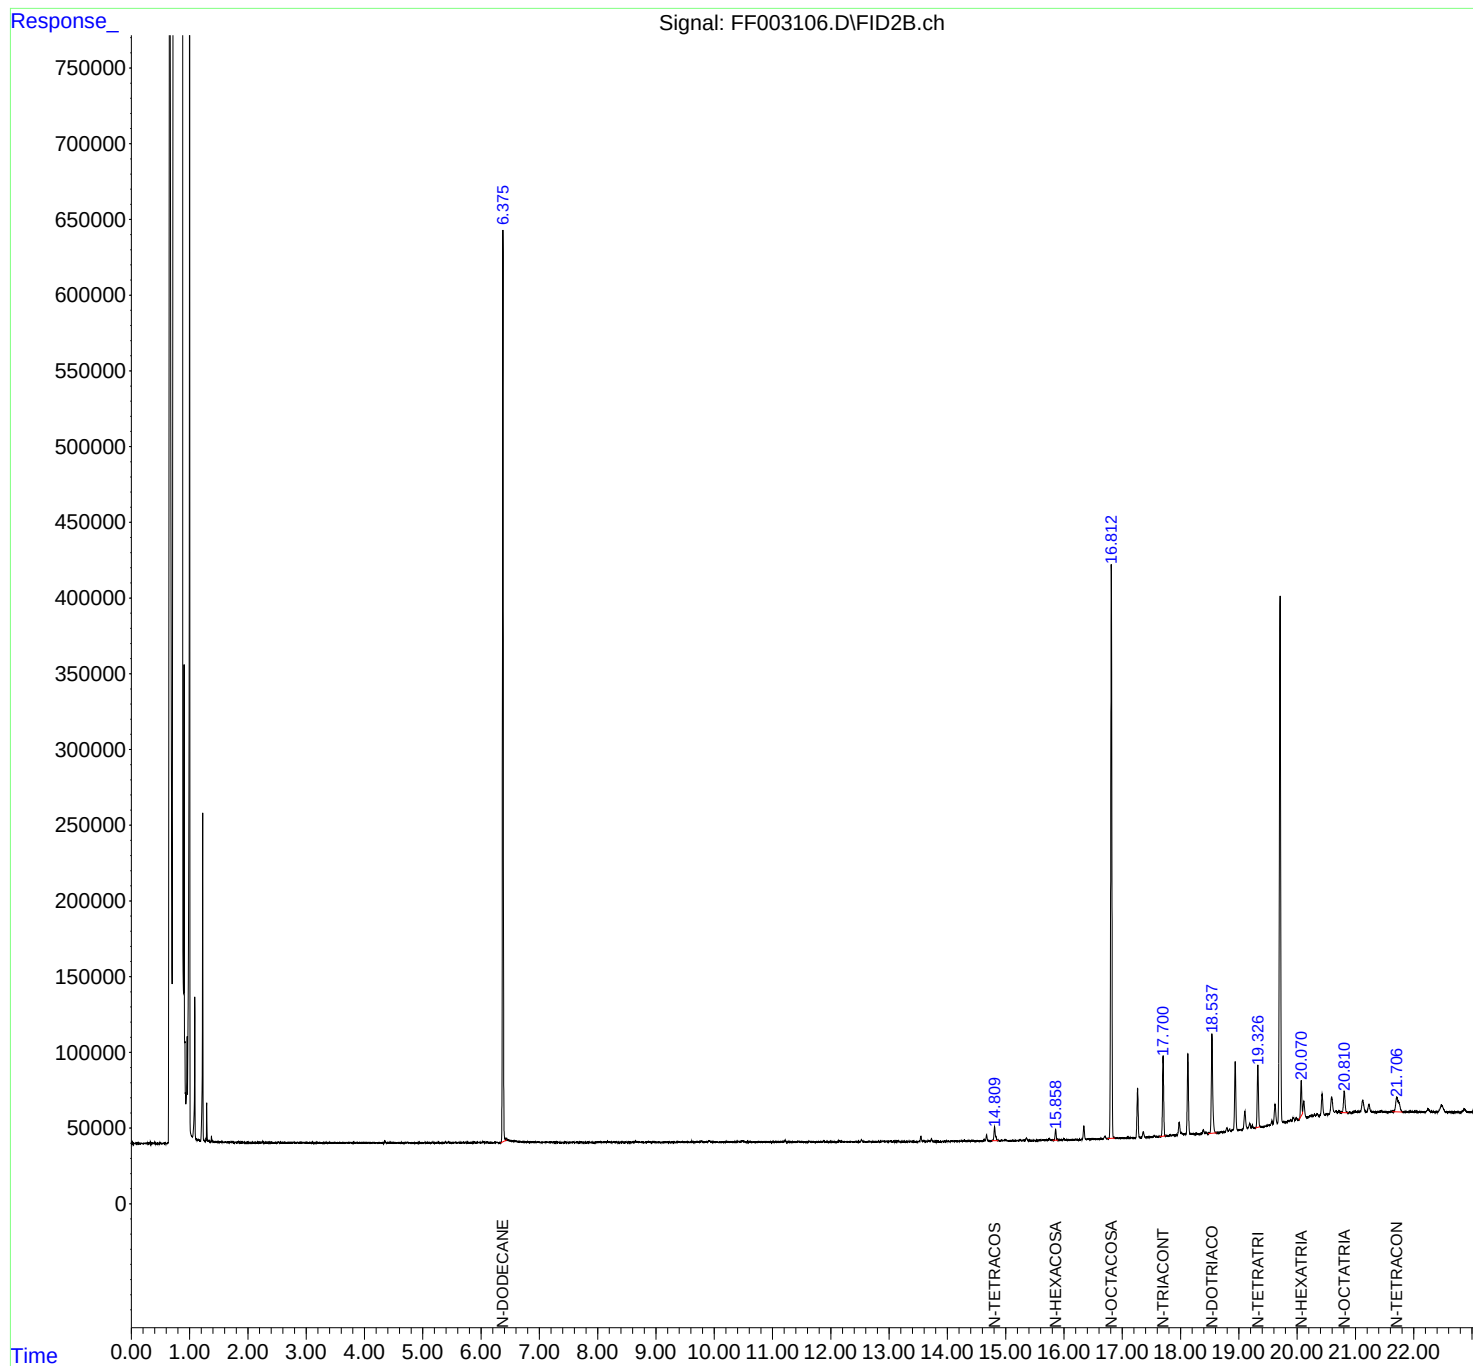

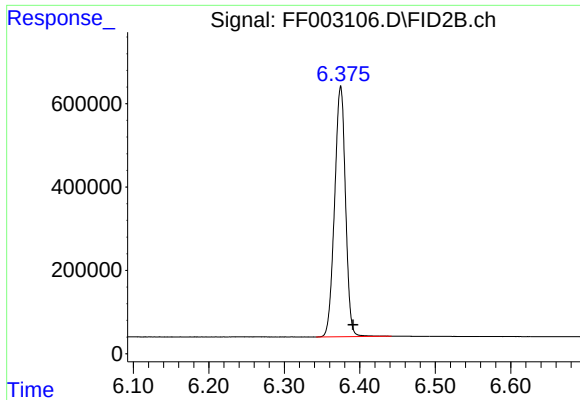


#3 N-DODECANE

R.T.: 6.375 min
Delta R.T.: -0.016 min
Response: 6035374
Conc: 38.01 ug/ml

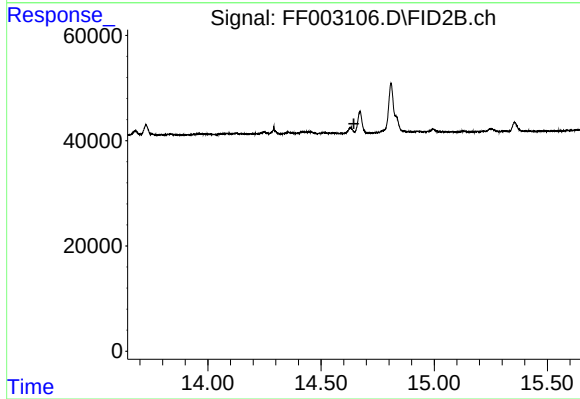


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.645 min
Response: 0
Conc: N.D.

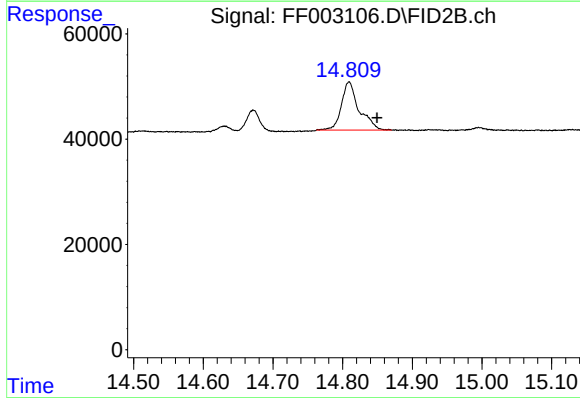


#10 N-TETRACOSANE

R.T.: 14.809 min
Delta R.T.: -0.040 min
Response: 160265
Conc: 1.11 ug/ml

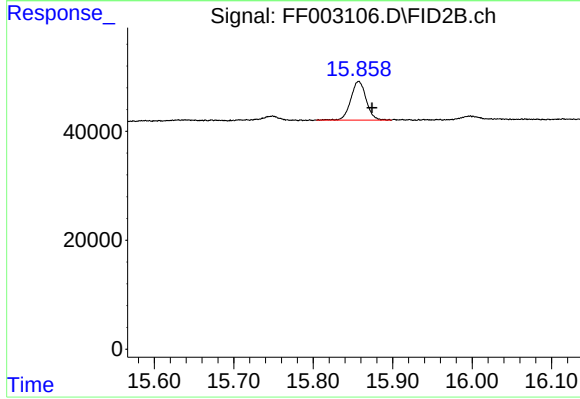


#11 N-HEXACOSANE

R.T.: 15.857 min
Delta R.T.: -0.017 min
Response: 95143
Conc: 0.68 ug/ml

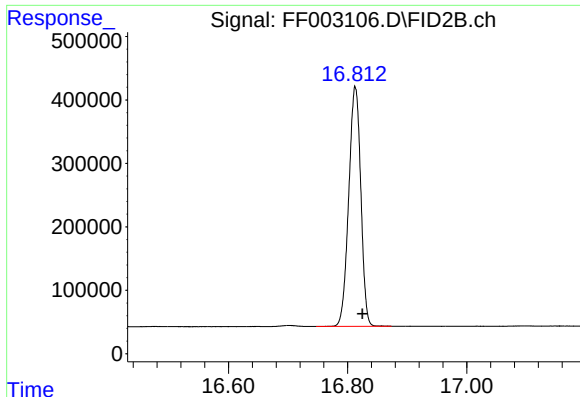


#12 N-OCTACOSANE

R.T.: 16.813 min
Delta R.T.: -0.012 min
Response: 5305287
Conc: 39.60 ug/ml

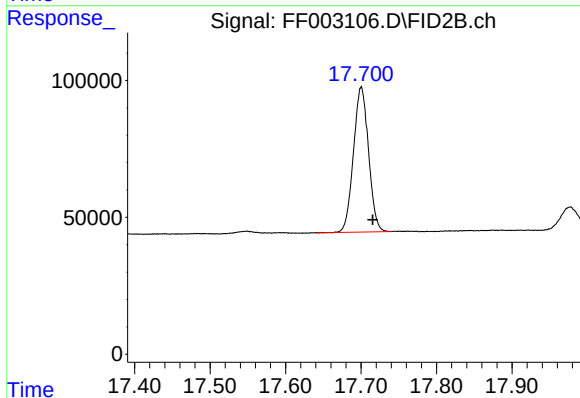


#13 N-TRIACONTANE

R.T.: 17.700 min
Delta R.T.: -0.015 min
Response: 733512
Conc: 5.72 ug/ml

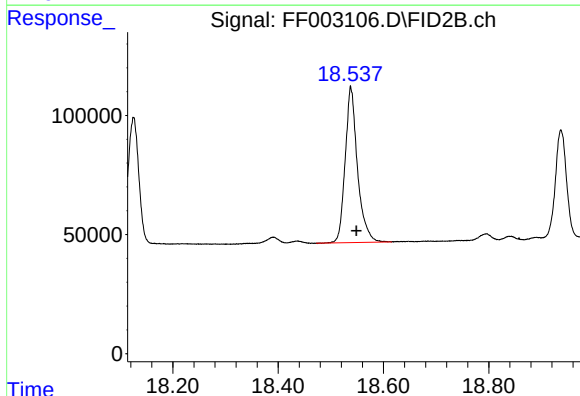


#14 N-DOTRIACONTANE

R.T.: 18.538 min
Delta R.T.: -0.010 min
Response: 1059037
Conc: 8.87 ug/ml

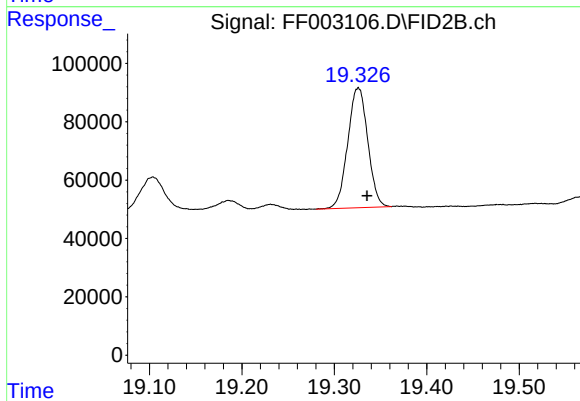


#15 N-TETRATRIACONTANE

R.T.: 19.326 min
Delta R.T.: -0.010 min
Response: 617271
Conc: 5.45 ug/ml

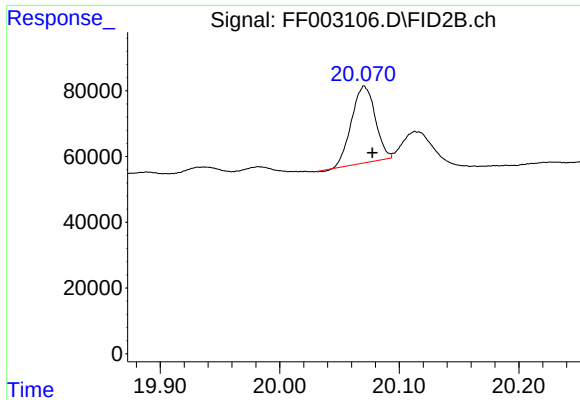


#16 N-HEXATRIACONTANE

R.T.: 20.071 min
Delta R.T.: -0.007 min
Response: 320796
Conc: 2.97 ug/ml

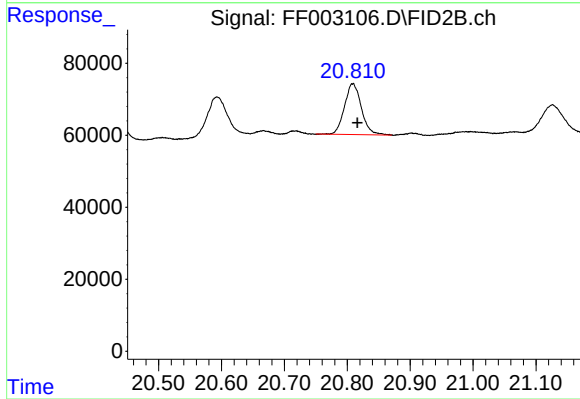

#17 N-OCTATRIACONTANE

R.T.: 20.809 min
Delta R.T.: -0.008 min
Response: 263879
Conc: 2.60 ug/ml

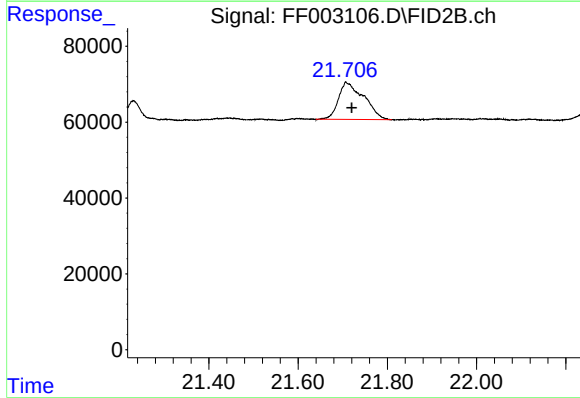

#18 N-TETRACONTANE

R.T.: 21.707 min
Delta R.T.: -0.013 min
Response: 386260
Conc: 3.67 ug/ml