

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122818\
 Data File : FF003107.D
 Signal(s) : FID2B.ch
 Acq On : 28 Dec 2018 14:59
 Operator : AJ\SJ
 Sample : PB116056BS
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 28 21:03:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.630	1895615	14.601 ug/ml
Target Compounds			
2) N-DECANE	4.356	2494719	15.924 ug/ml
3) N-DODECANE	6.378	2553973	16.083 ug/ml
4) N-TETRADECANE	8.171	2528877	15.777 ug/ml
5) N-HEXADECANE	9.772	2499472	15.607 ug/ml
6) N-OCTADECANE	11.215	2469731	15.590 ug/ml
7) N-EICOSANE	12.527	2413540	15.649 ug/ml
8) N-DOCOSANE	13.728	2361384	15.792 ug/ml
10) N-TETRACOSANE	14.834	2379107	16.463 ug/ml
11) N-HEXACOSANE	15.858	2278546	16.325 ug/ml
12) N-OCTACOSANE	16.812	2266136	16.913 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122818\
Data File : FF003107.D
Signal(s) : FID2B.ch
Acq On : 28 Dec 2018 14:59
Operator : AJ\SJ
Sample : PB116056BS
Misc :
ALS Vial : 55 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 28 21:03:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

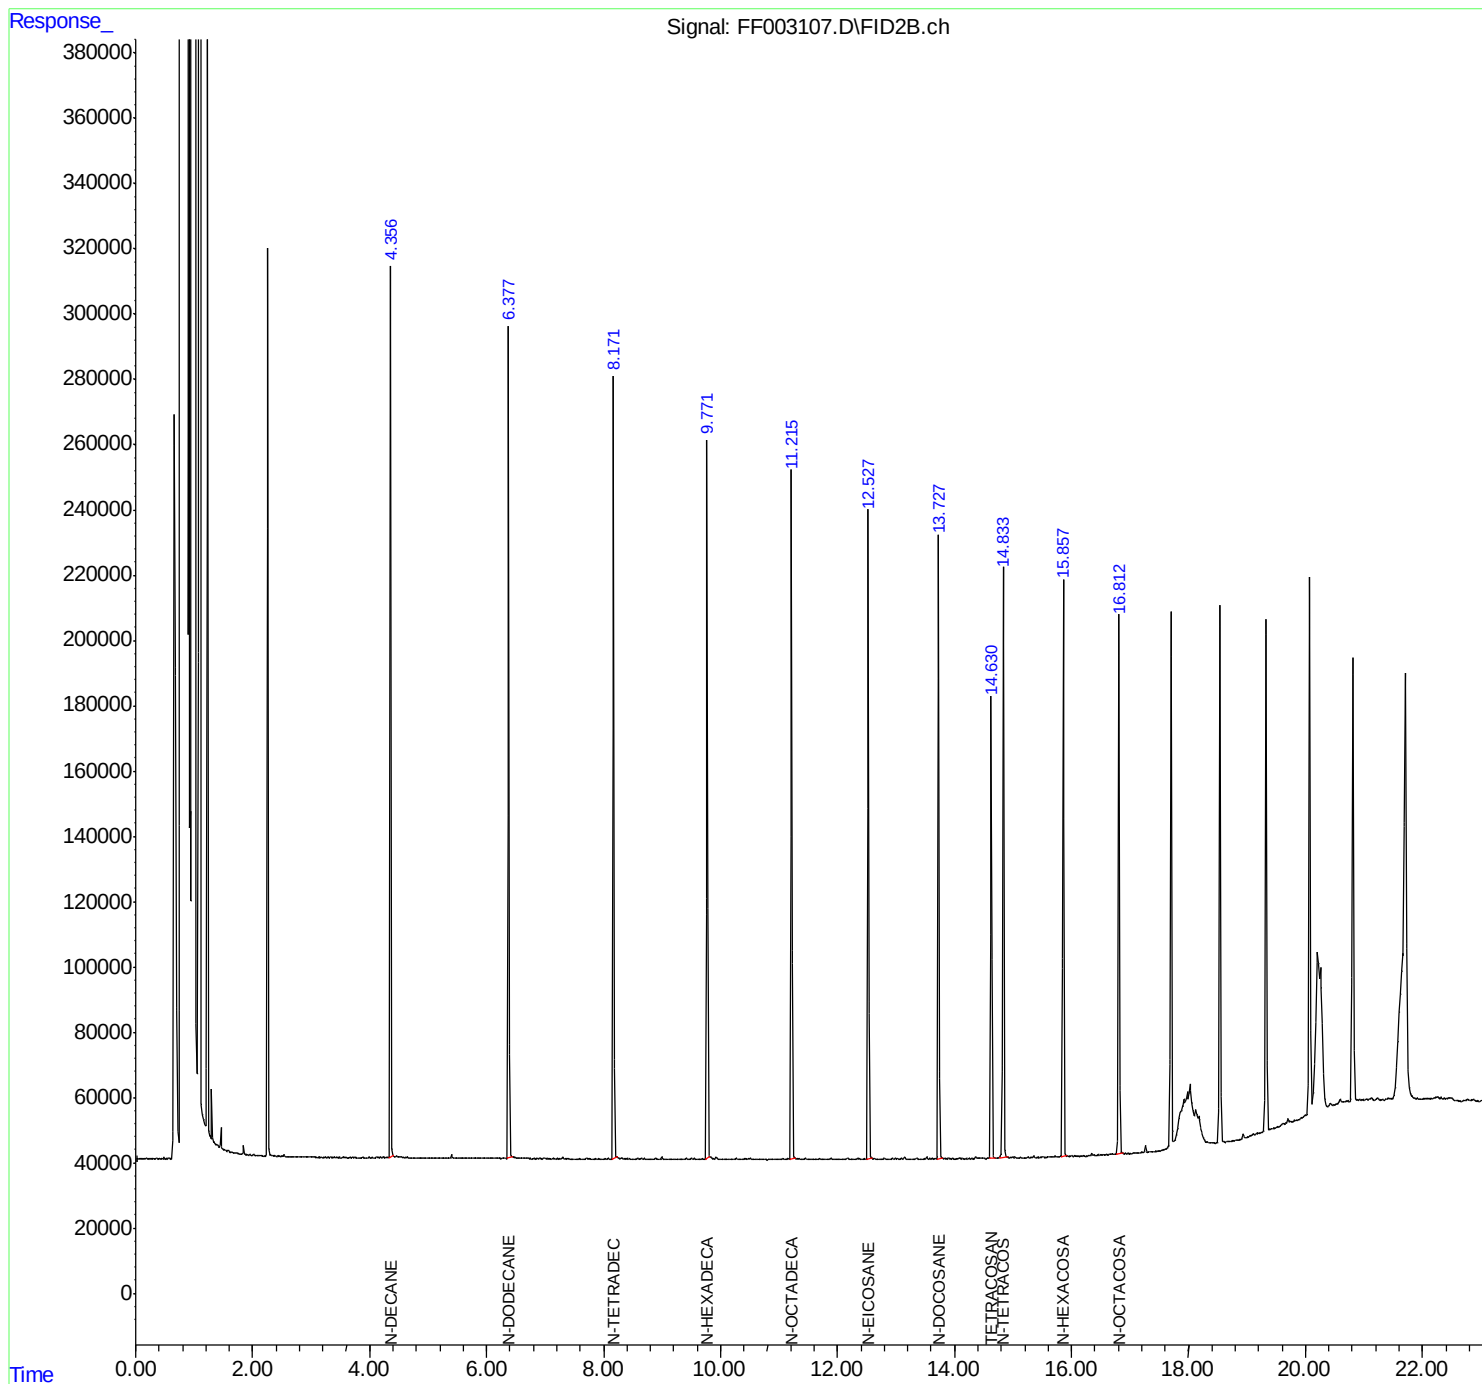

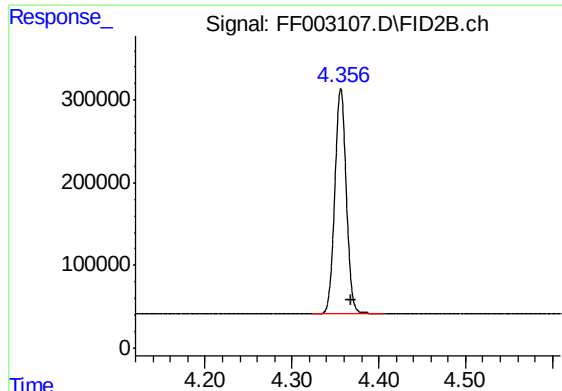


#2 N-DECANE

R.T.: 4.356 min
Delta R.T.: -0.011 min
Response: 2494719
Conc: 15.92 ug/ml

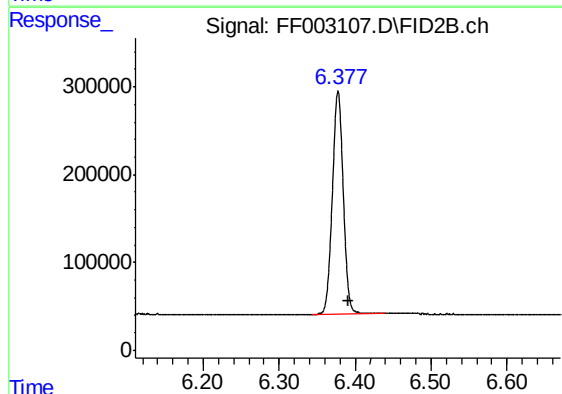


#3 N-DODECANE

R.T.: 6.378 min
Delta R.T.: -0.013 min
Response: 2553973
Conc: 16.08 ug/ml

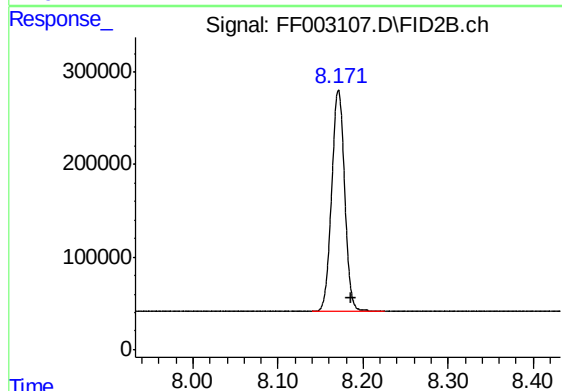


#4 N-TETRADECANE

R.T.: 8.171 min
Delta R.T.: -0.015 min
Response: 2528877
Conc: 15.78 ug/ml

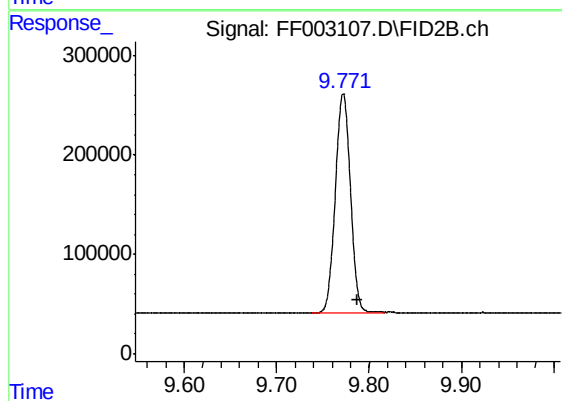


#5 N-HEXADECANE

R.T.: 9.772 min
Delta R.T.: -0.015 min
Response: 2499472
Conc: 15.61 ug/ml

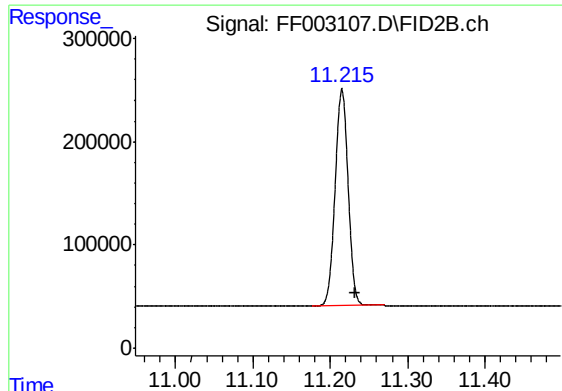


#6 N-OCTADECANE

R.T.: 11.215 min
Delta R.T.: -0.016 min
Response: 2469731
Conc: 15.59 ug/ml

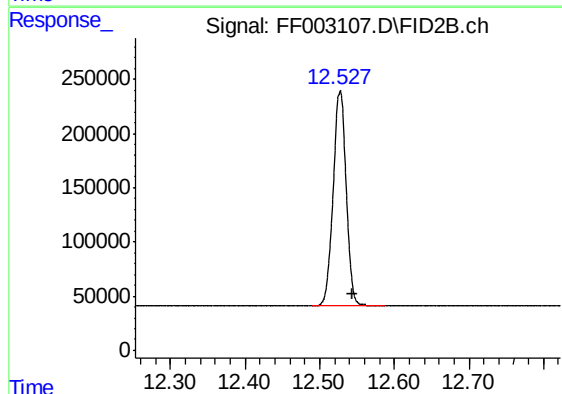


#7 N-EICOSANE

R.T.: 12.527 min
Delta R.T.: -0.016 min
Response: 2413540
Conc: 15.65 ug/ml

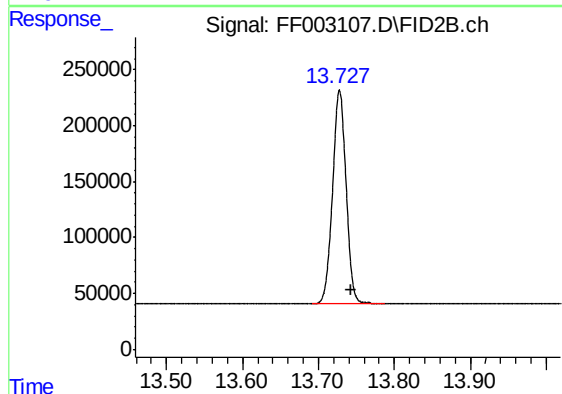


#8 N-DOCOSANE

R.T.: 13.728 min
Delta R.T.: -0.016 min
Response: 2361384
Conc: 15.79 ug/ml

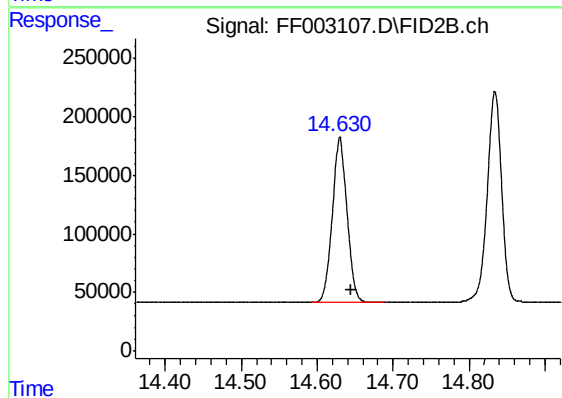


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.630 min
Delta R.T.: -0.015 min
Response: 1895615
Conc: 14.60 ug/ml

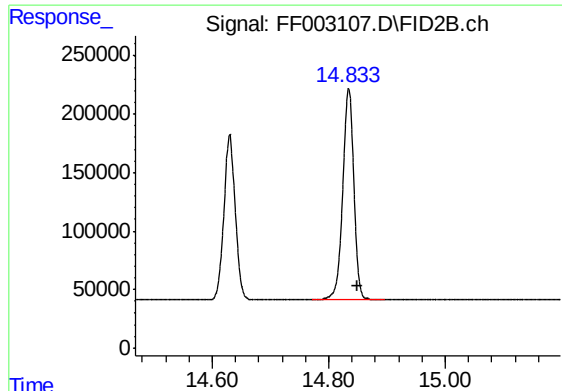


#10 N-TETRACOSANE

R.T.: 14.834 min
Delta R.T.: -0.015 min
Response: 2379107
Conc: 16.46 ug/ml

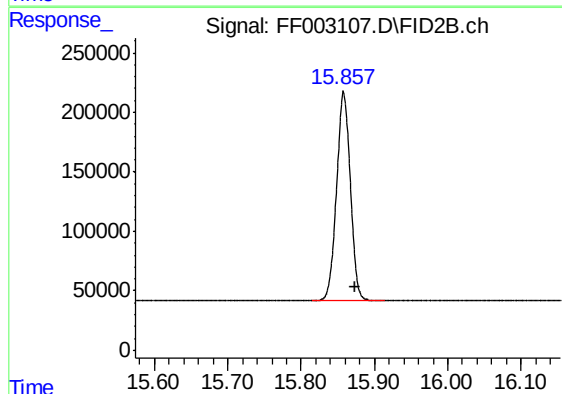

#11 N-HEXACOSANE

R.T.: 15.858 min
Delta R.T.: -0.016 min
Response: 2278546
Conc: 16.32 ug/ml

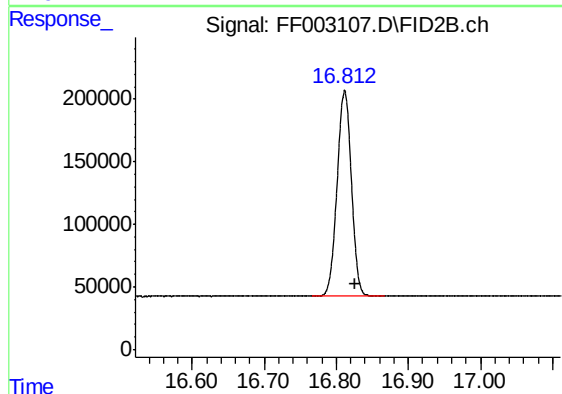

#12 N-OCTACOSANE

R.T.: 16.812 min
Delta R.T.: -0.013 min
Response: 2266136
Conc: 16.91 ug/ml